

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050916\
 Data File : BM005363.D
 Acq On : 09 May 2016 16:50
 Operator : UM/SJ
 Sample : H2888-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW4

Manual Integrations
 APPROVED

sohil
 5/10/2016 6:45:47 PM

Quant Time: May 10 05:13:09 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 04:23:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	96038	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	446445	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.41	164	273621	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.16	188	619612	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	641757	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	508195	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	5516	2.70	ng/uL	0.00
5) Phenol-d5	6.94	99	117460	13.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	71623	14.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	96583	14.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	99807	13.86	ng/ul	0.00
19) Nitrobenzene-d5	8.93	128	47537	14.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	54848	15.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	95966	14.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	138253	17.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	335260	15.29	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	402837	15.66	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	38288m	9.56	ng/ul	0.00
57) Fluorene-d10	15.40	176	293960	15.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	33572	9.63	ng/ul	0.00
70) Anthracene-d10	17.26	188	461189	16.84	ng/ul	0.00
76) Pyrene-d10	19.56	212	523760	17.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	383313	17.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.86	163	57023	2.60	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM050916\
Data File : BM005363.D
Acq On : 09 May 2016 16:50
Operator : UM/SJ
Sample : H2888-07
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9WW4

Manual Integrations
APPROVED

sohil
5/10/2016 6:45:47 PM

Quant Time: May 10 05:13:09 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 04:23:52 2016
Response via : Initial Calibration

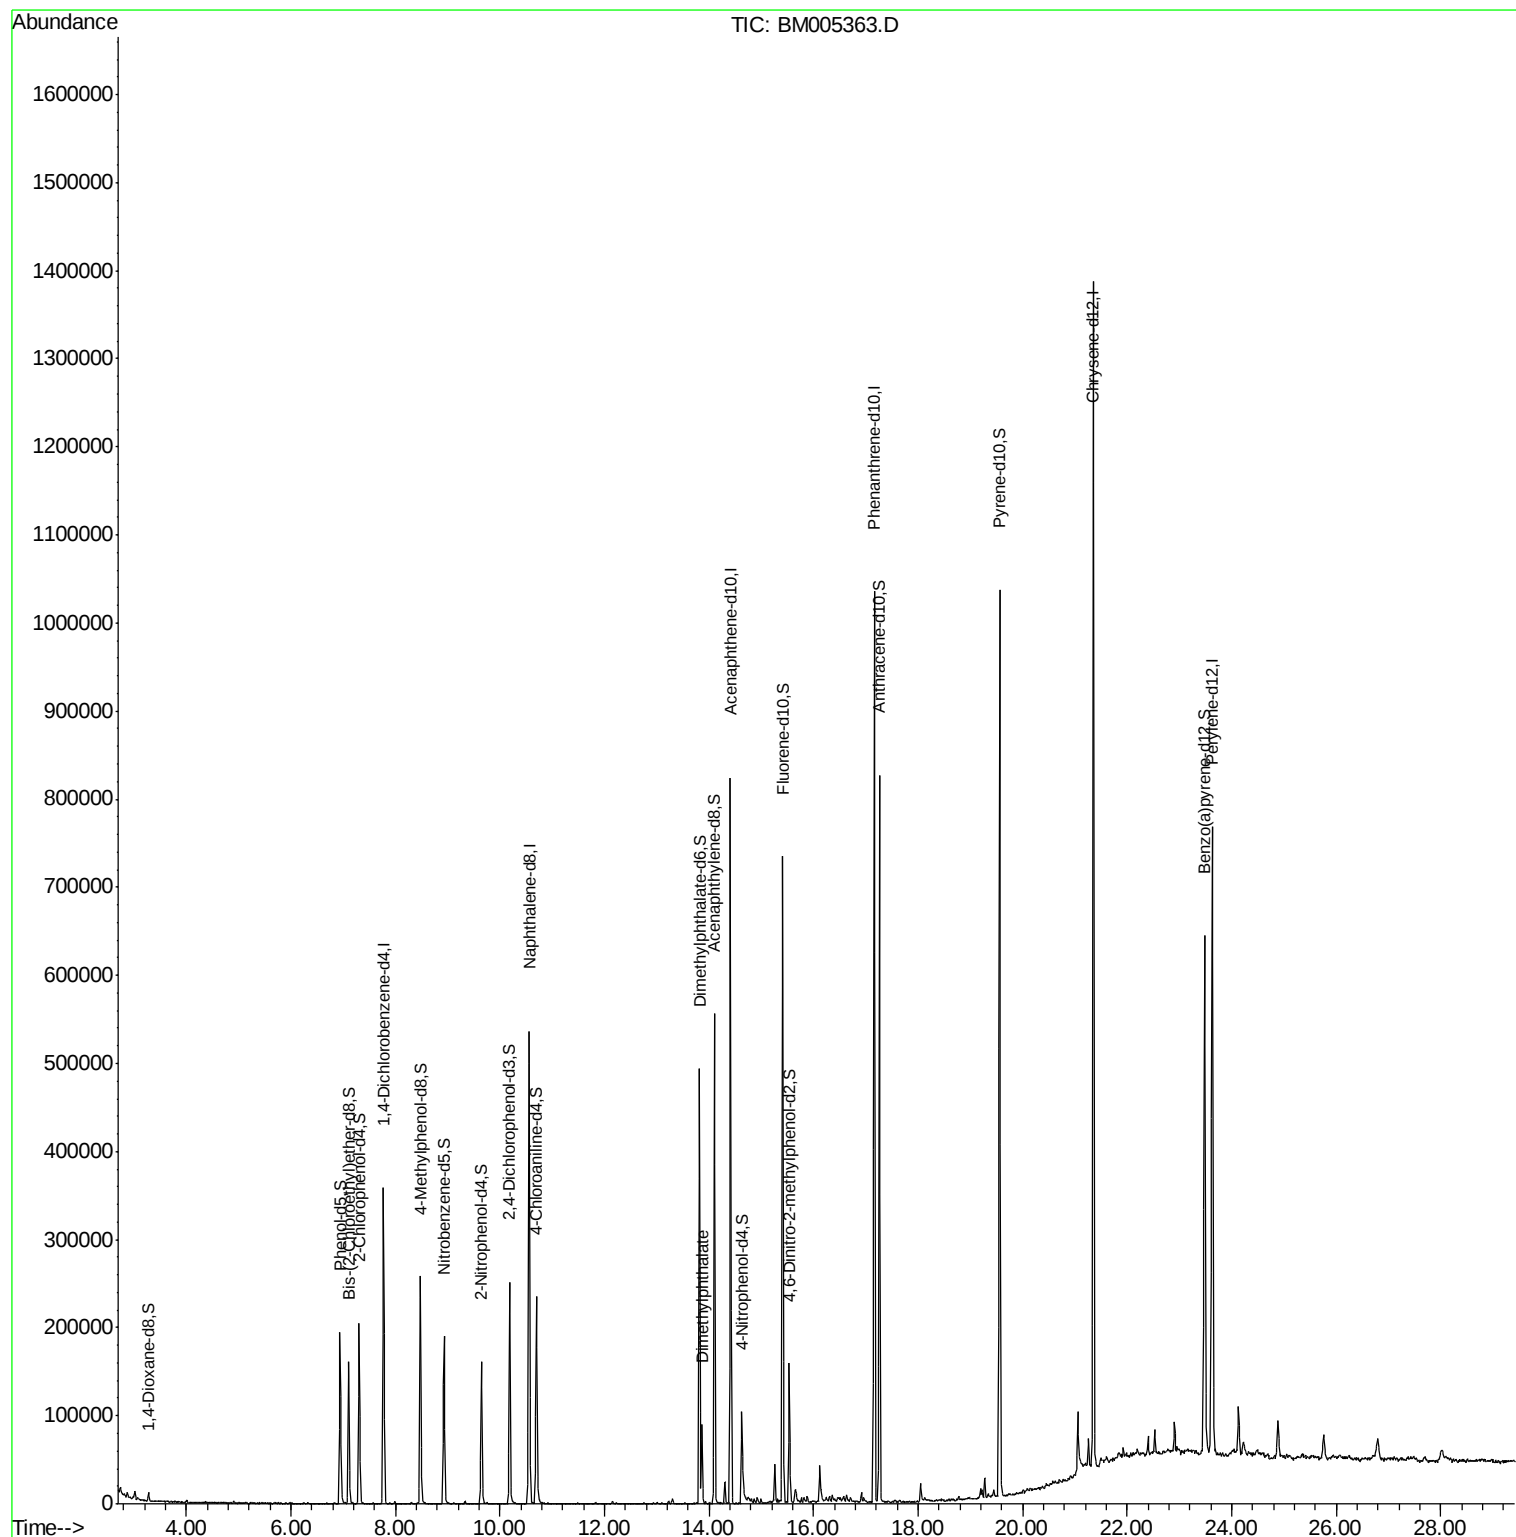

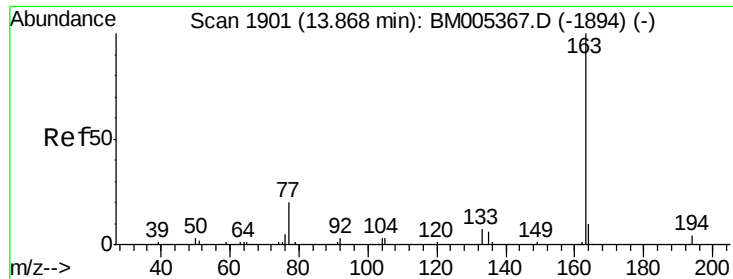

#44
 Dimethylphthalate
 Concen: 2.60 ng/ul
 RT: 13.86 min Scan# 1900
 Delta R.T. -0.01 min
 Lab File: BM005363.D
 Acq: 09 May 2016 16:50

Instrument :
 BNA_M
 ClientSampleId :
 D9WW4

Tot Ion	Ratio	Resp	Lower	Upper
163	100	57023		
194	4.1		3.4	5.0
164	10.3		7.9	11.9

Manual Integrations
 APPROVED

sohil
 5/10/2016 6:45:47 PM

