

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
 Data File : BM050162.D
 Acq On : 09 May 2025 16:46
 Operator : RC/JU
 Sample : Q1983-31
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OR-636-COMP-06

Quant Time: May 09 17:41:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 08 12:03:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	359803	20.000	ng	-0.03
21) Naphthalene-d8	10.533	136	1338107	20.000	ng	-0.03
39) Acenaphthene-d10	14.392	164	995259	20.000	ng	-0.02
64) Phenanthrene-d10	17.145	188	2096577	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	1711612	20.000	ng	-0.01
86) Perylene-d12	24.385	264	1319301	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.334	112	1244068	60.546	ng	-0.02
7) Phenol-d6	6.934	99	1669234	64.635	ng	-0.02
23) Nitrobenzene-d5	8.904	82	946556	34.857	ng	-0.02
42) 2,4,6-Tribromophenol	15.892	330	1034520	70.298	ng	-0.01
45) 2-Fluorobiphenyl	13.004	172	2698930	32.080	ng	-0.03
79) Terphenyl-d14	19.768	244	5653427	48.876	ng	-0.01


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
Data File : BM050162.D
Acq On : 09 May 2025 16:46
Operator : RC/JU
Sample : Q1983-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06


Quant Time: May 09 17:41:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration

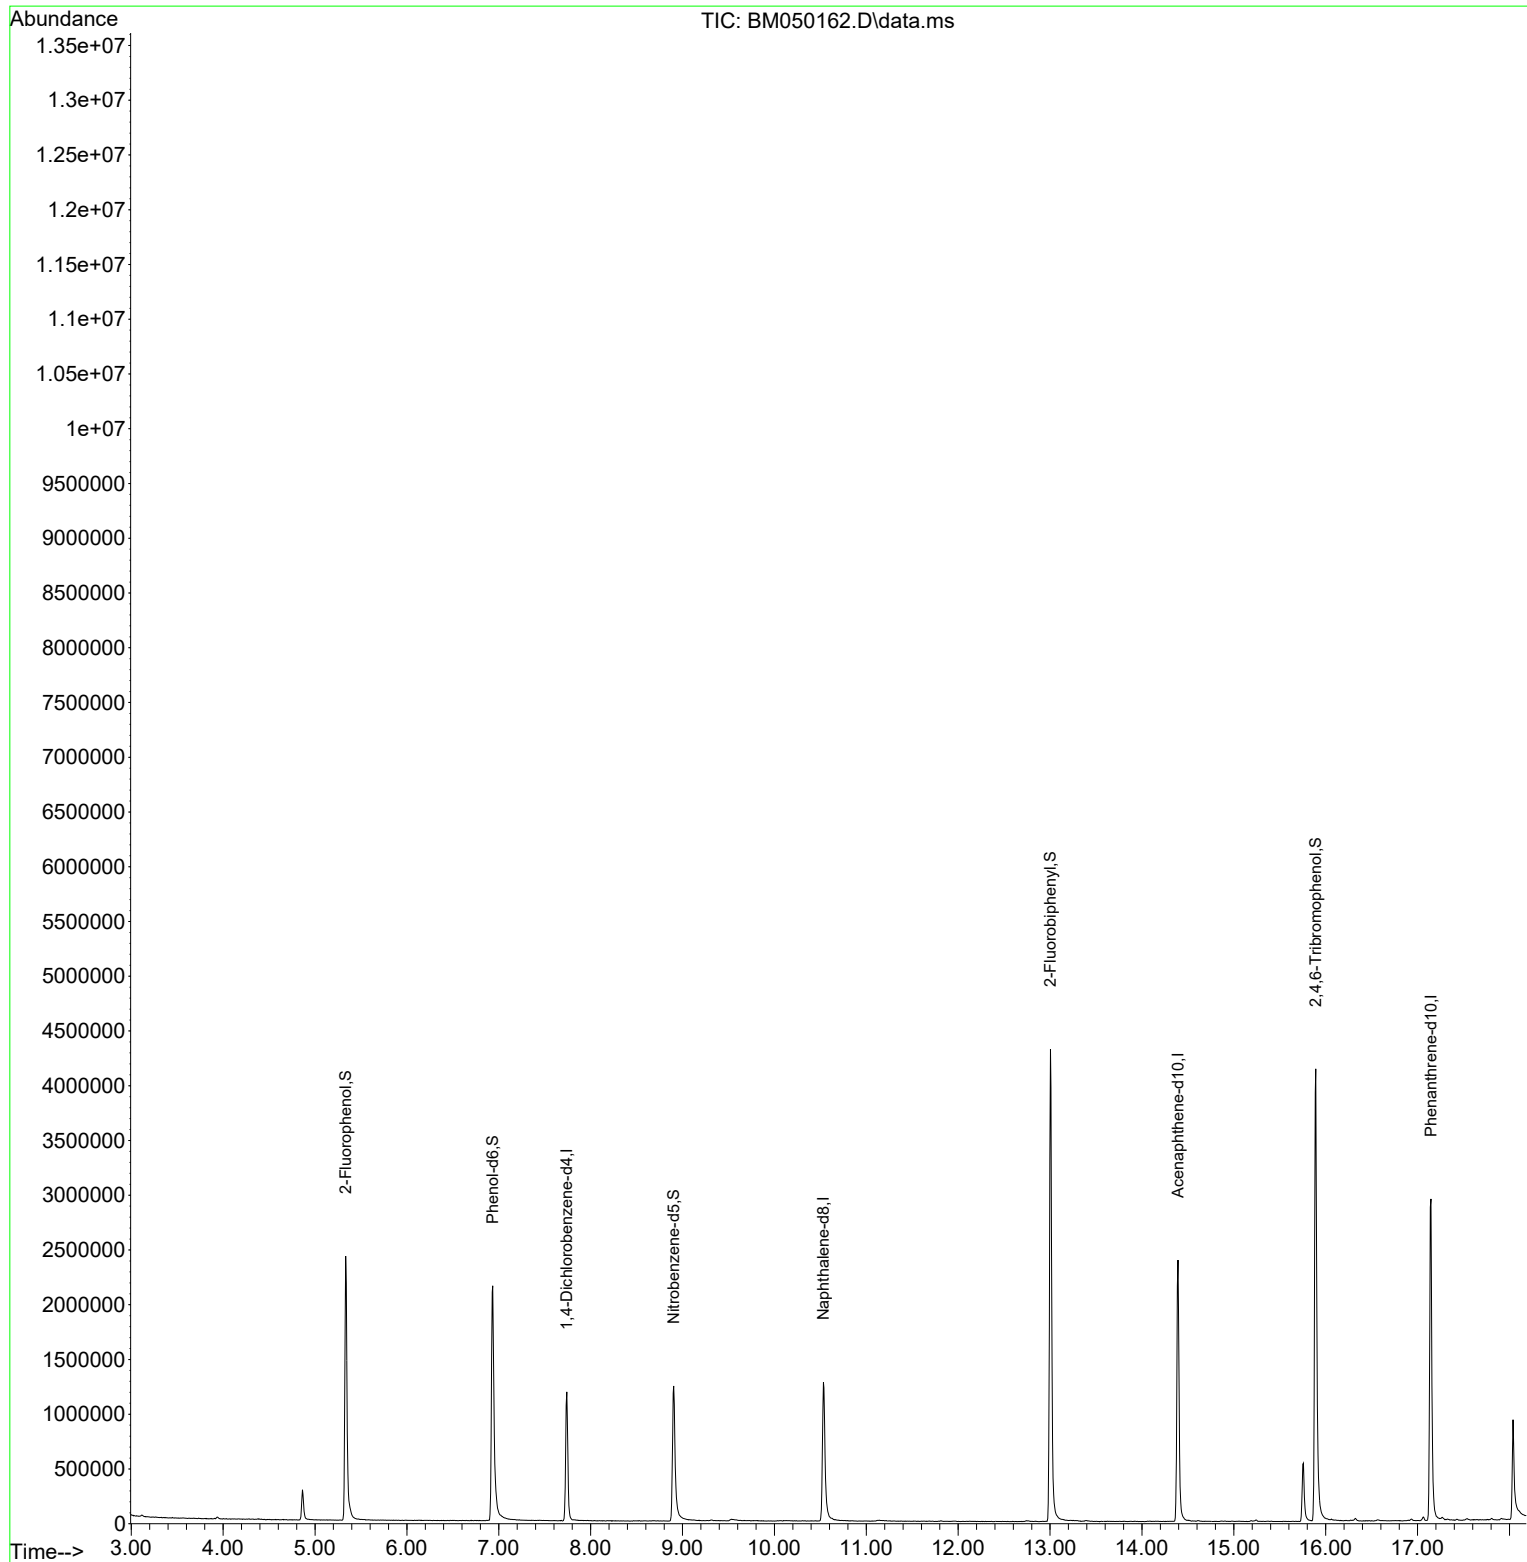

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
Data File : BM050162.D
Acq On : 09 May 2025 16:46
Operator : RC/JU
Sample : Q1983-31
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06

Quant Time: May 09 17:41:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration




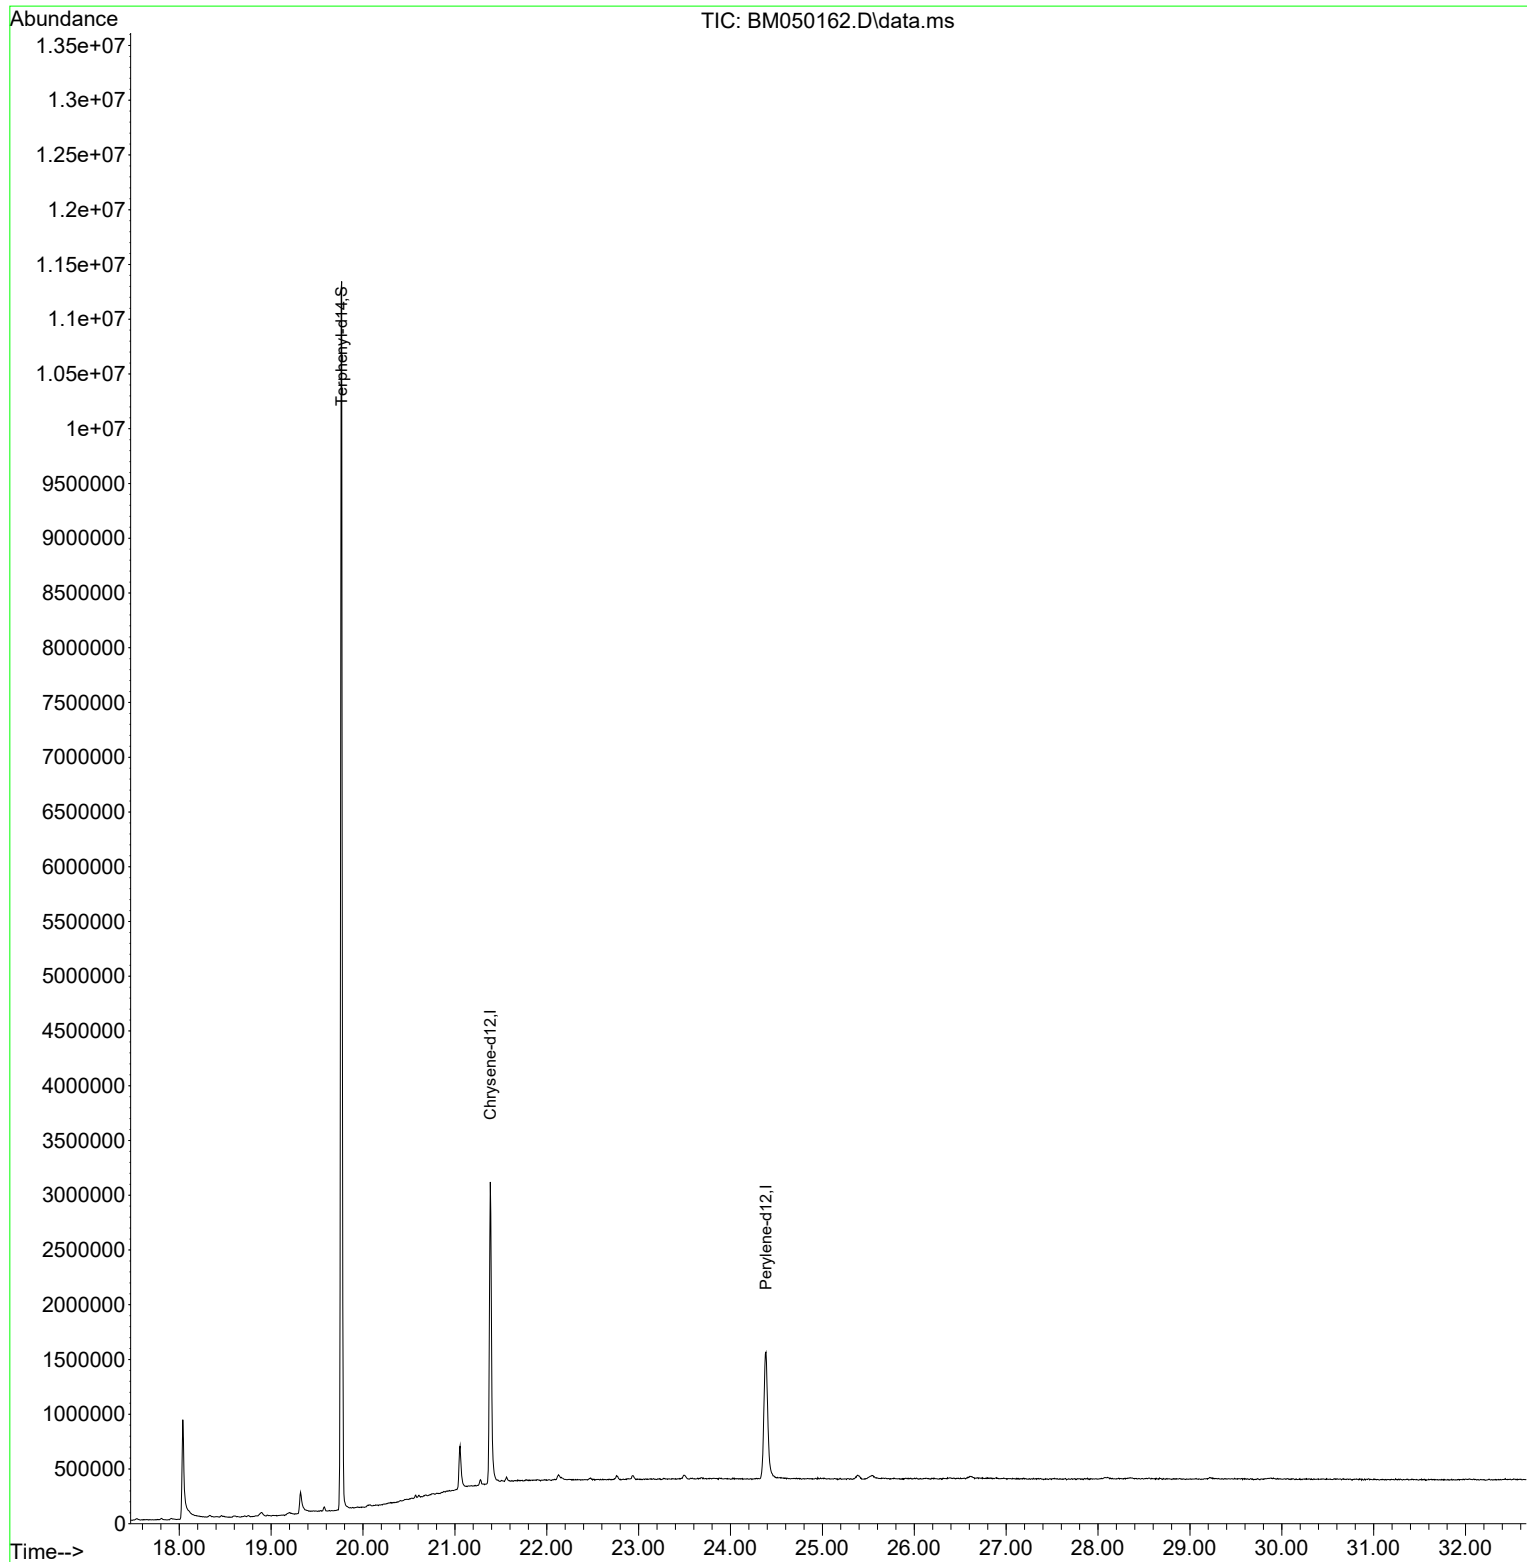




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.739 min Scan# 80
Delta R.T. -0.030 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46




Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06


Tgt Ion:152 Resp: 359803
Ion Ratio Lower Upper
152 100
150 155.4 124.1 186.1
115 52.9 41.2 61.8

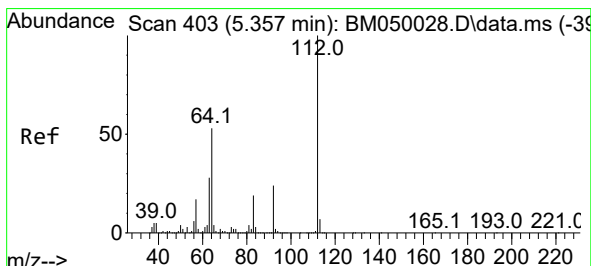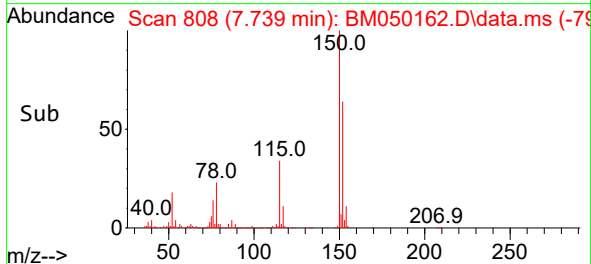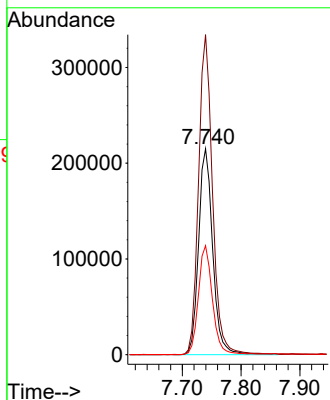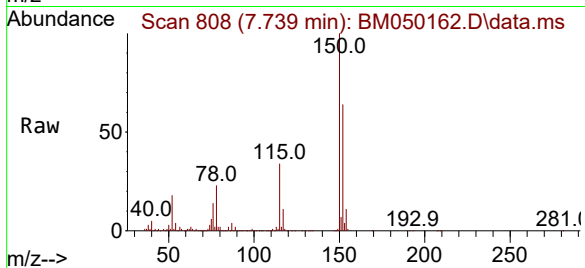

#5
2-Fluorophenol
Concen: 60.546 ng
RT: 5.334 min Scan# 399
Delta R.T. -0.024 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46

Tgt Ion:112 Resp: 1244068
Ion Ratio Lower Upper
112 100
64 53.6 42.6 64.0
63 28.2 22.2 33.4


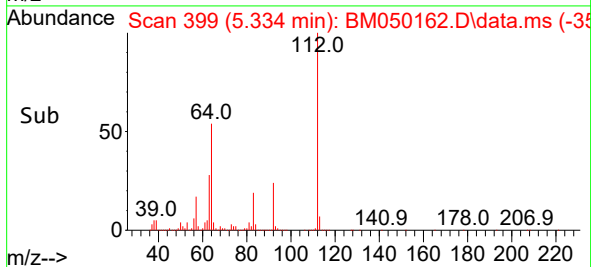
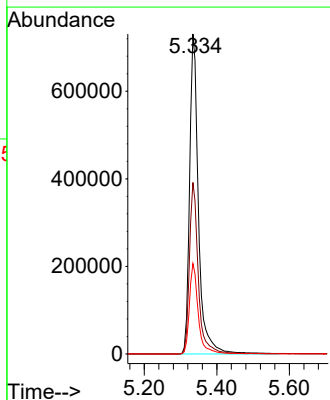
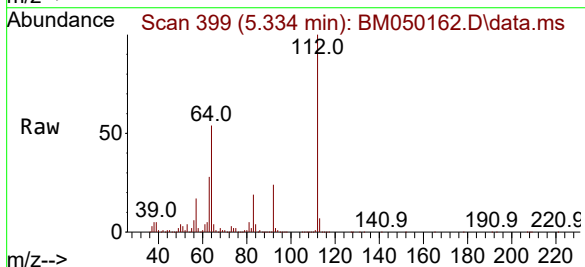


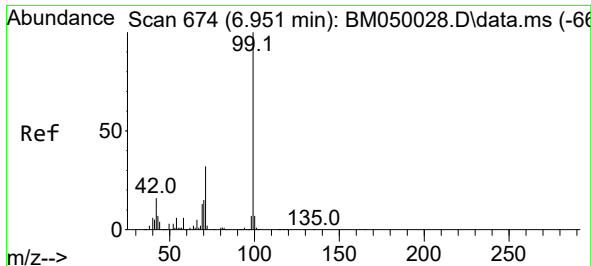

#7
Phenol-d6
Concen: 64.635 ng
RT: 6.934 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46




Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06


Tgt Ion: 99 Resp: 1669234
Ion Ratio Lower Upper
99 100
42 16.2 13.0 19.4
71 32.6 25.6 38.4

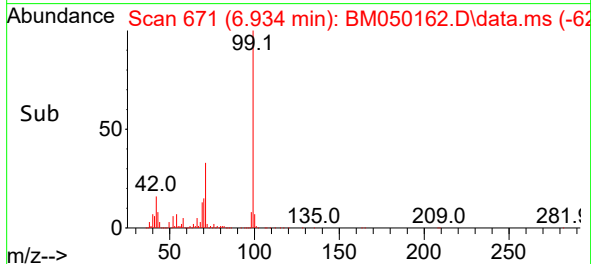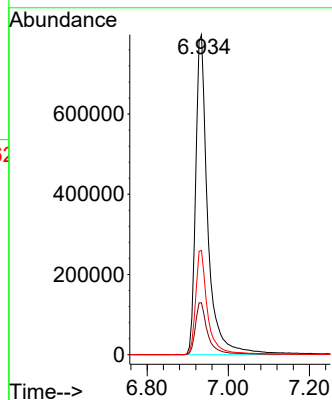

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.533 min Scan# 1283
Delta R.T. -0.029 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46

Tgt Ion: 136 Resp: 1338107
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 7.0 5.1 7.7
68 5.7 4.4 6.6


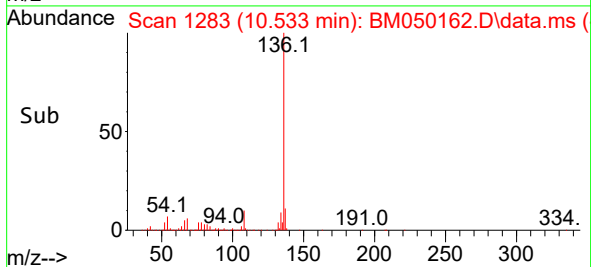
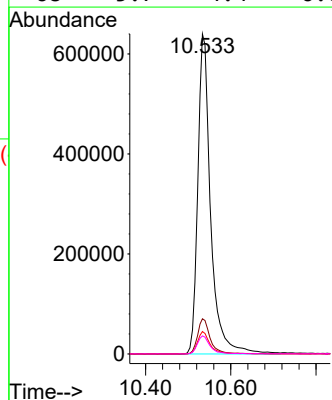
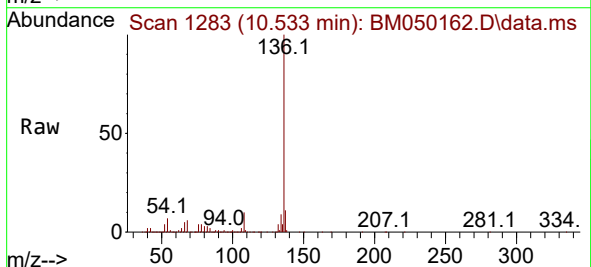


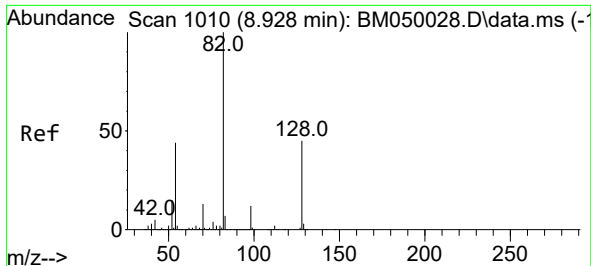

#23
Nitrobenzene-d5
Concen: 34.857 ng
RT: 8.904 min Scan# 1006
Delta R.T. -0.024 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46




Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06


Tgt Ion: 82 Resp: 946556
Ion Ratio Lower Upper
82 100
128 44.0 35.7 53.5
54 44.7 35.4 53.2

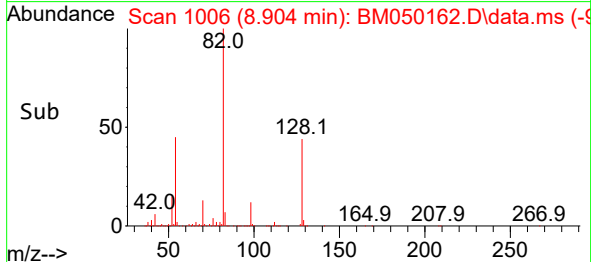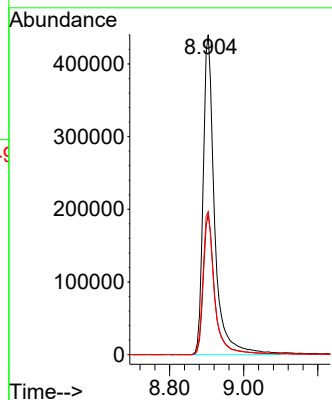

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.392 min Scan# 1939
Delta R.T. -0.018 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46


Tgt Ion: 164 Resp: 995259
Ion Ratio Lower Upper
164 100
162 99.5 79.4 119.0
160 44.9 36.2 54.4

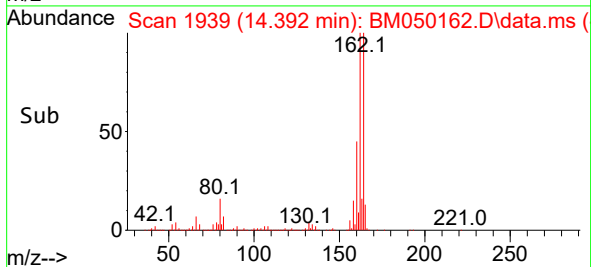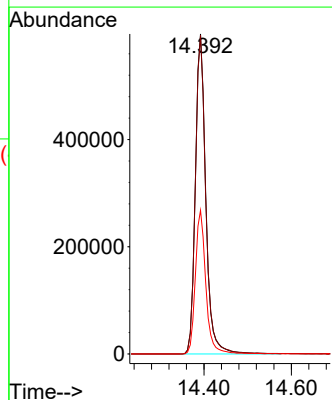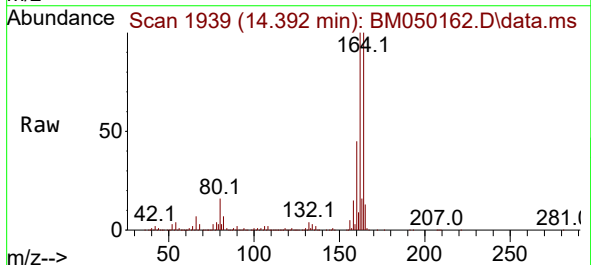



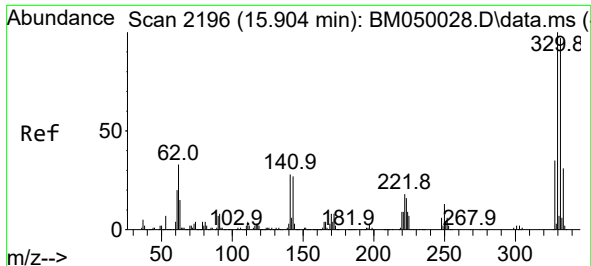


#42
2,4,6-Tribromophenol
Concen: 70.298 ng
RT: 15.892 min Scan# 2196
Delta R.T. -0.012 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46

Instrument :
BNA_M
ClientSampleId :
OR-636-COMP-06



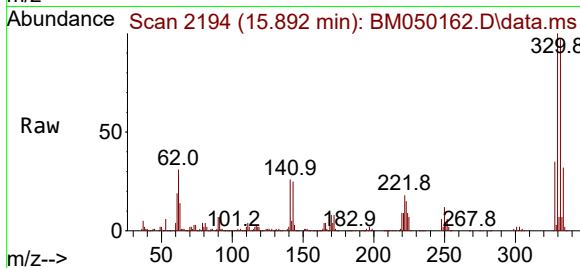



Tgt Ion:330 Resp: 1034520
Ion Ratio Lower Upper
330 100
332 96.9 77.3 115.9
141 28.7 22.5 33.7

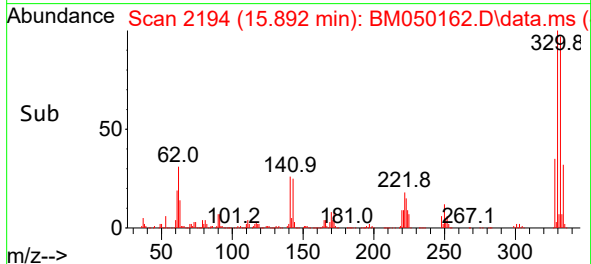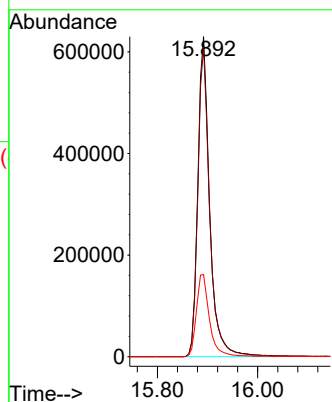

#45
2-Fluorobiphenyl
Concen: 32.080 ng
RT: 13.004 min Scan# 1703
Delta R.T. -0.029 min
Lab File: BM050162.D
Acq: 09 May 2025 16:46

Tgt Ion:172 Resp: 2698930
Ion Ratio Lower Upper
172 100
171 34.8 27.8 41.6
170 23.3 18.6 28.0

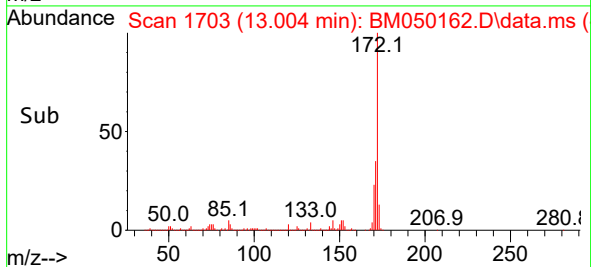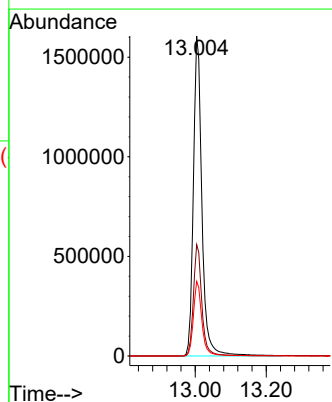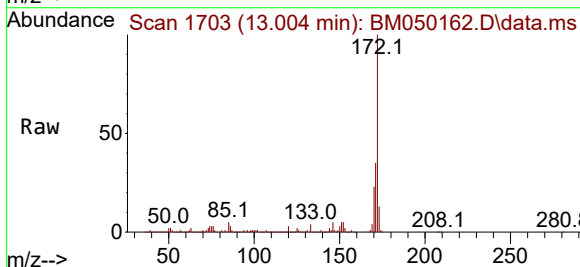



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.145 min Scan# 24

Delta R.T. -0.012 min

Lab File: BM050162.D

Acq: 09 May 2025 16:46

Instrument :

BNA_M

ClientSampleId :

OR-636-COMP-06





Tgt Ion:188 Resp: 2096577

Ion Ratio Lower Upper

188 100

94 7.1 5.7 8.5

80 7.8 6.2 9.4

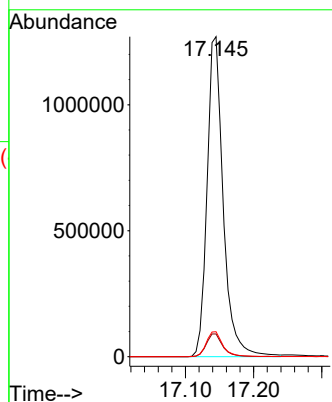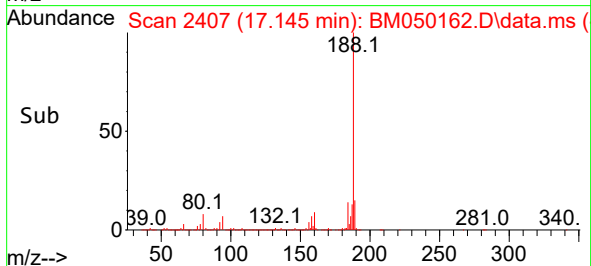

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.386 min Scan# 3128

Delta R.T. -0.011 min

Lab File: BM050162.D

Acq: 09 May 2025 16:46




Tgt Ion:240 Resp: 1711612


Ion Ratio Lower Upper

240 100

120 8.6 6.5 9.7

236 25.9 20.9 31.3

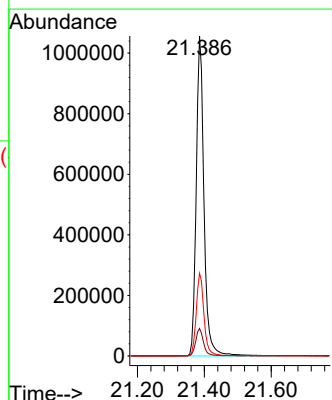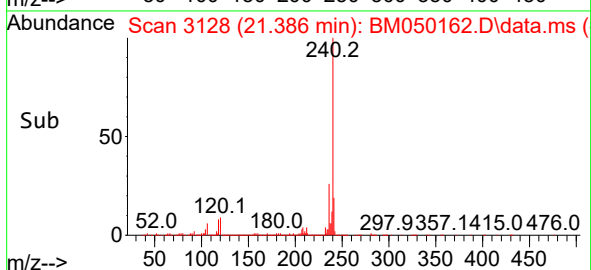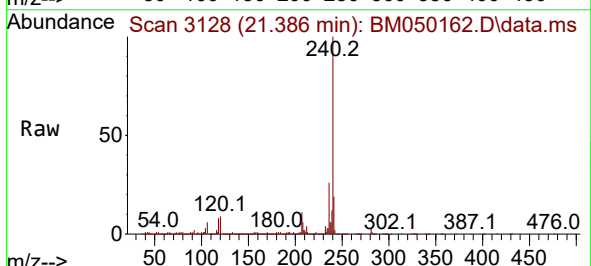



#79

Terphenyl-d14

Concen: 48.876 ng

RT: 19.768 min Scan# 21

Delta R.T. -0.012 min

Lab File: BM050162.D


Acq: 09 May 2025 16:46

Instrument :

BNA_M

ClientSampleId :

OR-636-COMP-06






Tgt Ion:244 Resp: 5653427

Ion Ratio Lower Upper

244 100

212 6.7 5.6 8.4

122 6.3 5.6 8.4

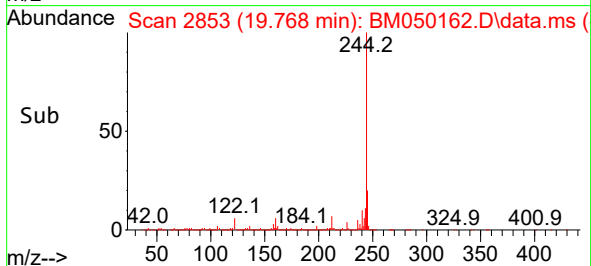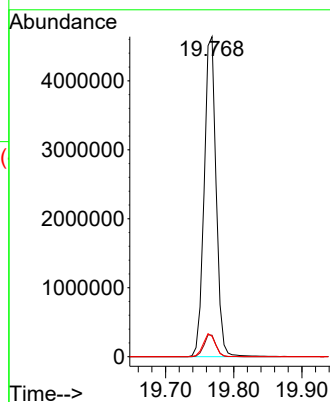

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.385 min Scan# 3638

Delta R.T. -0.018 min

Lab File: BM050162.D

Acq: 09 May 2025 16:46

Tgt Ion:264 Resp: 1319301

Ion Ratio Lower Upper

264 100

260 24.0 18.8 28.2

265 21.8 17.0 25.4

