


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
Data File : BM050156.D
Acq On : 09 May 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 08 12:03:21 2025

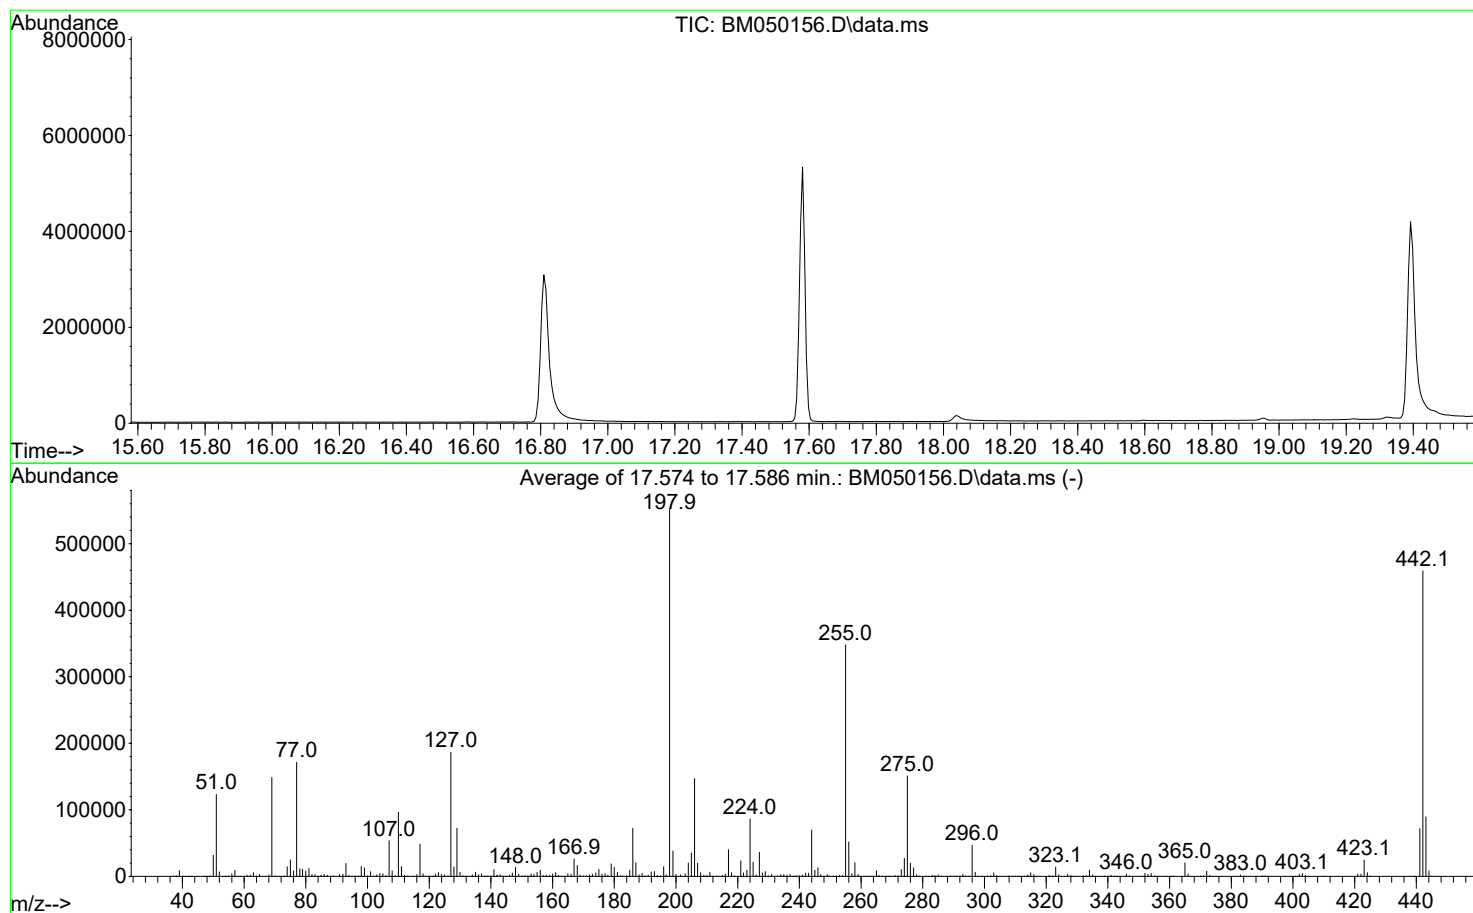

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	22.3	123205	PASS
68	69	0.00	2	1.6	2382	PASS
69	198	0.00	100	26.9	148735	PASS
70	69	0.00	2	0.5	692	PASS
127	198	10	80	33.7	186475	PASS
197	198	0.00	2	0.4	2398	PASS
198	198	100	100	100.0	552853	PASS
199	198	5	9	6.9	38037	PASS
275	198	10	60	27.3	151051	PASS
365	198	1	100	3.7	20423	PASS
441	198	0.01	100	13.0	71747	PASS
442	442	50	100	100.0	459179	PASS
443	442	15	24	19.5	89448	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/9/2025	BNA_M	<u>BM050156.D</u>
Compound Name	Response	Retention Time
DDT	1813443	20.621
DDD	24993	20.233
DDE	3322	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28315	1841758	1.54

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
Data File : BM050156.D
Acq On : 09 May 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 09 13:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration

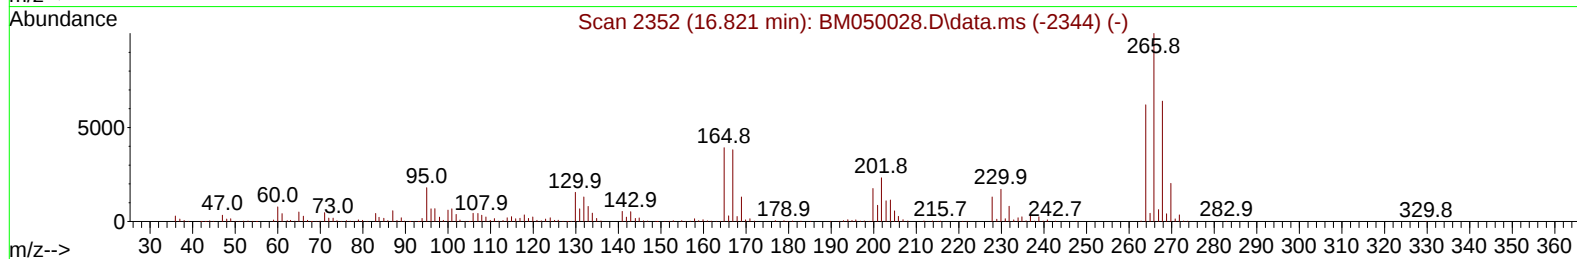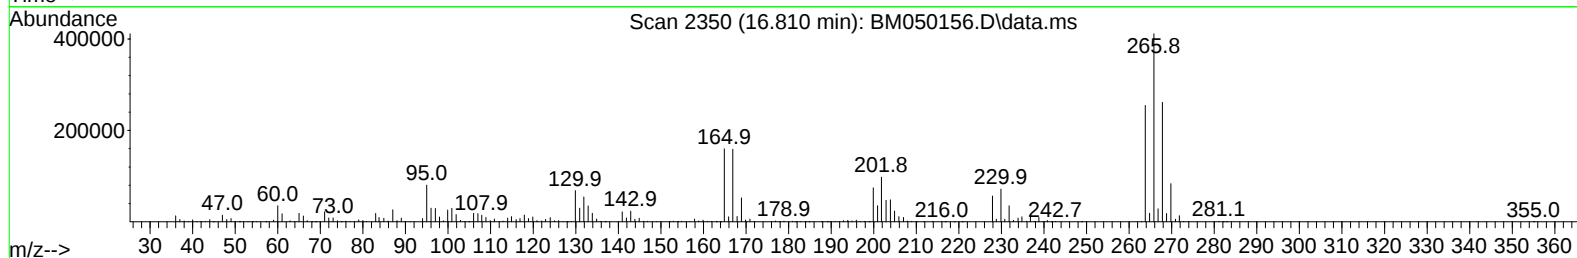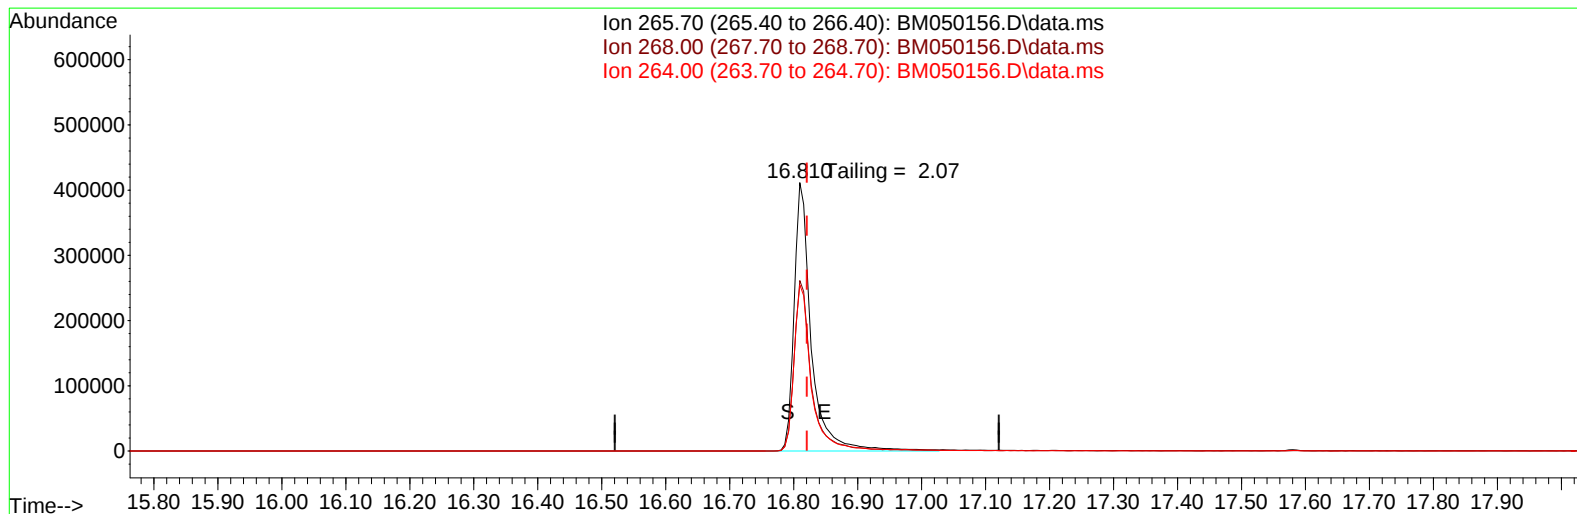

TIC: BM050156.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.011) 0.00 ng




response 768482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.51
264.00	62.00	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050925\
Data File : BM050156.D
Acq On : 09 May 2025 12:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 09 13:48:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 08 12:03:21 2025
Response via : Initial Calibration

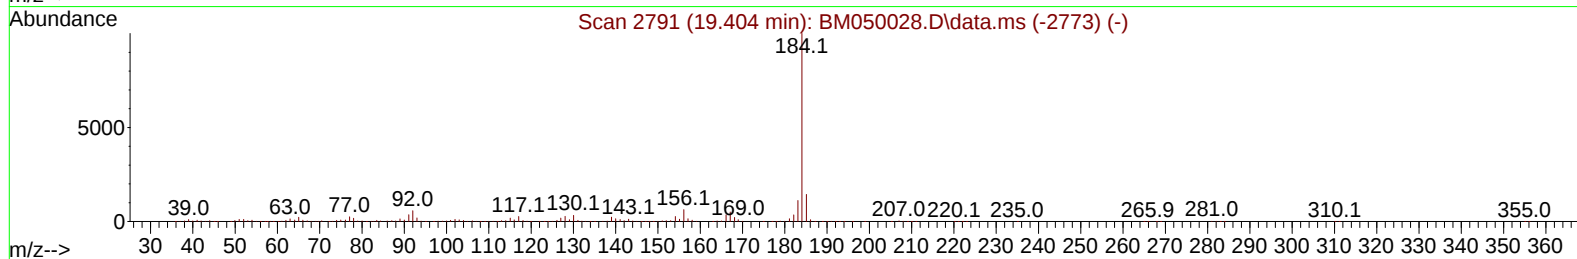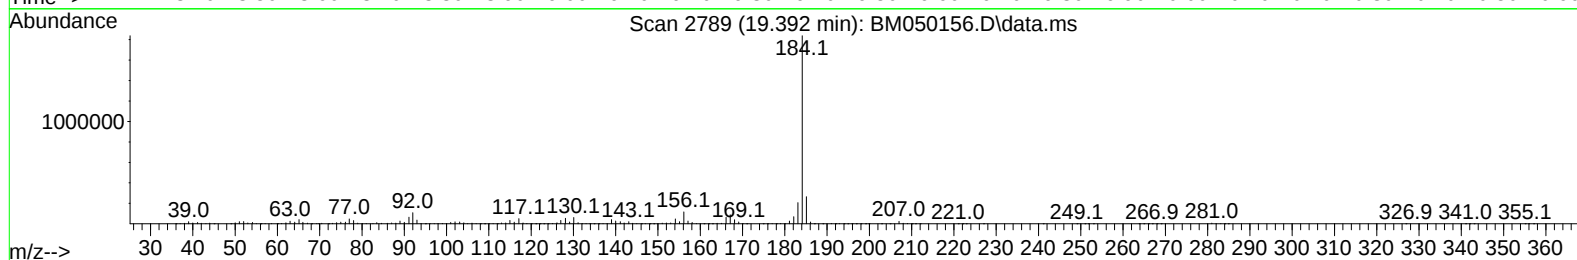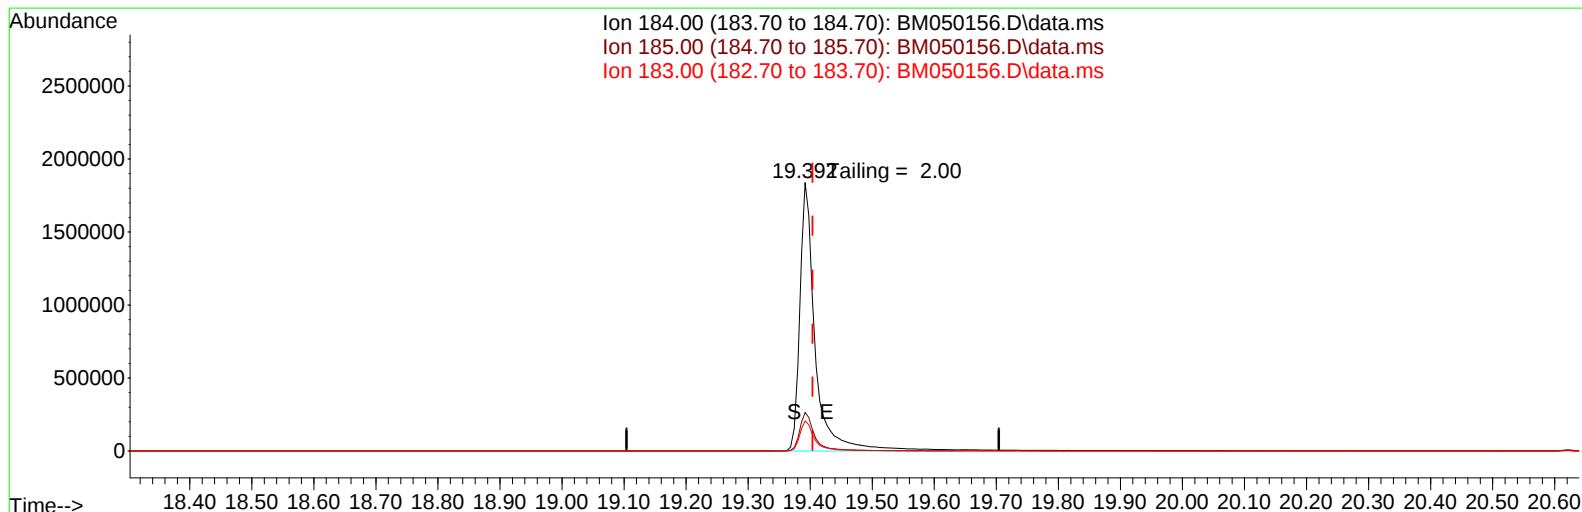

TIC: BM050156.D\data.ms

(77) Benzidine

19.392min (-0.012) 32977.87 ng

response 3196740

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	11.10	11.21
0.00	0.00	0.00