

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051016\
 Data File : BM005372.D
 Acq On : 10 May 2016 13:17
 Operator : UM/SJ
 Sample : H2888-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WW9

Quant Time: May 11 07:57:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 11 07:57:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	76758	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	373466	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	253595	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	614309	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	699969	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	581664	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	6816	4.18	ng/uL	0.00
5) Phenol-d5	6.93	99	157684	22.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	96875	24.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	125593	23.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	133367	23.18	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	66676	25.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	78419	25.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	130836	23.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	191228	28.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	521691	25.67	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	581330	24.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	90548	24.40	ng/ul	0.00
57) Fluorene-d10	15.40	176	437843	24.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	80207	23.21	ng/ul	0.00
70) Anthracene-d10	17.25	188	711843	26.21	ng/ul	0.00
76) Pyrene-d10	19.55	212	842204	26.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	686200	26.65	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	133346	6.57	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051016\
Data File : BM005372.D
Acq On : 10 May 2016 13:17
Operator : UM/SJ
Sample : H2888-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WW9

Quant Time: May 11 07:57:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 11 07:57:14 2016
Response via : Initial Calibration

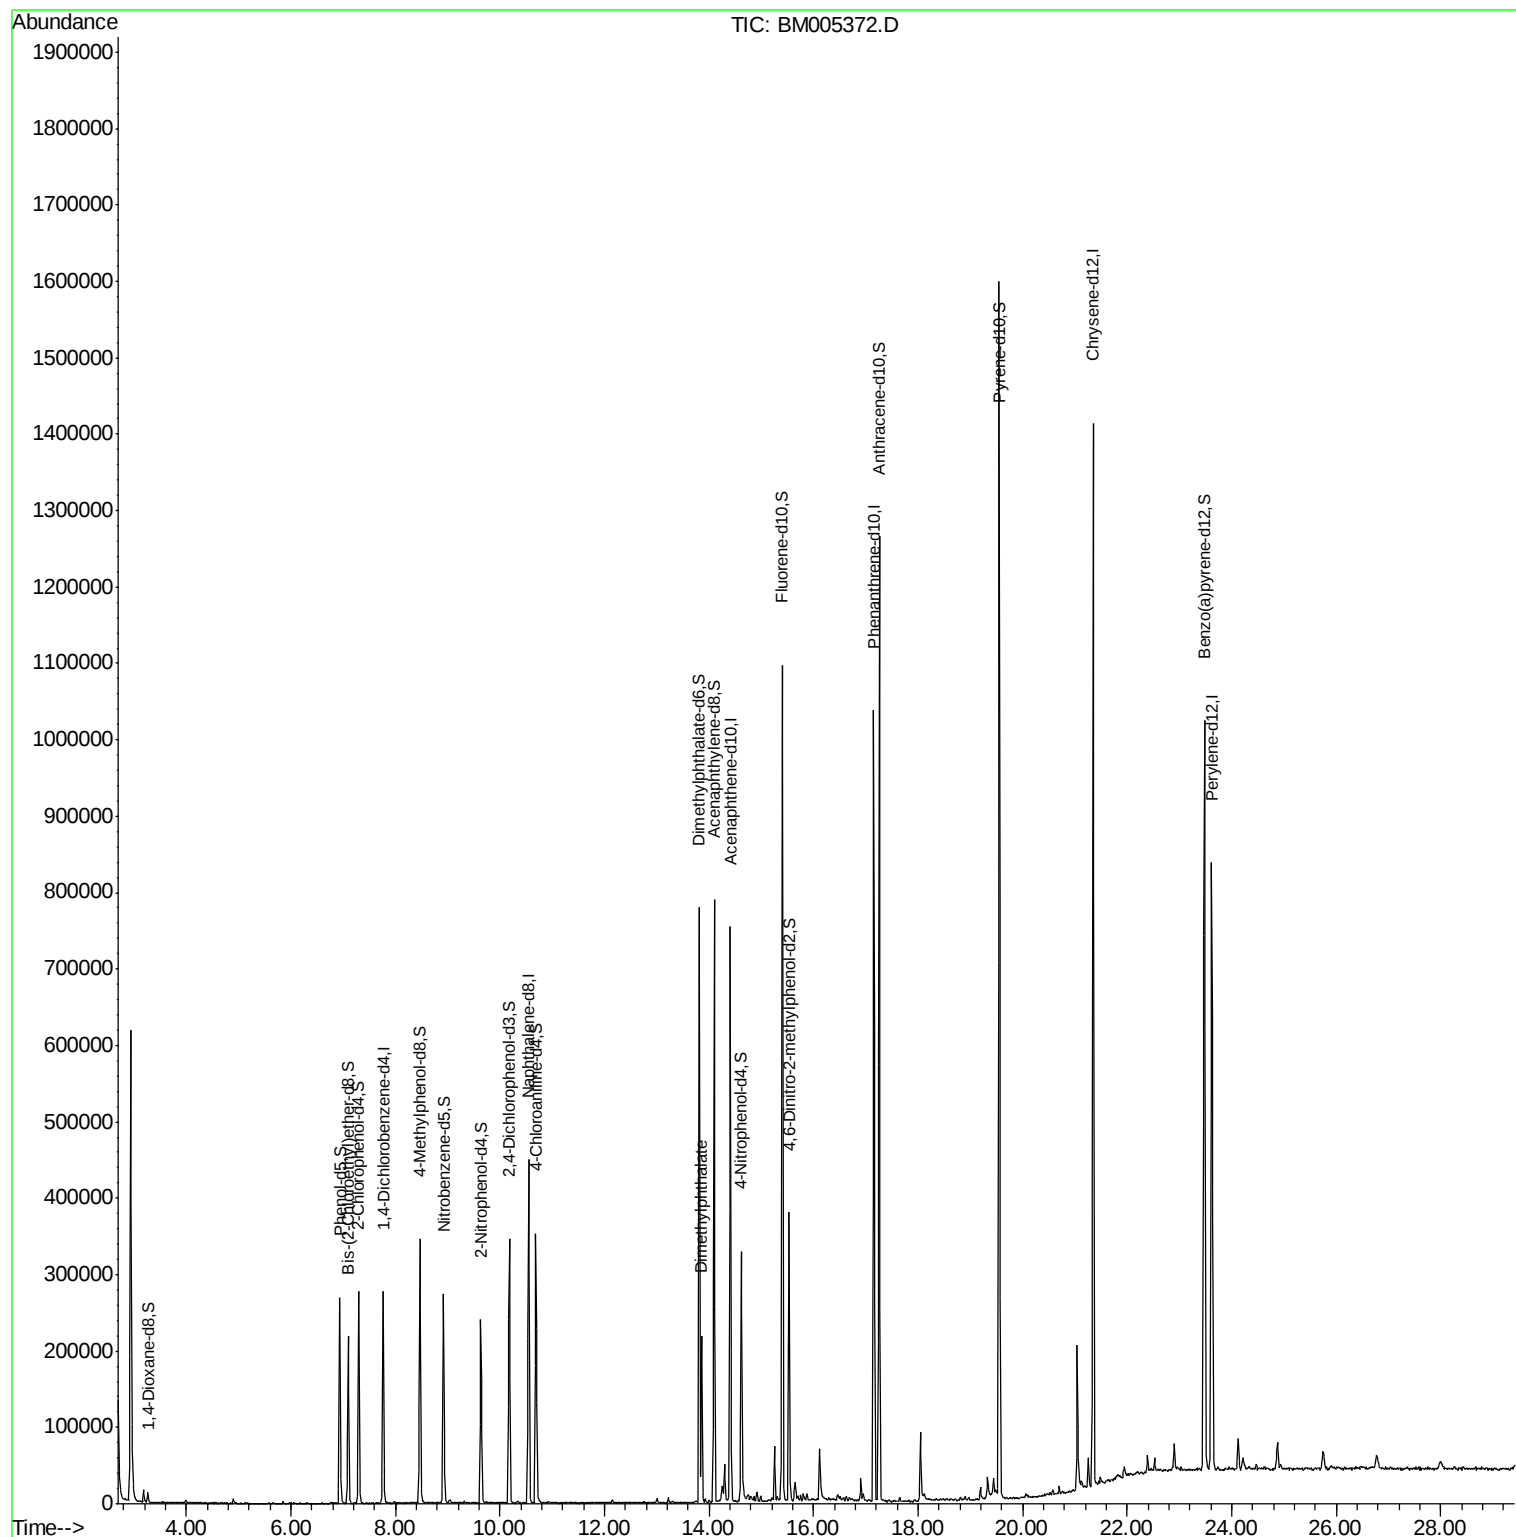

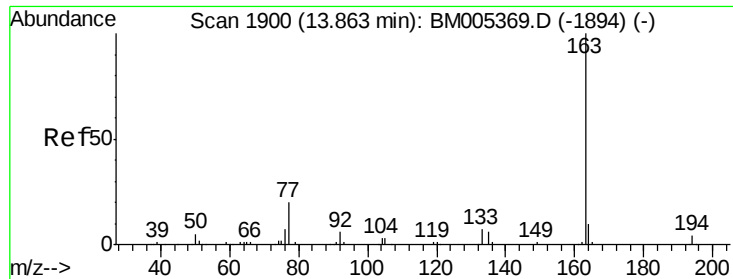

#44

Dimethylphthalate

Concen: 6.57 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. -0.01 min

Lab File: BM005372.D

Acq: 10 May 2016 13:17

Instrument :

BNA_M

ClientSampleId :

D9WW9


Tgt Ion:163 Resp: 133346

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.3 7.9 11.9

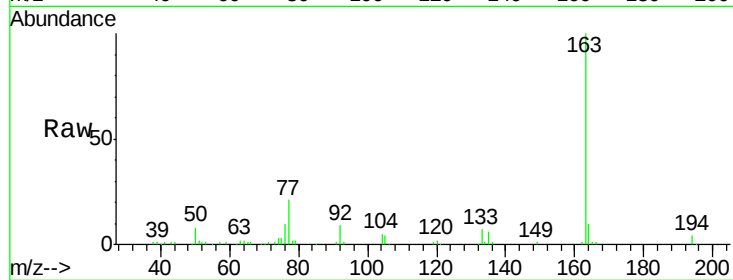

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

