

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051016\
 Data File : BM005376.D
 Acq On : 10 May 2016 15:42
 Operator : UM/SJ
 Sample : H2888-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WX7

Quant Time: May 11 07:58:12 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 11 07:57:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	74150	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	354538	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	240725	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	596337	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	798214	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	832256	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	4695	2.98	ng/uL	0.00
5) Phenol-d5	6.93	99	109243	16.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	65035	16.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	85646	16.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	94249	16.96	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	44430	17.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	52355	18.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	91833	17.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	130666	20.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	351585	18.22	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	405948	17.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	63198	17.94	ng/ul	0.00
57) Fluorene-d10	15.40	176	308747	18.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	53449	15.93	ng/ul	0.00
70) Anthracene-d10	17.25	188	497448	18.87	ng/ul	0.00
76) Pyrene-d10	19.55	212	642096	17.43	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	714132	19.38	ng/ul	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.86	163	58554	3.04	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051016\
 Data File : BM005376.D
 Acq On : 10 May 2016 15:42
 Operator : UM/SJ
 Sample : H2888-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WX7

Quant Time: May 11 07:58:12 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 11 07:57:14 2016
 Response via : Initial Calibration

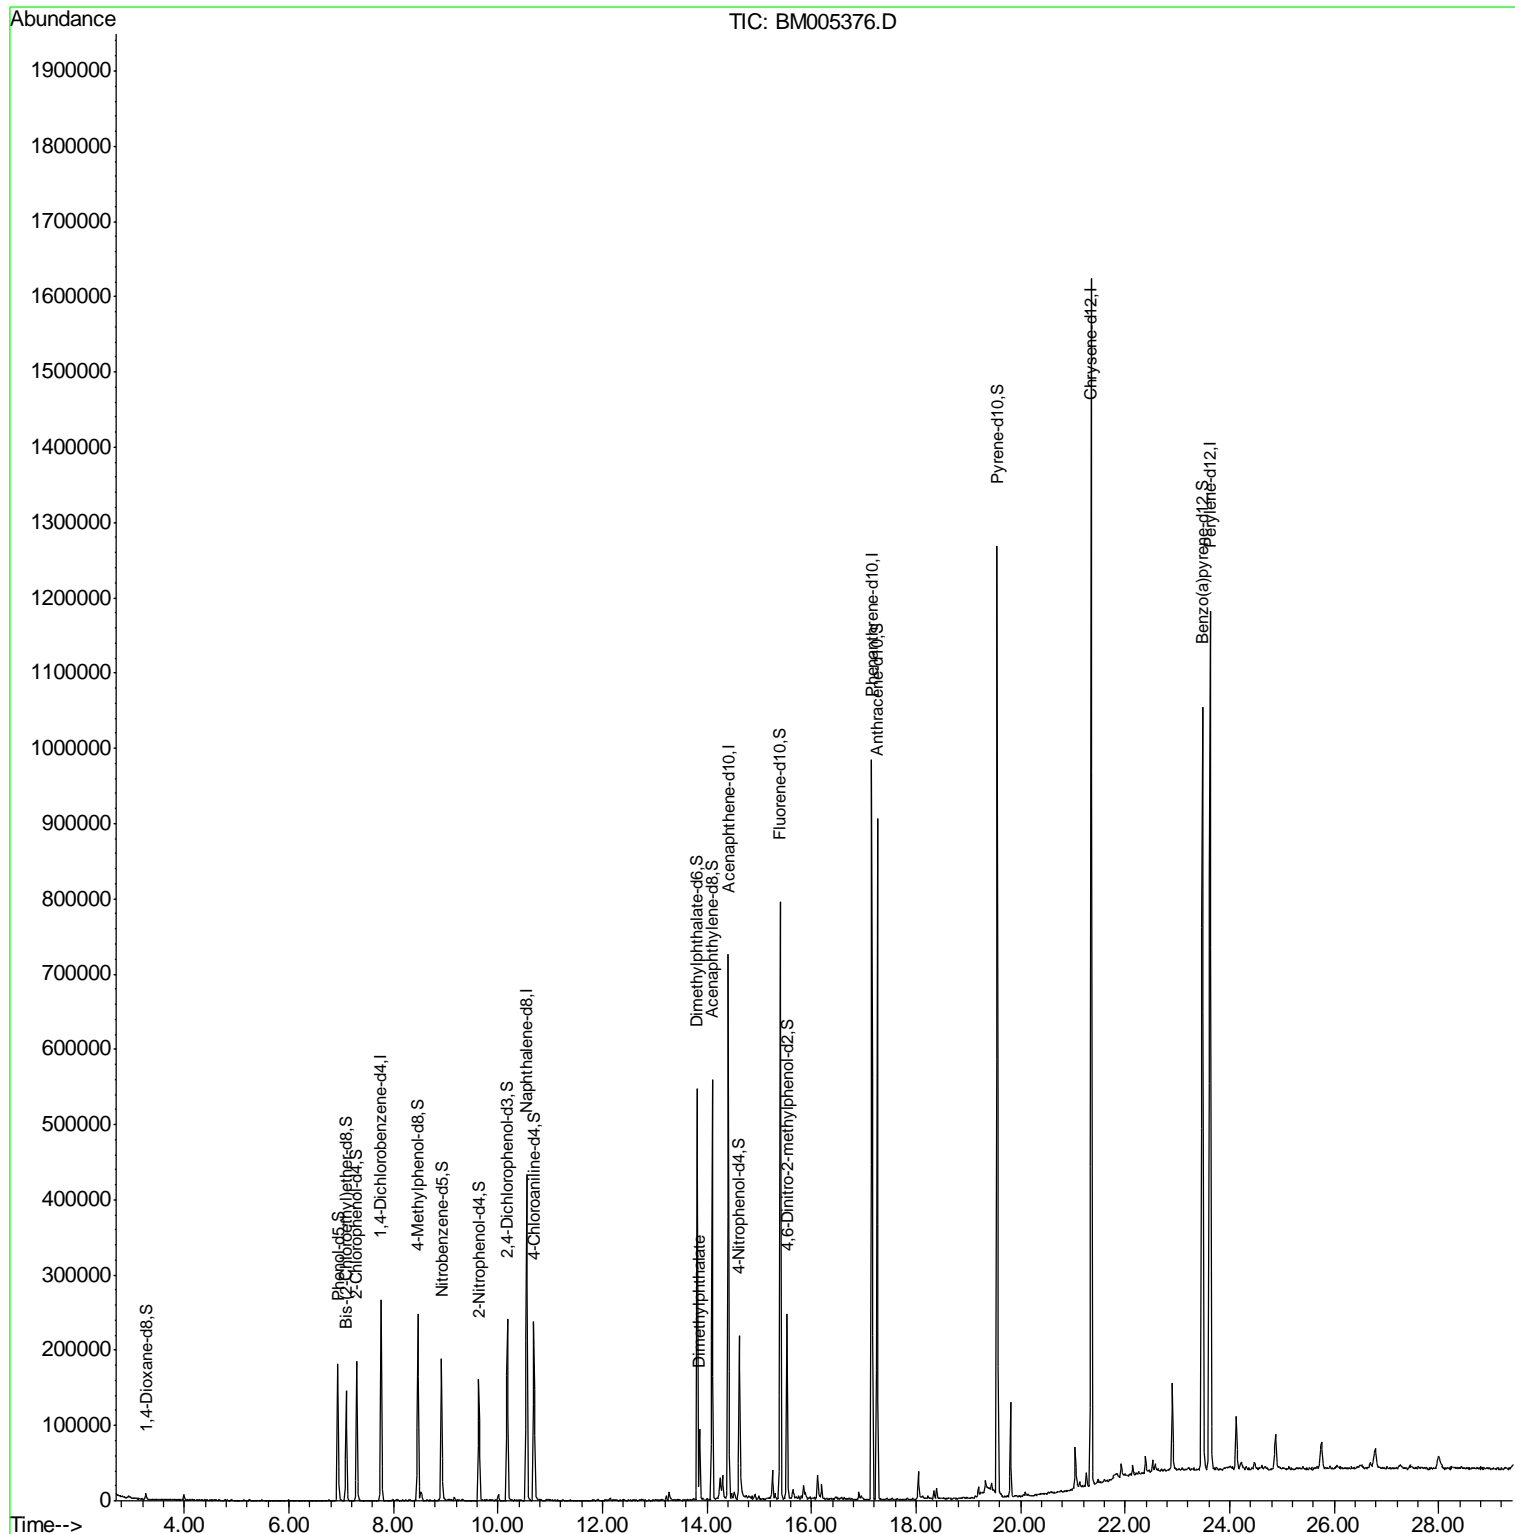

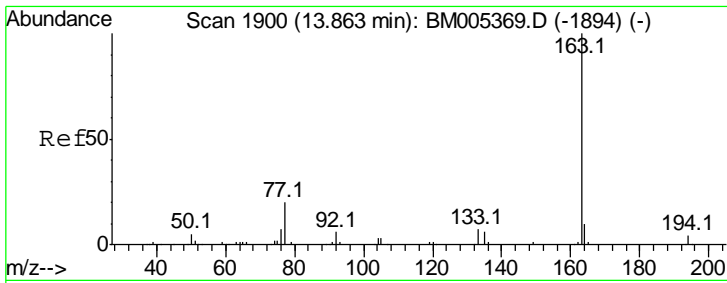

#44
 Dimethylphthalate
 Concen: 3.04 ng/ul
 RT: 13.86 min Scan# 1899
 Delta R.T. -0.01 min
 Lab File: BM005376.D
 Acq: 10 May 2016 15:42

Instrument :
 BNA_M
ClientSampled :
 D9WX7

Tot Ion	Ion	Ratio	Lower	Upper
58554	163	100		
	194	4.6	3.4	5.0
	164	10.0	7.9	11.9

