


Data Path : Z:\HPCHEM1\BNA M\Data\BM051016\
 Data File : BM005368.D
 Acq On : 10 May 2016 10:52
 Operator : UM/SJ
 Sample : DFTPP35
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP35

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 28 06:36:34 2015

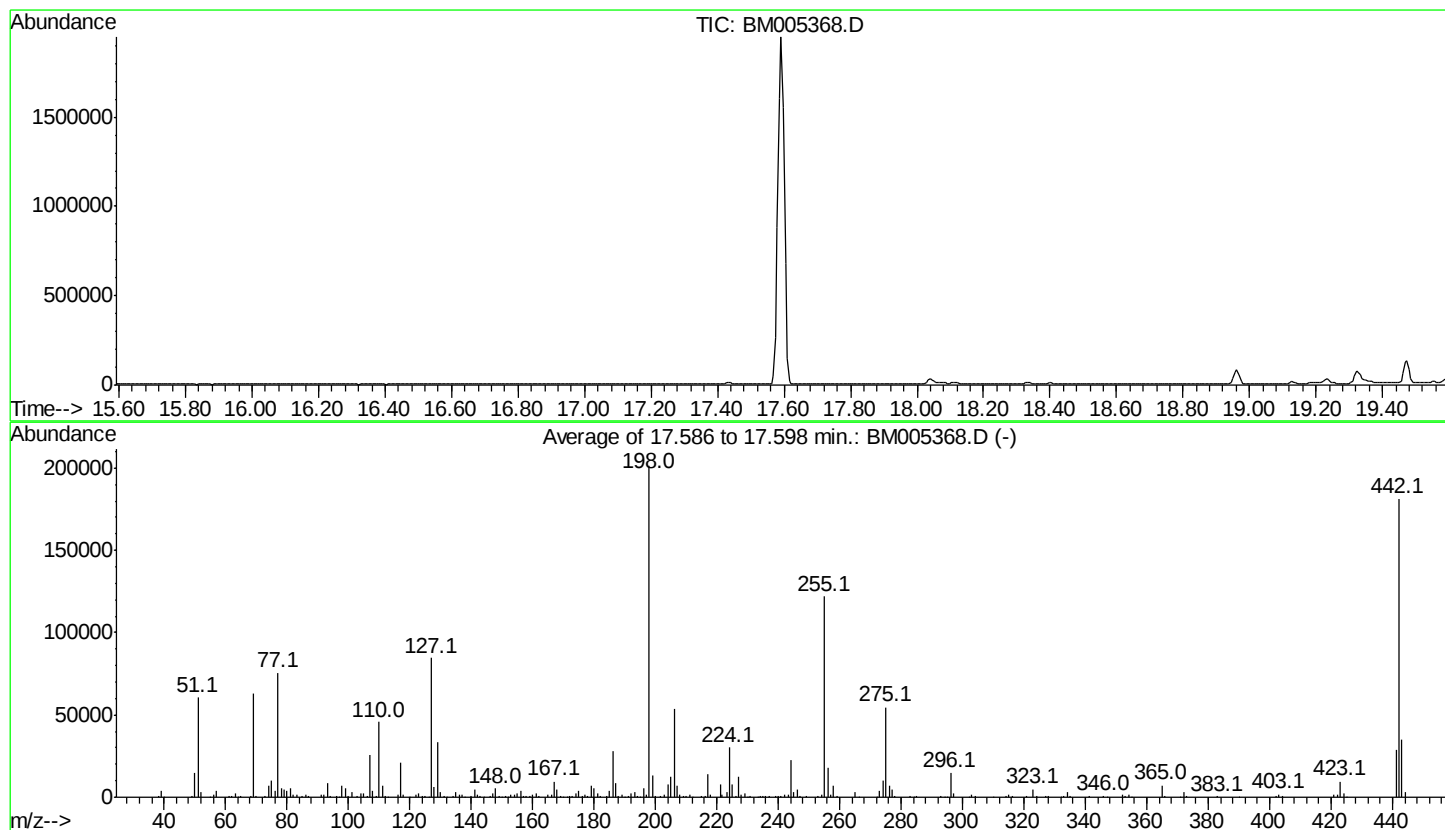

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	60533	PASS
68	69	0.00	2	1.9	1182	PASS
69	198	0.00	100	31.5	63362	PASS
70	69	0.00	2	0.7	430	PASS
127	198	10	80	42.0	84565	PASS
197	198	0.00	2	0.7	1485	PASS
198	198	100	100	100.0	201408	PASS
199	198	5	9	6.7	13504	PASS
275	198	10	60	27.2	54746	PASS
365	198	1	100	3.6	7177	PASS
441	443	0.01	100	81.4	28530	PASS
442	198	50	100	90.1	181546	PASS
443	442	15	24	19.3	35056	PASS

Scan 2527 (17.551 min): BM005368.D
DFTPP35

m/z	Abundance
40.00	351.0
41.00	445.0
43.00	1036.0
44.00	1060.0
45.00	527.0
55.00	438.0
57.00	361.0
60.00	415.0
73.00	370.0
207.10	436.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
38.00	682.0
39.10	4199.0
40.00	376.0
41.10	420.0
43.10	769.0
44.00	733.0
45.00	418.0
49.10	538.0
50.10	15457.0
51.10	64136.0
52.10	3555.0
55.00	586.0
56.00	1858.0
57.00	4347.0
61.00	749.0
62.10	960.0
63.00	2750.0
64.00	425.0
65.10	1212.0
68.10	1251.0
69.00	66040.0
70.00	353.0
73.00	840.0
74.10	6929.0
75.10	11342.0
76.10	3721.0
77.10	78496.0
78.10	5682.0
79.00	5211.0
80.00	3886.0
81.00	5838.0
82.00	1523.0
83.00	1338.0
85.00	1044.0
86.00	1794.0
87.00	772.0
91.00	1332.0
92.00	1385.0
93.00	8866.0
94.00	756.0
96.10	608.0
98.00	7546.0
99.00	5461.0
100.00	510.0
101.00	3162.0
103.00	1072.0
104.00	2176.0
105.00	2025.0
106.10	696.0
107.00	26008.0
108.10	4027.0
109.10	742.0
110.00	46312.0
111.00	7103.0
112.00	800.0
113.00	300.0
116.10	1489.0
117.00	21056.0
118.00	1440.0
122.00	1961.0
123.00	2788.0
124.00	1098.0
125.00	1140.0
127.10	84664.0
128.00	6800.0
129.00	33176.0
130.00	2970.0
131.00	516.0
132.10	307.0
134.00	1053.0
135.00	2812.0
136.00	1337.0
137.00	1476.0
137.90	339.0
140.00	413.0
141.00	4518.0
142.00	1693.0
143.00	996.0
146.00	774.0
147.00	2519.0
148.00	5509.0
149.10	1139.0
150.10	322.0
151.00	610.0
151.90	348.0
153.00	1516.0
154.10	1274.0
155.00	2419.0
156.10	4279.0
157.00	838.0
158.00	818.0
159.00	744.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

160.00	1449.0
161.00	2177.0
162.00	759.0
165.00	1667.0
166.00	1388.0
167.10	9577.0
168.00	4674.0
169.00	952.0
170.00	367.0
171.00	357.0
172.00	766.0
173.00	1063.0
174.00	1988.0
175.10	3918.0
176.10	988.0
177.00	1850.0
178.00	750.0
179.00	6711.0
180.00	4880.0
181.00	2267.0
182.00	439.0
184.10	621.0
185.10	3612.0
186.10	27128.0
187.10	8129.0
188.00	803.0
189.00	1779.0
191.00	802.0
192.00	2372.0
193.10	2775.0
194.10	581.0
195.10	308.0
196.00	5025.0
197.10	1385.0
198.00	193216.0
199.00	13605.0
200.00	1166.0
201.60	781.0
203.00	1365.0
204.10	7039.0
205.10	12217.0
206.10	52072.0
207.10	7163.0
208.00	1745.0
209.00	584.0
210.10	761.0
211.10	2042.0
215.10	572.0
216.10	1006.0
217.00	13209.0
218.10	1954.0
221.10	7253.0
221.80	2012.0
223.10	3029.0
224.10	28600.0
225.10	7377.0
226.10	682.0
227.00	12145.0
228.10	1683.0
229.00	2561.0
230.00	367.0
231.00	998.0
234.00	825.0
235.00	936.0
236.00	586.0
237.00	984.0
238.90	493.0
240.00	468.0
241.00	633.0
242.10	1511.0
243.10	1553.0
244.10	20856.0
245.10	2817.0
246.10	4748.0
247.00	907.0
249.00	778.0
253.10	445.0
254.20	1184.0
255.10	109808.0
256.10	16371.0
257.00	1281.0
258.10	6402.0
259.00	1120.0
265.00	2512.0
272.10	343.0
273.10	3129.0
274.10	9134.0
275.10	49456.0
276.10	6737.0
277.00	4312.0
278.00	720.0
283.10	552.0
284.00	314.0
285.10	635.0
293.10	1012.0
295.10	339.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

296.10	13740.0
297.00	1901.0
303.10	1350.0
304.00	427.0
314.00	604.0
315.00	1454.0
316.10	832.0
321.00	444.0
323.10	4087.0
324.10	799.0
327.00	876.0
328.00	354.0
332.10	326.0
333.00	533.0
334.10	2722.0
335.10	724.0
341.10	453.0
346.00	843.0
352.00	1177.0
353.10	828.0
354.10	1361.0
355.10	343.0
365.00	6123.0
366.00	956.0
371.00	308.0
372.10	1929.0
373.10	427.0
383.00	626.0
402.00	928.0
403.00	1506.0
404.10	505.0
421.10	989.0
422.10	1028.0
423.10	7675.0
424.10	2098.0
441.10	21736.0
442.10	138944.0
443.10	28360.0
444.10	2635.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
38.10	765.0
39.10	4519.0
40.00	361.0
41.00	480.0
43.00	701.0
44.00	776.0
45.00	441.0
49.10	454.0
50.10	17040.0
51.10	68224.0
52.10	3182.0
55.10	684.0
56.00	2185.0
57.10	4590.0
61.00	867.0
62.00	1049.0
63.10	2993.0
64.00	440.0
65.10	1281.0
68.10	1277.0
69.00	72560.0
70.00	588.0
73.10	978.0
74.10	7915.0
75.00	12112.0
76.10	4289.0
77.10	85544.0
78.10	5529.0
79.10	5462.0
80.00	4310.0
81.10	6462.0
82.00	1518.0
83.00	1368.0
85.10	1325.0
86.00	1863.0
87.00	916.0
91.00	1492.0
92.10	1666.0
93.00	9898.0
94.10	773.0
96.00	648.0
97.10	392.0
98.10	8371.0
99.00	6101.0
100.00	583.0
101.10	3651.0
103.00	1188.0
104.10	2352.0
105.00	2314.0
106.10	668.0
107.00	29560.0
108.00	4273.0
109.10	913.0
110.00	51048.0
111.00	7469.0
112.00	1008.0
113.00	369.0
116.10	1560.0
117.00	23608.0
118.00	1552.0
120.00	398.0
122.00	2014.0
123.00	3159.0
124.00	1469.0
125.00	1241.0
127.10	96664.0
128.00	7425.0
129.00	38000.0
130.00	3377.0
131.00	608.0
132.00	341.0
134.10	1163.0
135.00	3305.0
136.00	1356.0
137.10	1683.0
140.00	520.0
141.00	5555.0
142.00	1880.0
143.00	1103.0
144.00	303.0
146.00	1163.0
147.00	2857.0
148.00	5868.0
149.00	1292.0
150.10	379.0
151.10	607.0
151.90	413.0
153.00	1835.0
154.00	1214.0
155.10	3117.0
156.10	4778.0
157.00	798.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

158.00	1028.0
159.00	762.0
160.00	1742.0
161.00	2454.0
162.00	819.0
165.00	2187.0
166.10	1733.0
167.10	11289.0
168.10	5201.0
169.10	890.0
170.00	428.0
171.00	457.0
172.00	1049.0
173.00	1451.0
174.10	2216.0
175.10	4538.0
176.00	1342.0
177.10	2092.0
178.00	638.0
179.00	8115.0
180.10	5991.0
181.10	2701.0
182.00	567.0
184.00	665.0
185.10	4172.0
186.10	32680.0
187.10	9502.0
188.10	887.0
189.00	2174.0
190.00	391.0
191.00	940.0
192.00	2654.0
193.10	3265.0
194.00	683.0
195.00	346.0
196.00	6292.0
197.20	1900.0
198.00	230400.0
199.00	14952.0
200.00	1180.0
201.40	821.0
203.00	1710.0
204.10	8743.0
205.10	14877.0
206.10	62328.0
207.10	8271.0
208.00	2214.0
209.00	727.0
210.00	960.0
211.10	1959.0
211.90	370.0
215.00	681.0
216.10	1392.0
217.00	16278.0
218.00	2221.0
221.10	8365.0
223.10	3628.0
224.10	34456.0
225.10	8638.0
226.10	1116.0
227.00	14135.0
228.00	2016.0
229.00	2768.0
230.00	344.0
231.00	1267.0
234.00	858.0
235.00	1098.0
236.00	805.0
237.10	1160.0
239.00	499.0
240.00	490.0
241.00	948.0
242.10	2036.0
243.10	1903.0
244.10	25480.0
245.10	3469.0
246.10	5678.0
247.00	1153.0
249.00	1011.0
253.00	522.0
254.20	1579.0
255.10	140032.0
256.10	20752.0
257.10	1572.0
258.00	8322.0
259.10	1215.0
265.10	3441.0
266.10	580.0
272.10	354.0
273.10	4109.0
274.10	11525.0
275.10	62952.0
276.10	8007.0
277.00	5514.0
278.00	843.0
283.00	628.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

284.10	470.0
285.10	993.0
293.00	1074.0
295.10	390.0
296.10	17520.0
297.00	2341.0
302.00	307.0
303.10	2153.0
304.10	569.0
310.00	353.0
314.00	795.0
315.00	2095.0
316.00	1188.0
321.00	493.0
323.10	5348.0
324.10	987.0
327.00	966.0
328.10	500.0
332.00	462.0
333.10	636.0
334.10	3767.0
335.10	1045.0
341.00	597.0
346.00	1366.0
347.00	324.0
352.10	1709.0
353.00	1220.0
354.10	2037.0
355.00	394.0
365.00	8329.0
366.00	1039.0
371.00	493.0
372.10	3421.0
373.10	745.0
383.00	769.0
390.00	379.0
402.00	1324.0
403.00	1947.0
404.00	672.0
421.00	1546.0
422.10	1699.0
423.10	11034.0
424.10	2503.0
425.10	335.0
441.10	32648.0
442.10	209408.0
443.10	40536.0
444.00	3571.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
38.00	682.0
39.10	3499.0
40.00	418.0
41.00	414.0
43.00	766.0
44.00	992.0
45.00	538.0
49.00	410.0
50.10	11772.0
51.10	49240.0
52.10	2315.0
55.00	611.0
56.00	1631.0
57.00	3392.0
60.00	305.0
61.00	694.0
62.00	759.0
63.10	2029.0
64.00	354.0
65.00	1061.0
68.10	1019.0
69.00	51488.0
70.00	349.0
73.00	744.0
74.10	5486.0
75.00	8101.0
76.10	3123.0
77.10	63024.0
78.10	4252.0
79.00	3999.0
80.00	2941.0
81.00	4558.0
82.00	1158.0
83.10	990.0
85.00	922.0
86.00	1422.0
87.00	507.0
91.00	1157.0
92.00	1181.0
93.10	7480.0
94.00	593.0
96.10	412.0
98.00	5587.0
99.00	4373.0
99.90	419.0
101.00	2713.0
103.00	948.0
104.00	1812.0
105.00	1746.0
106.10	601.0
107.10	21136.0
108.00	3229.0
109.10	621.0
110.00	39280.0
111.00	5562.0
112.00	780.0
116.00	1149.0
117.00	17256.0
118.00	1262.0
122.00	1355.0
123.00	2174.0
124.10	890.0
125.00	881.0
126.20	544.0
127.10	72368.0
128.00	5203.0
129.00	28856.0
130.00	2281.0
131.00	539.0
134.00	988.0
135.00	2442.0
136.00	927.0
137.10	1165.0
140.10	378.0
141.00	3959.0
142.00	1306.0
142.90	907.0
146.10	839.0
147.10	2143.0
148.00	4688.0
149.00	962.0
150.00	330.0
151.10	526.0
153.00	1138.0
154.00	1089.0
155.00	2507.0
156.10	3611.0
157.00	623.0
158.00	668.0
159.00	534.0
160.00	1213.0
161.00	1996.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

162.00	508.0
165.00	1585.0
166.00	1308.0
167.10	8100.0
168.00	3921.0
169.00	782.0
171.00	338.0
172.00	740.0
173.10	1044.0
174.00	1970.0
175.10	3204.0
176.00	964.0
177.00	1549.0
178.00	570.0
179.00	6061.0
180.00	4490.0
181.00	2180.0
182.00	371.0
184.00	539.0
185.10	3386.0
186.10	25120.0
187.10	7379.0
188.00	741.0
189.00	1604.0
191.00	885.0
192.10	2121.0
193.10	2644.0
194.00	473.0
195.00	346.0
196.00	5061.0
197.10	1172.0
198.00	180608.0
199.00	11956.0
200.10	955.0
201.50	712.0
203.00	1448.0
204.10	6589.0
205.10	11241.0
206.10	47496.0
207.10	6367.0
208.00	1625.0
209.10	627.0
210.20	775.0
211.10	1717.0
215.00	540.0
216.00	1076.0
217.00	12598.0
218.00	1680.0
221.10	7445.0
221.80	1592.0
223.10	2675.0
224.10	27512.0
225.10	6749.0
226.10	763.0
227.00	11421.0
228.00	1651.0
229.00	2337.0
230.00	310.0
231.00	856.0
233.10	306.0
234.00	705.0
235.00	839.0
236.00	492.0
237.00	1020.0
239.00	498.0
240.00	385.0
241.00	666.0
242.10	1568.0
243.10	1570.0
244.10	21288.0
245.10	2710.0
246.10	4103.0
247.00	765.0
249.00	851.0
253.10	422.0
254.20	1224.0
255.10	115504.0
256.10	16208.0
257.00	1076.0
258.00	6507.0
259.00	1080.0
265.00	2637.0
266.10	482.0
273.10	3500.0
274.10	9131.0
275.10	51832.0
276.10	6876.0
277.10	4415.0
278.00	766.0
283.10	429.0
284.10	458.0
285.00	884.0
293.00	1007.0
294.10	336.0
296.10	14293.0
297.00	2051.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

303.10	1812.0
304.10	525.0
314.10	828.0
315.00	1809.0
316.10	971.0
320.90	399.0
323.10	4887.0
324.10	932.0
327.00	888.0
328.00	467.0
332.00	326.0
333.00	534.0
334.10	3475.0
335.00	947.0
341.00	513.0
346.00	1055.0
352.00	1458.0
353.10	984.0
354.10	1783.0
355.00	364.0
365.00	7080.0
366.00	1054.0
371.00	389.0
372.10	2923.0
373.10	757.0
383.10	756.0
390.10	340.0
402.10	1144.0
403.10	1594.0
404.00	590.0
421.00	1599.0
422.10	1332.0
423.10	10414.0
424.10	2397.0
441.10	31208.0
442.10	196288.0
443.10	36272.0
444.10	3375.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35