

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051017\
 Data File : BM009981.D
 Acq On : 10 May 2017 22:11
 Operator : SJ/MA
 Sample : I3062-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TWP-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.299	201	206	215	rBV	727543	1031497	12.53%	3.155%
2	4.899	301	308	322	rBV	1354214	1831940	22.25%	5.603%
3	5.357	379	386	399	rBV	461959	752098	9.13%	2.300%
4	5.957	482	488	496	rBV	257008	375422	4.56%	1.148%
5	6.951	651	657	669	rVB	338037	609095	7.40%	1.863%
6	7.304	709	717	732	rBV	843395	1393467	16.92%	4.262%
7	7.763	789	795	802	rBV	303192	484840	5.89%	1.483%
8	8.081	842	849	858	rBV	1089853	1783852	21.66%	5.456%
9	8.940	987	995	1009	rBV	1028042	1755214	21.31%	5.368%
10	10.557	1264	1270	1281	rVB	397333	690362	8.38%	2.112%
11	11.381	1402	1410	1416	rBV2	126623	235855	2.86%	0.721%
12	13.033	1682	1691	1698	rBV	2753771	3944100	47.90%	12.063%
13	13.880	1829	1835	1843	rBV	310850	452825	5.50%	1.385%
14	14.421	1921	1927	1935	rVB2	618869	960871	11.67%	2.939%
15	15.245	2062	2067	2071	rVB4	87233	114504	1.39%	0.350%
16	15.921	2176	2182	2192	rBV	1613997	2335735	28.36%	7.144%
17	16.110	2209	2214	2220	rBV	78119	129481	1.57%	0.396%
18	17.174	2389	2395	2400	rBV	901468	1305902	15.86%	3.994%
19	18.057	2540	2545	2550	rBV2	323334	428314	5.20%	1.310%
20	19.339	2758	2763	2767	rBV	244393	337397	4.10%	1.032%
21	19.804	2835	2842	2850	rBV	6577247	8234693	100.00%	25.187%
22	21.050	3050	3054	3059	rBV	261962	328607	3.99%	1.005%
23	21.362	3102	3107	3113	rBV	1402744	1702429	20.67%	5.207%
24	23.656	3491	3497	3506	rVB	783497	1476275	17.93%	4.515%


Sum of corrected areas: 32694775

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051017\
Data File : BM009981.D
Acq On : 10 May 2017 22:11
Operator : SJ/MA
Sample : I3062-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TWP-02

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM050517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

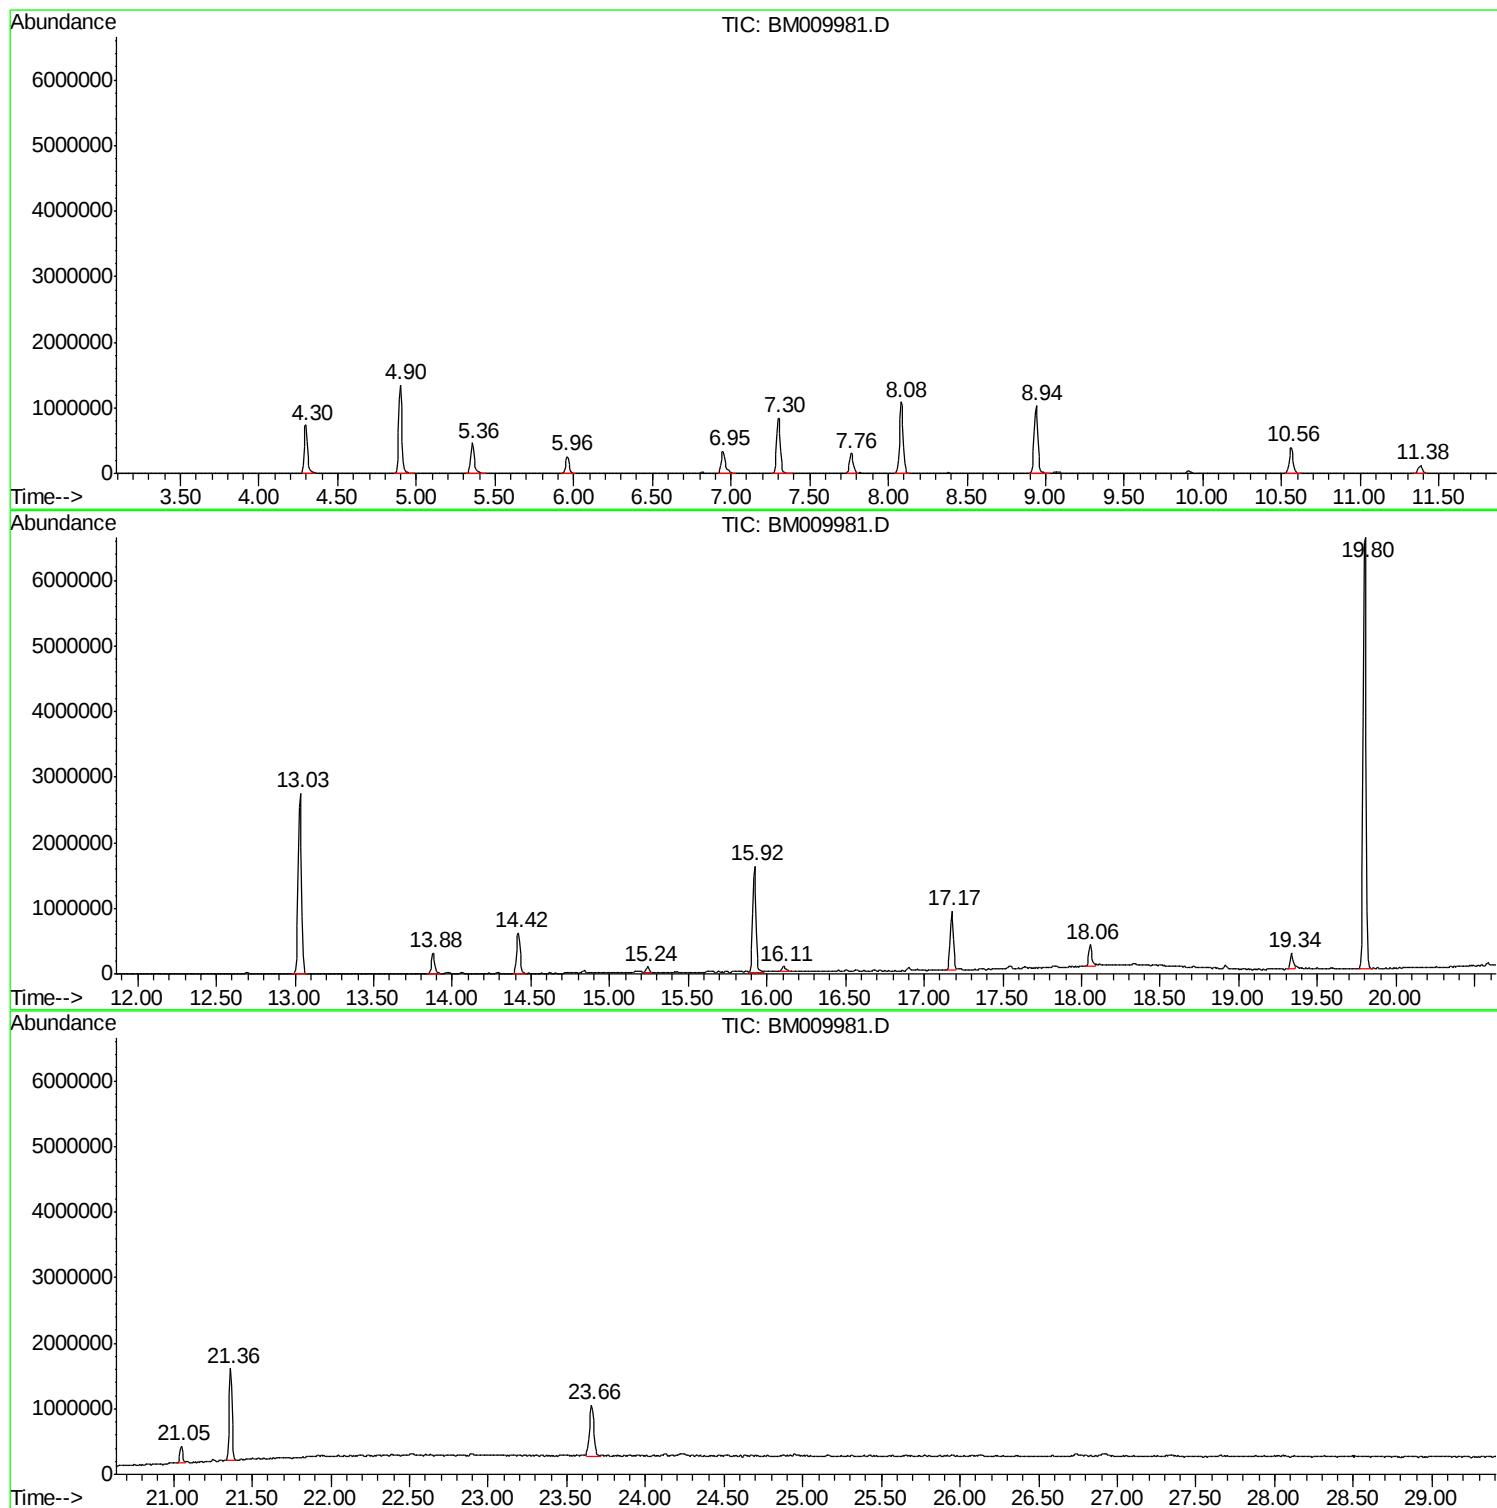

Data_Path : Z:\HPCHEM1\BNA_M\DATA\BM051017\
Data_File : BM009981.D
Acq_On : 10 May, 2017. 22:111
Operator : SJ/MAA
Sample : I3062-155
Misc :
ALS_Vial : 16 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
TWP-02

Quant_Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM050517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
