


Data Path : Z:\HPCHEM1\BNA M\Data\BM051017\
 Data File : BM009966.D
 Acq On : 10 May 2017 12:09
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

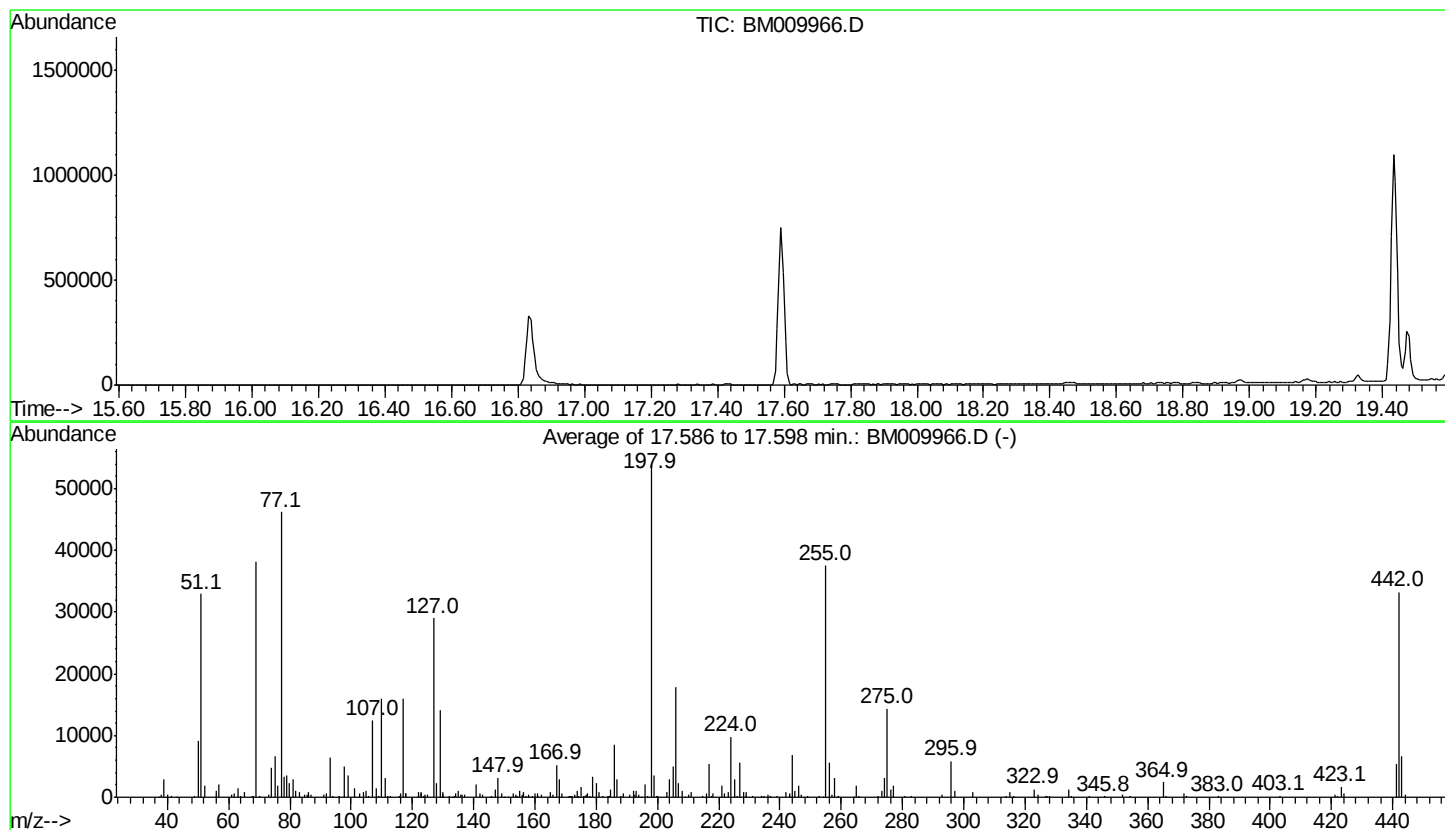

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.3	32925	PASS
68	69	0.00	2	0.8	308	PASS
69	198	0.00	100	71.2	38272	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	53.9	28962	PASS
197	198	0.00	2	0.5	293	PASS
198	198	100	100	100.0	53738	PASS
199	198	5	9	6.7	3615	PASS
275	198	10	60	26.8	14412	PASS
365	198	1	100	4.5	2424	PASS
441	442	0.01	24	16.2	5382	PASS
442	198	50	100	61.9	33250	PASS
443	442	15	24	20.2	6710	PASS