


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
Data File : BM029951.D
Acq On : 11 May 2021 20:13
Operator : CG/JU
Sample : M2177-21
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG591

Manual Integrations
APPROVED

mohammad
5/12/2021 2:06:50 PM

Quant Time: May 12 01:16:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 15:21:38 2021
Response via : Initial Calibration

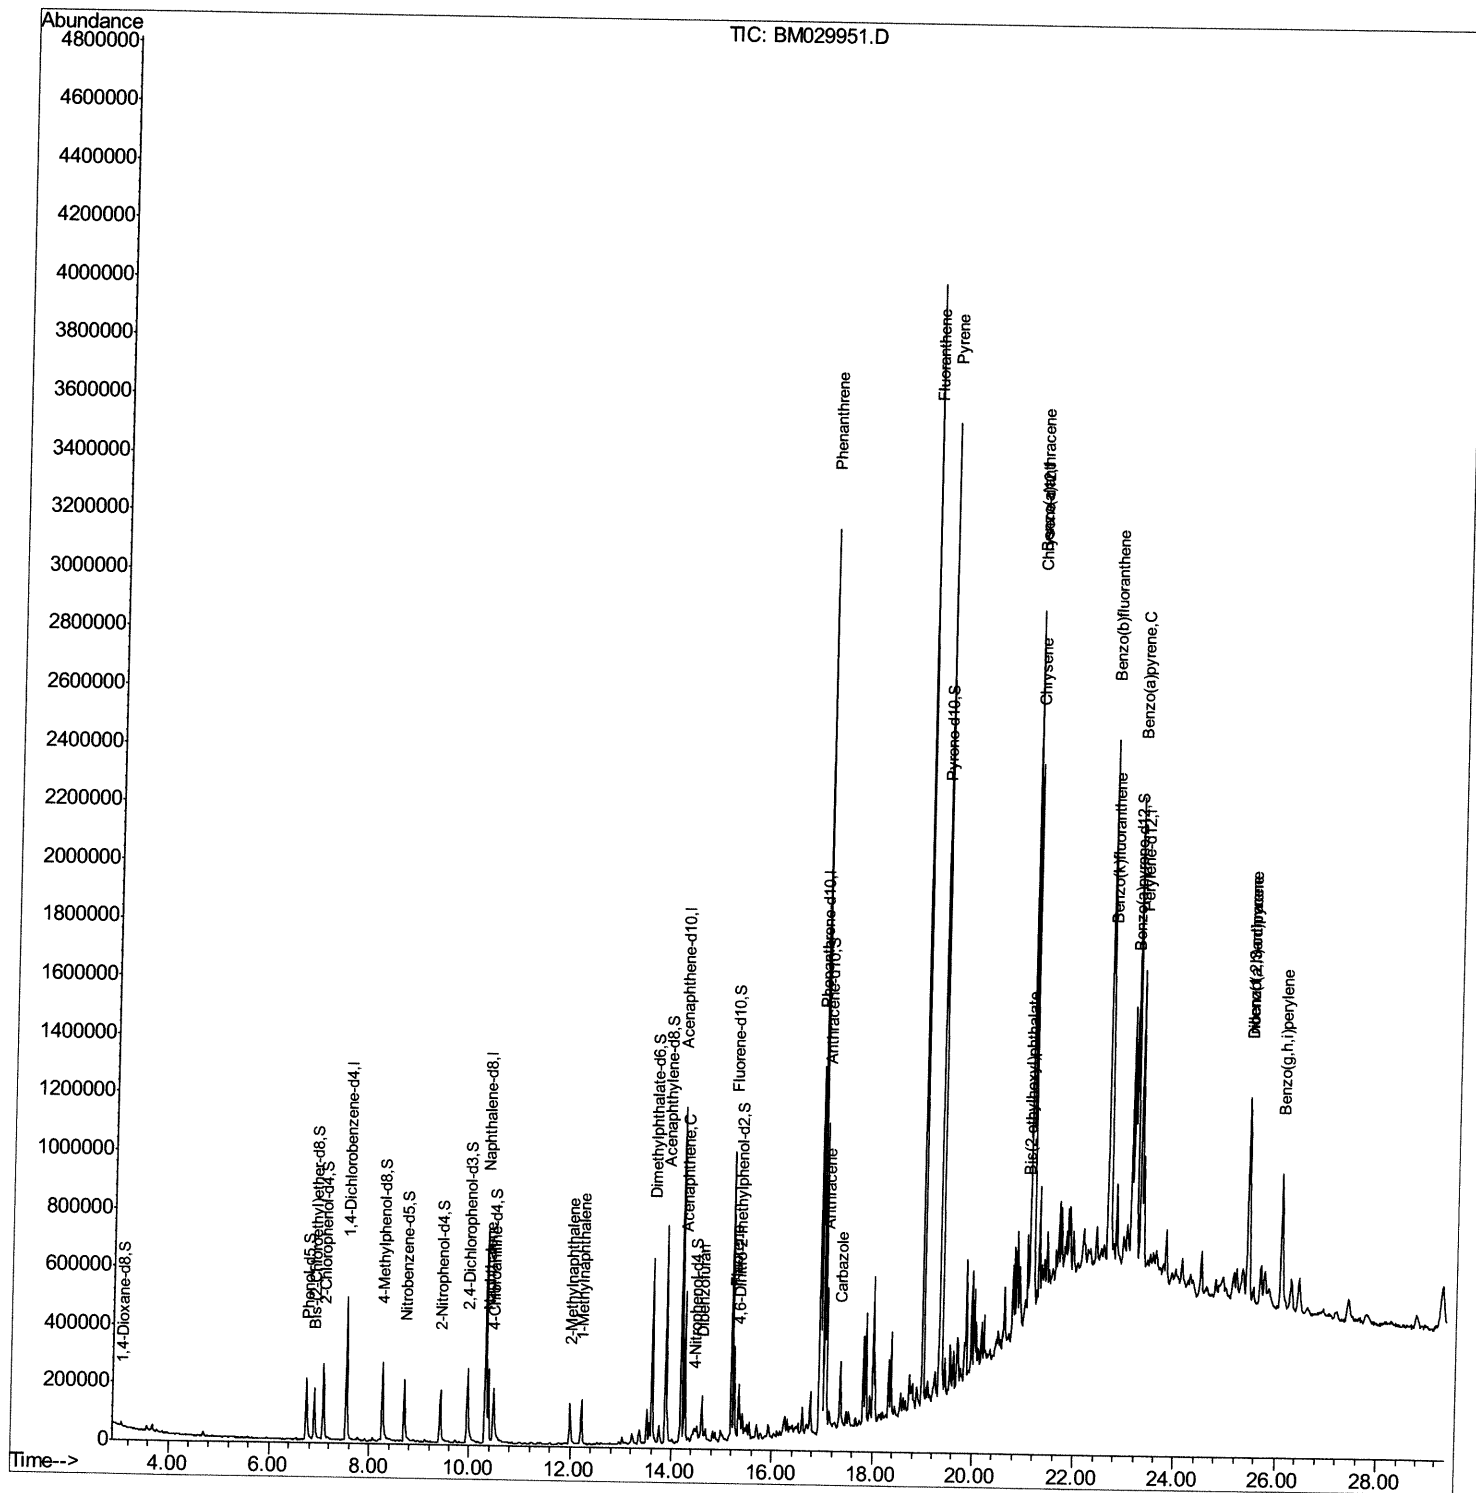

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029951.D
 Acq On : 11 May 2021 20:13
 Operator : CG/JU
 Sample : M2177-21
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG591

Manual Integrations
 APPROVED

mohammad
 5/12/2021 2:06:50 PM

Quant Time: May 12 01:13:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

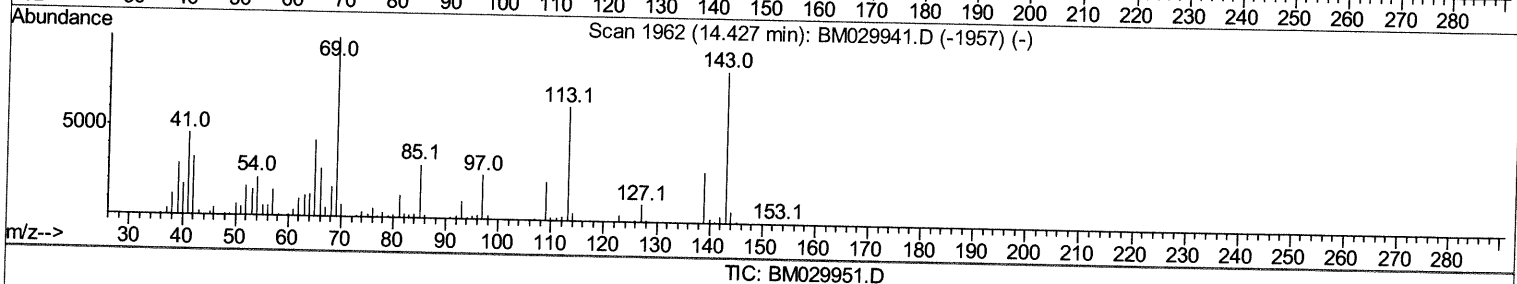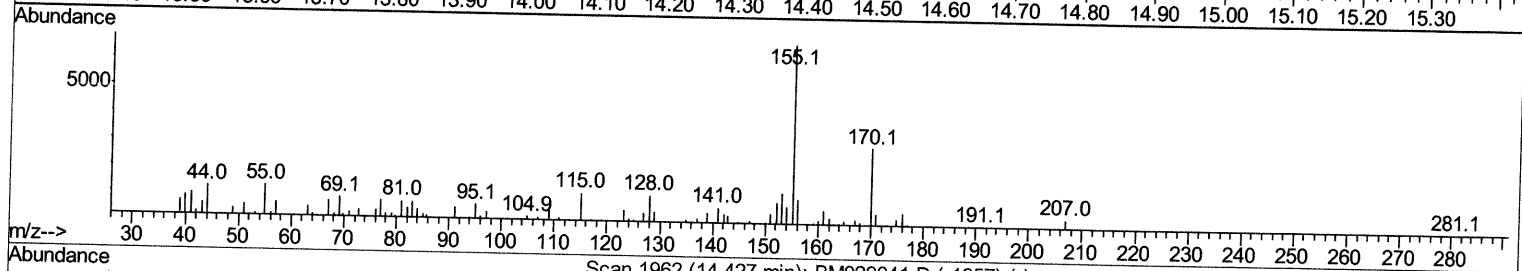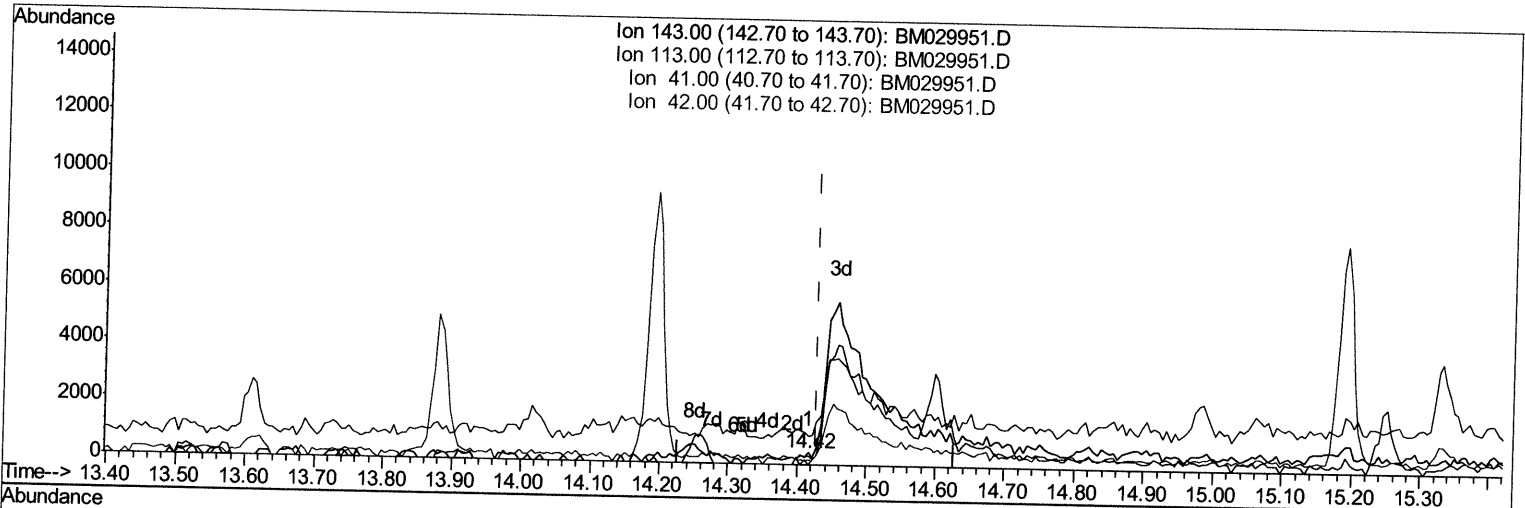

TIC: BM029951.D

(54) 4-Nitrophenol-d4 (S)

14.416min (-0.011) 0.04ng/ul

response 206

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	0.00#
41.00	44.70	236.50#
42.00	28.30	68.86#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029951.D
 Acq On : 11 May 2021 20:13
 Operator : CG/JU
 Sample : M2177-21
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BG591

Manual Integrations
APPROVED

mohammad
 5/12/2021 2:06:50 PM

Quant Time: May 12 01:13:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

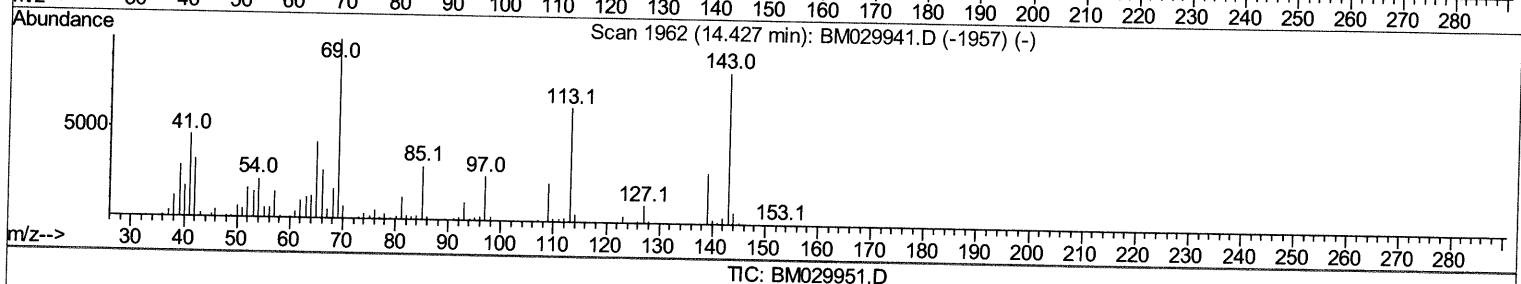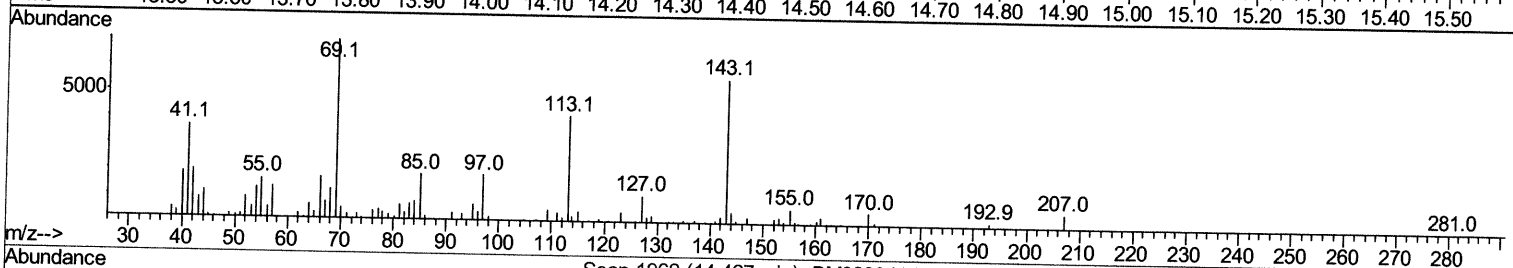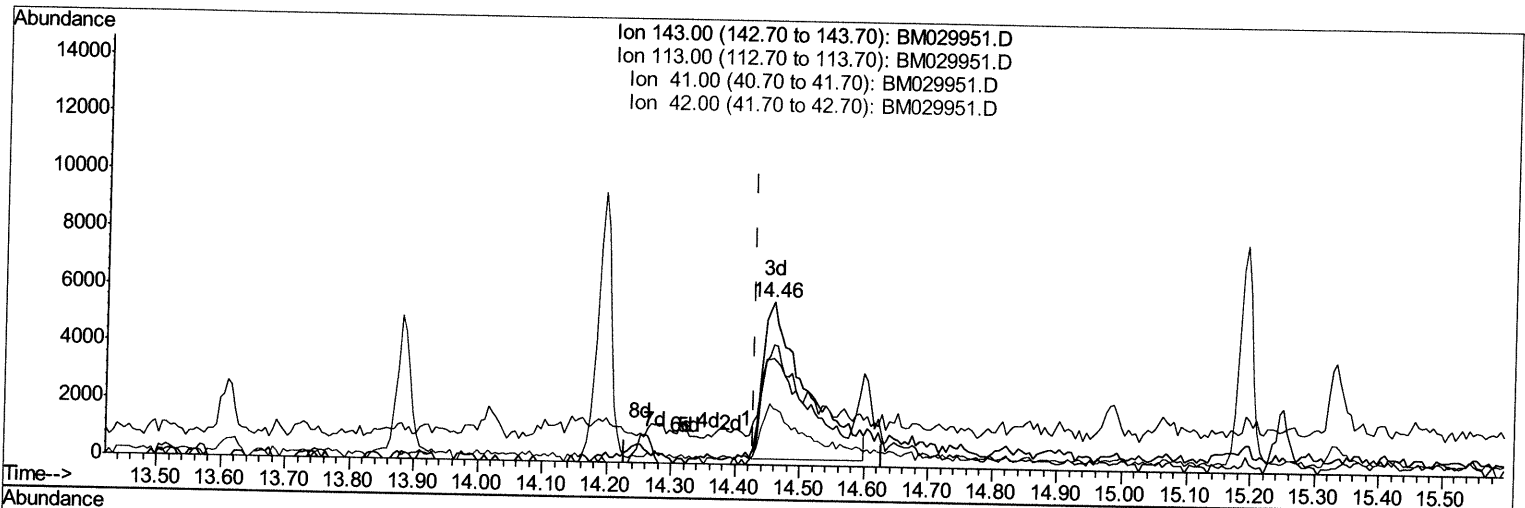

(54) 4-Nitrophenol-d4 (S)

14.457min (+0.030) 5.46ng/ul 05/13/21 JU

response 25739

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	73.98
41.00	44.70	65.31#
42.00	28.30	35.03#

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029951.D
 Acq On : 11 May 2021 20:13
 Operator : CG/JU
 Sample : M2177-21
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BG591

Manual Integrations
APPROVED

mohammad
 5/12/2021 2:06:50 PM

Quant Time: May 12 01:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

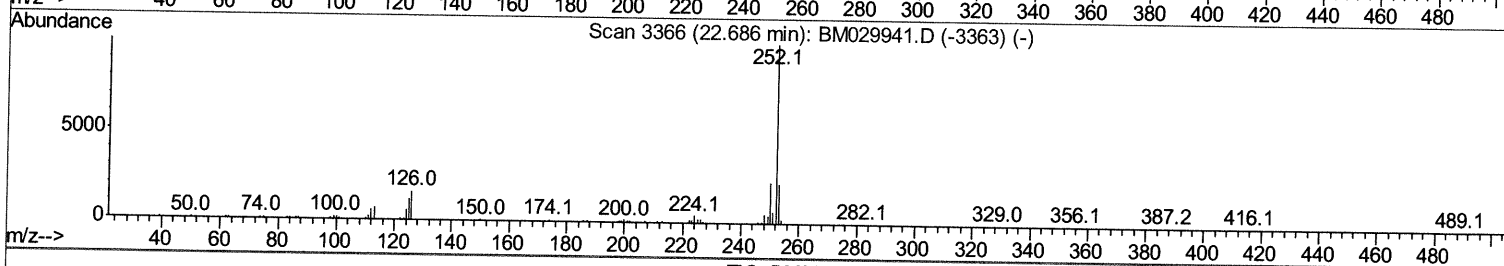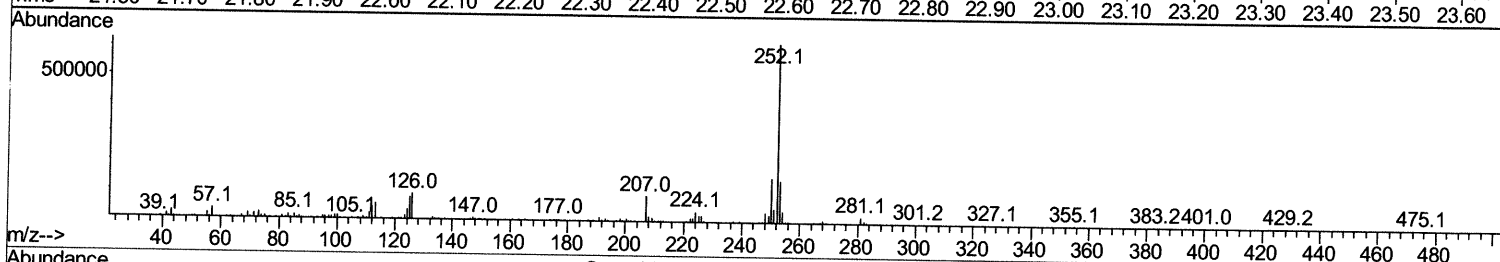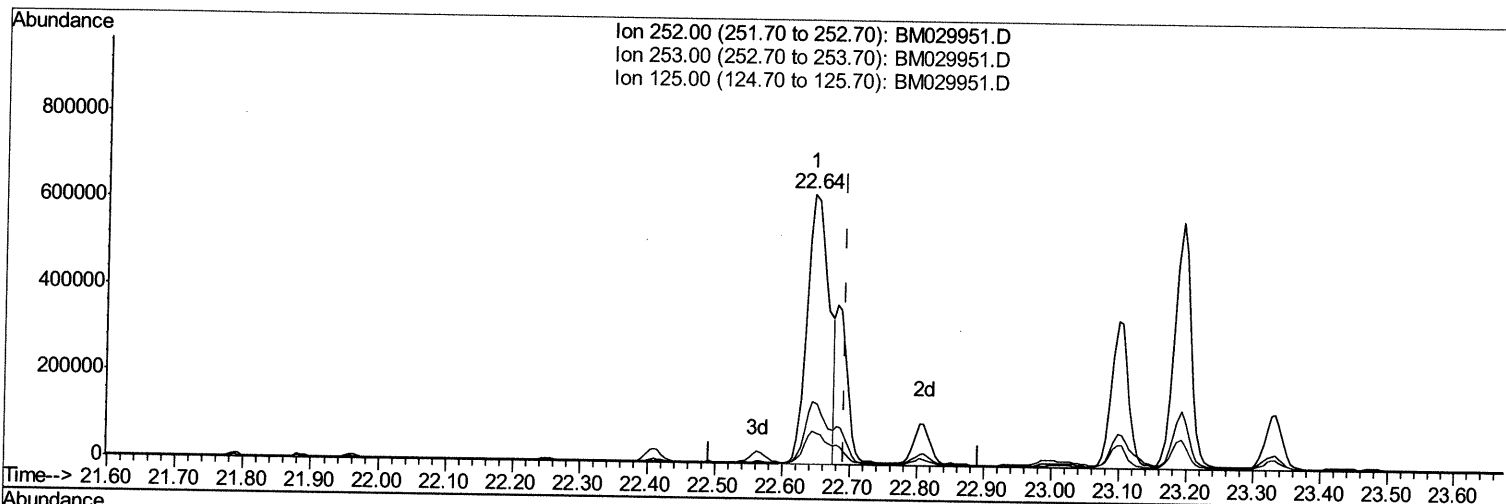

TIC: BM029951.D

(91) Benzo(k)fluoranthene

22.645min (-0.047) 29.83ng/ul

response 1386360

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.15
125.00	10.50	12.09
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029951.D
 Acq On : 11 May 2021 20:13
 Operator : CG/JU
 Sample : M2177-21
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG591

Manual Integrations
 APPROVED

mohammad
 5/12/2021 2:06:50 PM

Quant Time: May 12 01:15:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

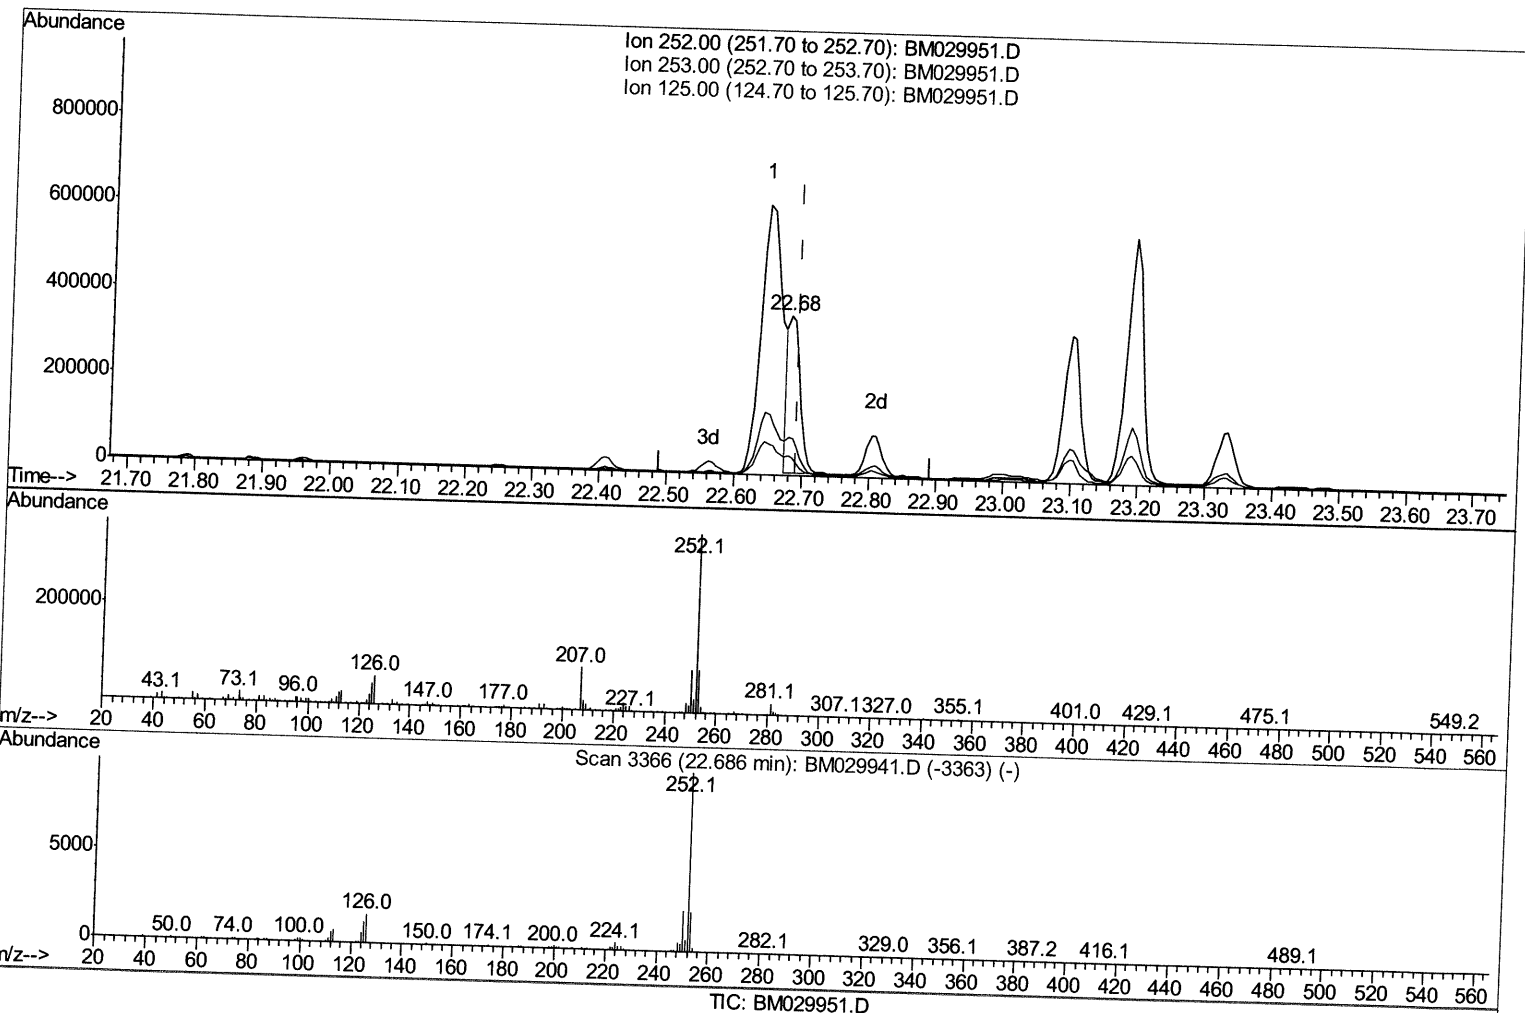

(91) Benzo(k)fluoranthene

22.680min (-0.012) 9.46ng/ul m 05/11/21 JU

response 439641

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	24.04
125.00	10.50	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029951.D
 Acq On : 11 May 2021 20:13
 Operator : CG/JU
 Sample : M2177-21
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG591

Manual Integrations
 APPROVED

mohammad
 5/12/2021 2:06:50 PM

Quant Time: May 12 01:16:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	137241	20.00	ng/ul	0.00
20) Naphthalene-d8	10.32	136	604668	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.19	164	373329	20.00	ng/ul	-0.01
64) Phenanthrene-d10	16.94	188	713549	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	662641	20.00	ng/ul	0.00
88) Perylene-d12	23.29	264	681482	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	5917	1.72	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	150157	11.77	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.89	67	103220	13.04	ng/ul	0.00
11) 2-Chlorophenol-d4	7.08	132	127856	12.98	ng/ul	0.00
15) 4-Methylphenol-d8	8.26	113	126835	12.02	ng/ul	0.00
21) Nitrobenzene-d5	8.70	128	55099	13.22	ng/ul	0.00
24) 2-Nitrophenol-d4	9.42	143	59792	12.71	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.96	165	122564	13.00	ng/ul	0.00
31) 4-Chloroaniline-d4	10.47	131	134161	9.35	ng/ul	0.00
46) Dimethylphthalate-d6	13.62	166	416522	14.39	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	517647	14.12	ng/ul	0.00
54) 4-Nitrophenol-d4	14.46	143	25739m >	5.46	ng/ul >	0.0305/13/21JU
60) Fluorene-d10	15.19	176	370676	15.09	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.33	200	37078	8.00	ng/ul	0.00
73) Anthracene-d10	17.04	188	538637	14.99	ng/ul	0.00
81) Pyrene-d10	19.34	212	577204	16.98	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.15	264	594883	15.40	ng/ul	0.00

Target Compounds

					Ovalue	
30) Naphthalene	10.37	128	199775	5.952	ng/ul	99
36) 2-Methylnaphthalene	11.99	142	79417	3.262	ng/ul	97
37) 1-Methylnaphthalene	12.22	142	75631	3.135	ng/ul	95
52) Acenaphthene	14.26	153	195584	7.803	ng/ul	99
56) Dibenzofuran	14.60	168	83358	2.428	ng/ul	96
61) Fluorene	15.25	166	137410	4.682	ng/ul	99
72) Phenanthrene	16.99	178	1805144	42.904	ng/ul	100
74) Anthracene	17.07	178	298604	6.942	ng/ul	98
77) Carbazole	17.35	167	150170	3.810	ng/ul	98
80) Fluoranthene	19.00	202	2182408	52.752	ng/ul	98
82) Pyrene	19.37	202	1935827	44.463	ng/ul	99
85) Benzo(a)anthracene	21.12	228	1032563	23.883	ng/ul	99
86) Bis(2-ethylhexyl)phthalate	21.06	149	60448	2.266	ng/ul	98
87) Chrysene	21.17	228	973133	22.599	ng/ul	98
90) Benzo(b)fluoranthene	22.64	252	1386360	31.362	ng/ul	97
91) Benzo(k)fluoranthene	22.68	252	439641m >	9.460	ng/ul >	05/13/21JU
93) Benzo(a)pyrene	23.19	252	969854	24.158	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.43	276	644187	13.257	ng/ul	95
95) Dibenzo(a,h)anthracene	25.44	278	167928	4.077	ng/ul#	92
96) Benzo(a,h,i)perylene	26.09	276	517017	13.132	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
Data File : BM029951.D
Acq On : 11 May 2021 20:13
Operator : CG/JU
Sample : M2177-21
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG591

Manual Integrations
APPROVED

mohammad
5/12/2021 2:06:50 PM

Quant Time: May 12 01:16:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 15:21:38 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						