


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029994.D
Acq On : 12 May 2021 22:49
Operator : CG/JU
Sample : M2232-06
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5A3

Manual Integrations
APPROVED

Sohil
5/13/2021 10:31:23 AM

Quant Time: May 13 02:41:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 13 01:09:15 2021
Response via : Initial Calibration

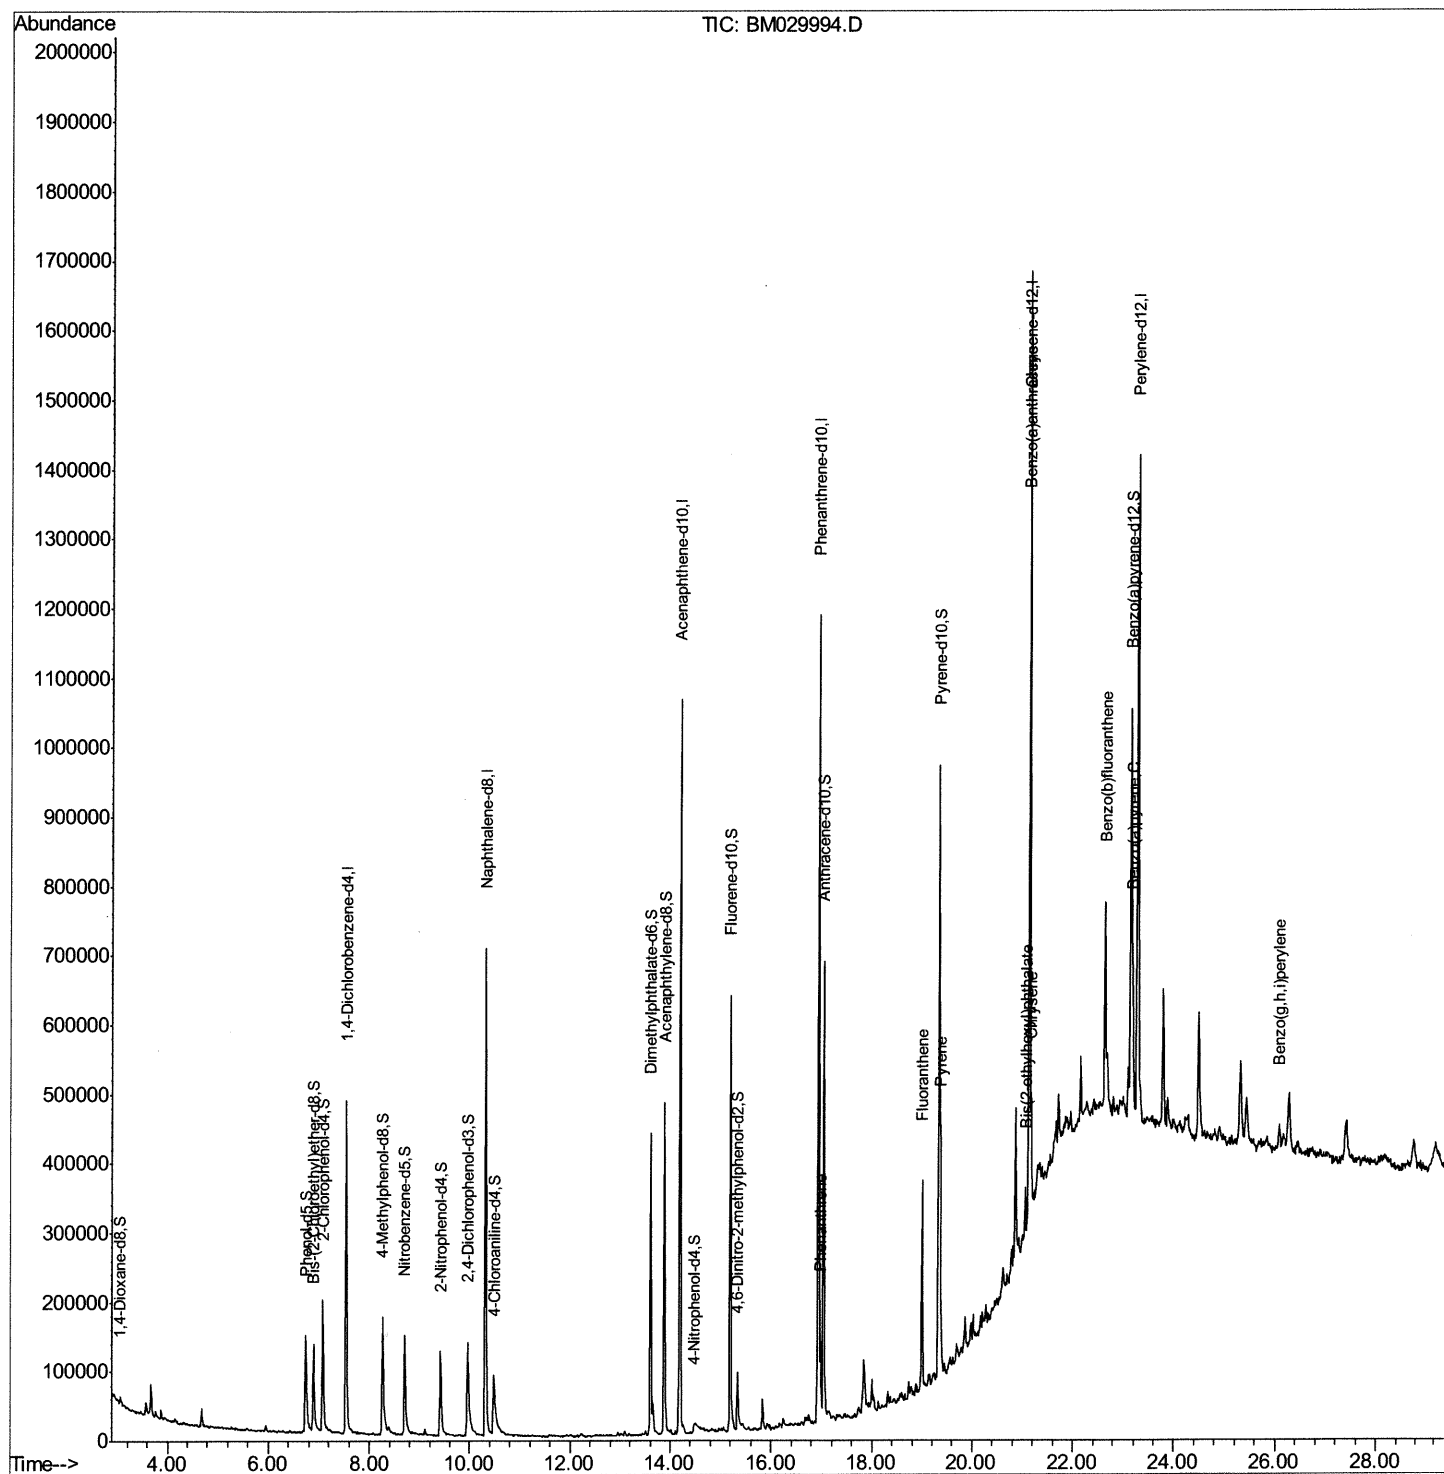




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029994.D
Acq On : 12 May 2021 22:49
Operator : CG/JU
Sample : M2232-06
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5A3

Manual Integrations
APPROVED

Sohil
5/13/2021 10:31:23 AM

Quant Time: May 13 02:38:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 13 01:09:15 2021
Response via : Initial Calibration

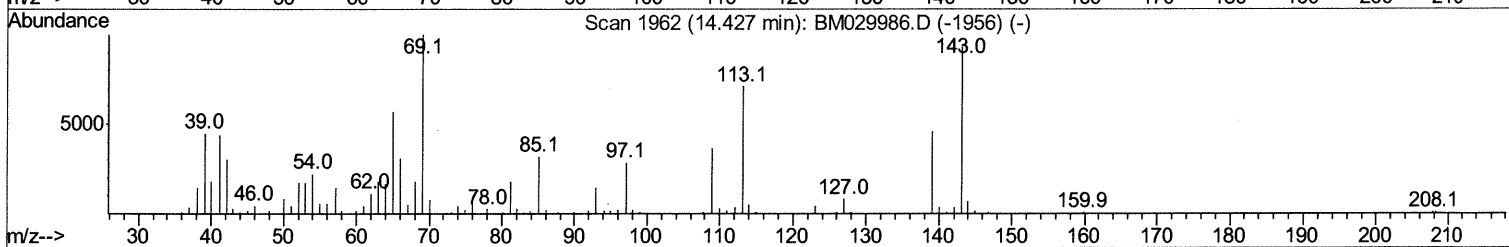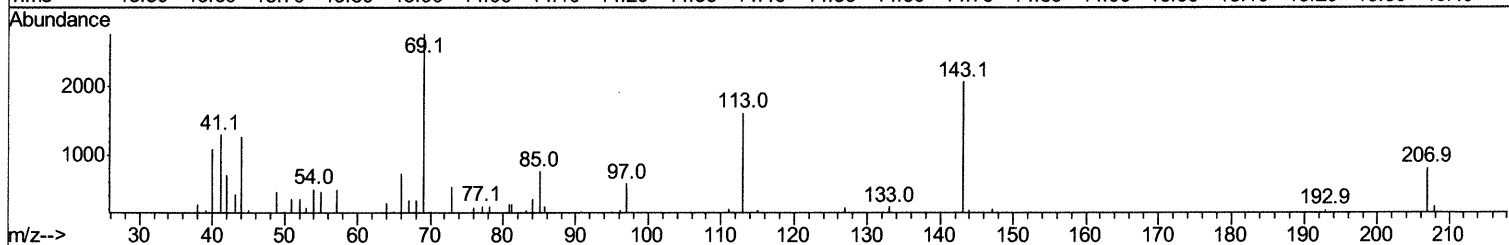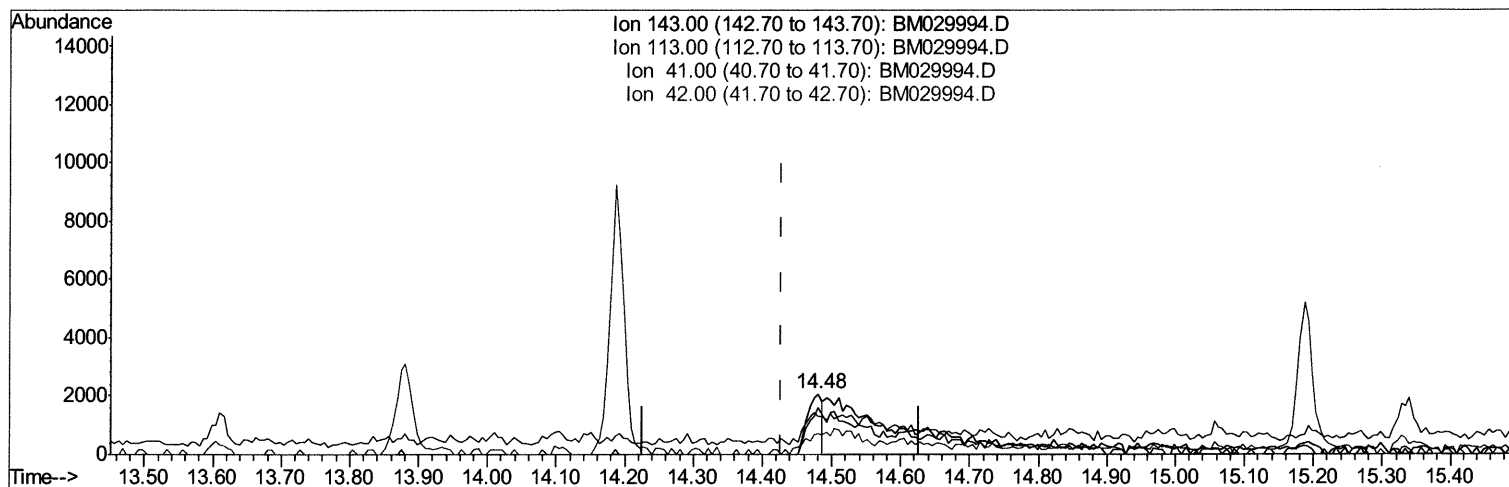

TIC: BM029994.D

(54) 4-Nitrophenol-d4 (S)

14.481min (+0.053) 0.72ng/ul

response 3247

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	77.83
41.00	44.70	62.53#
42.00	28.30	33.86

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029994.D
 Acq On : 12 May 2021 22:49
 Operator : CG/JU
 Sample : M2232-06
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG5A3

Manual Integrations
 APPROVED

Sohil
 5/13/2021 10:31:23 AM

Quant Time: May 13 02:38:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 13 01:09:15 2021
 Response via : Initial Calibration

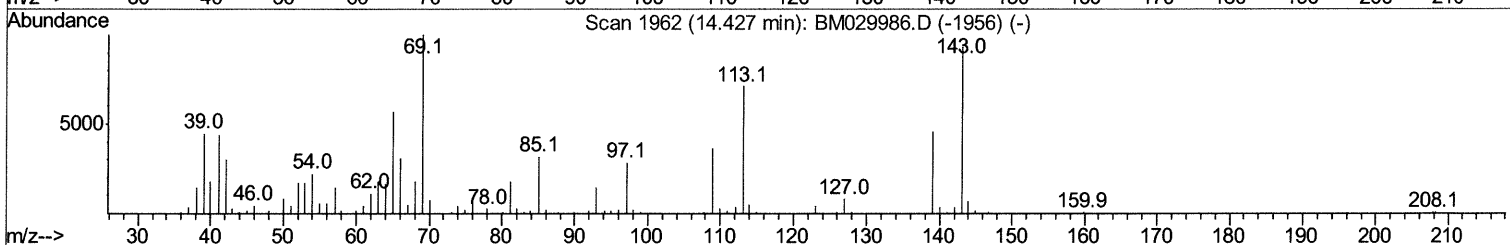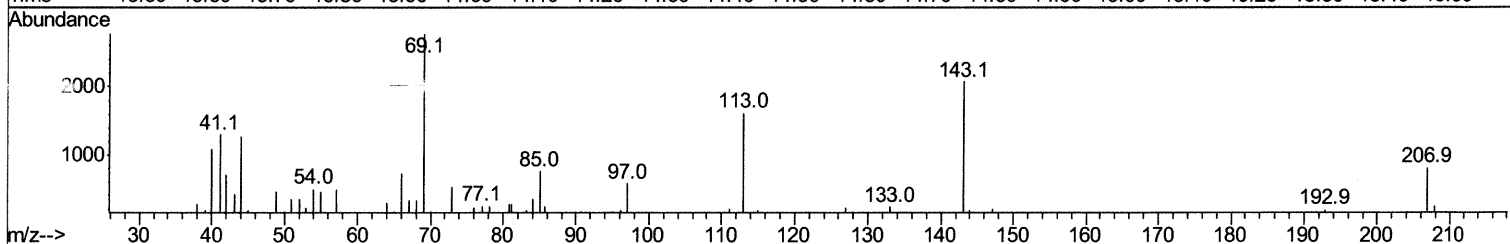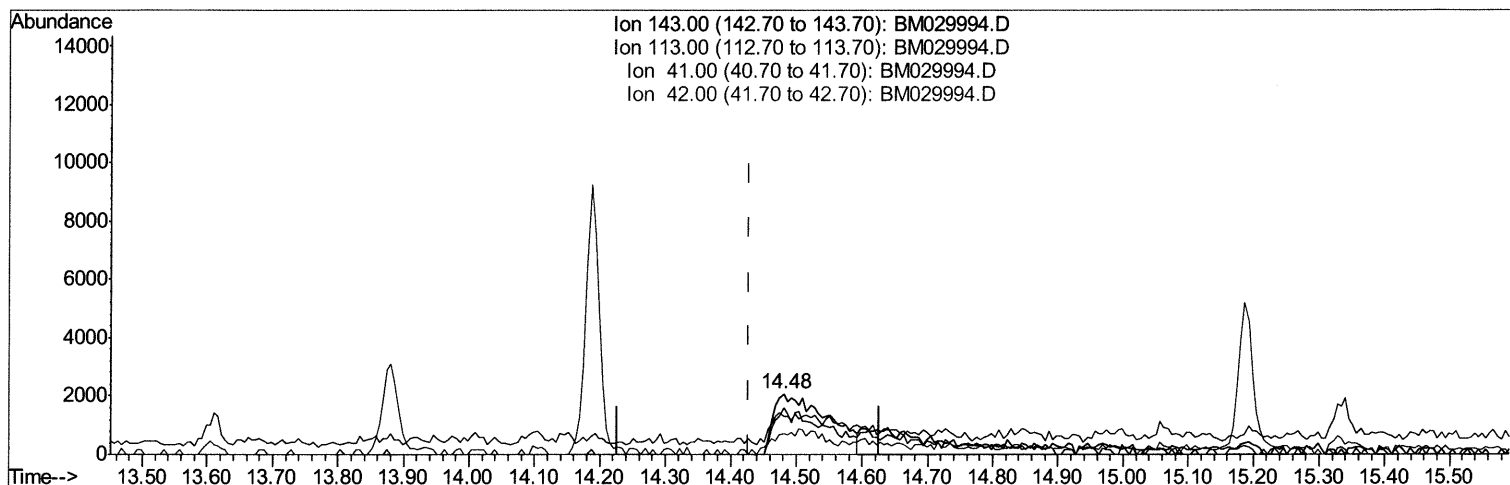

TIC: BM029994.D

(54) 4-Nitrophenol-d4 (S)

14.481min (+0.053) 2.58ng/ul m 05/13/2021

response 11727

Ion	Exp%	Act%
143.00	100	100
113.00	71.10	77.83
41.00	44.70	62.53#
42.00	28.30	33.86




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029994.D
Acq On : 12 May 2021 22:49
Operator : CG/JU
Sample : M2232-06
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5A3

Manual Integrations
APPROVED

Sohil
5/13/2021 10:31:23 AM

Quant Time: May 13 02:38:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 13 01:09:15 2021
Response via : Initial Calibration

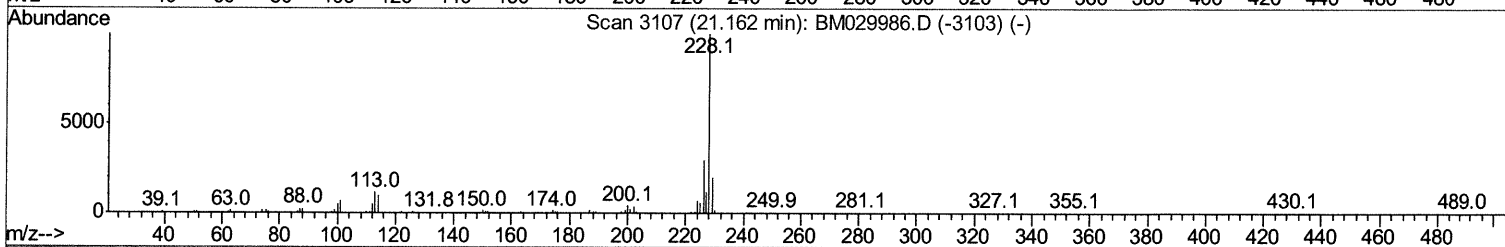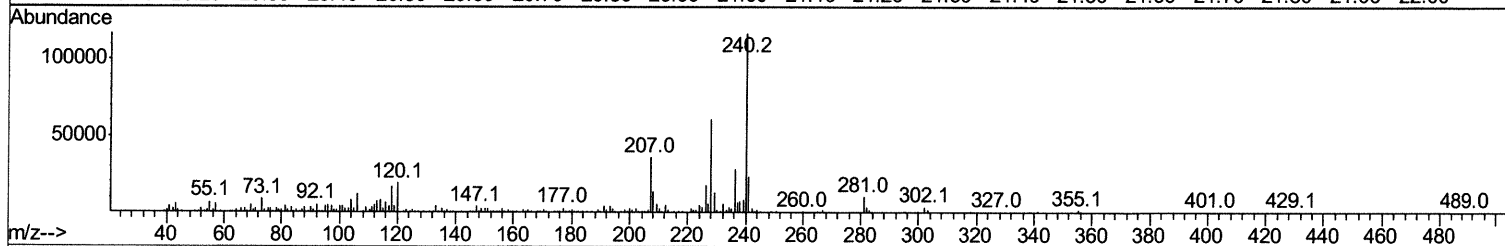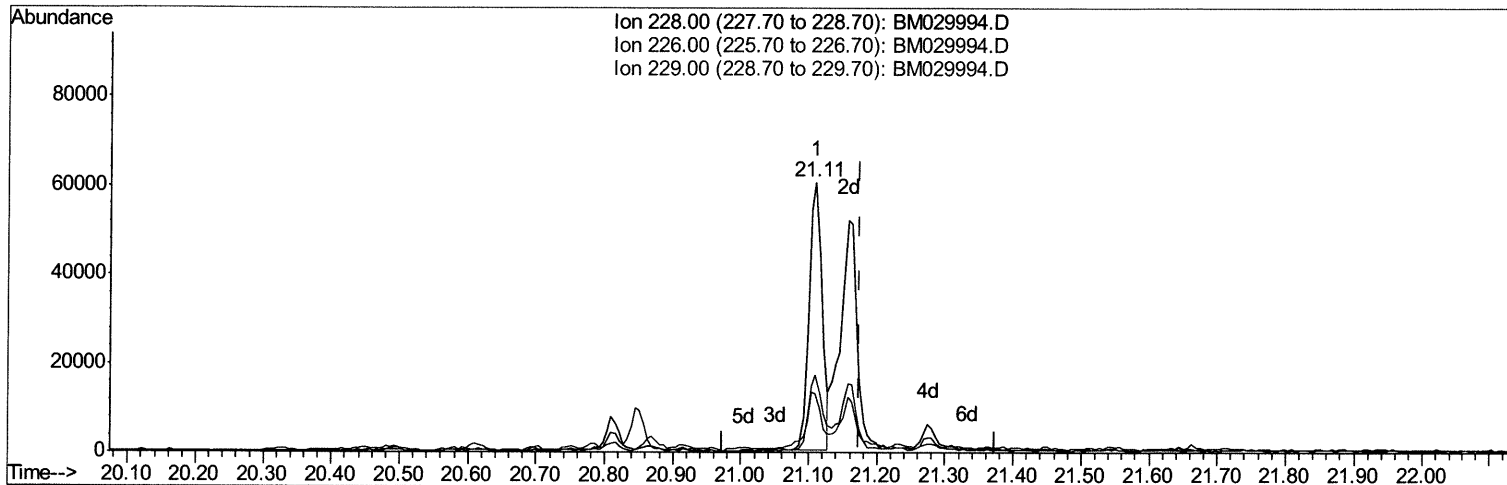

TIC: BM029994.D

(87) Chrysene

21.110min (-0.064) 2.04ng/ul

response 80283

Ion	Exp%	Act%
228.00	100	100
226.00	29.90	28.69
229.00	19.50	21.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029994.D
 Acq On : 12 May 2021 22:49
 Operator : CG/JU
 Sample : M2232-06
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG5A3

Manual Integrations
 APPROVED

Sohil
 5/13/2021 10:31:23 AM

Quant Time: May 13 02:38:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 13 01:09:15 2021
 Response via : Initial Calibration

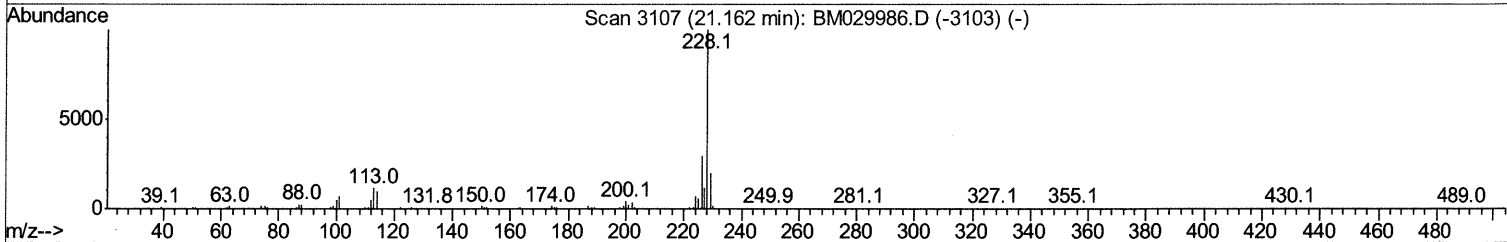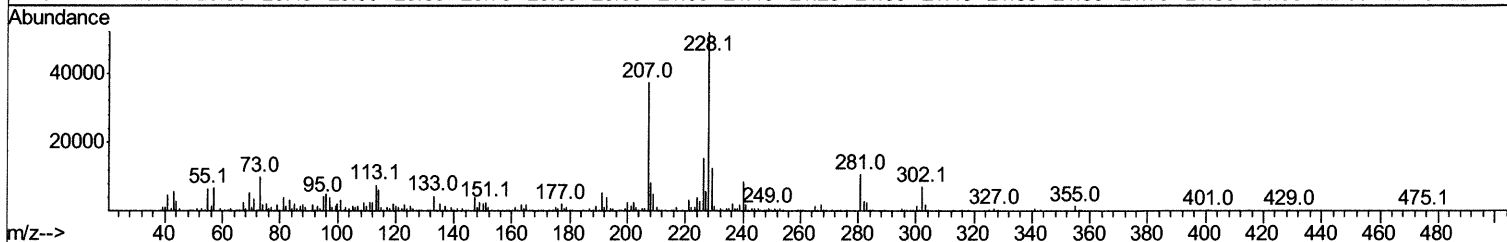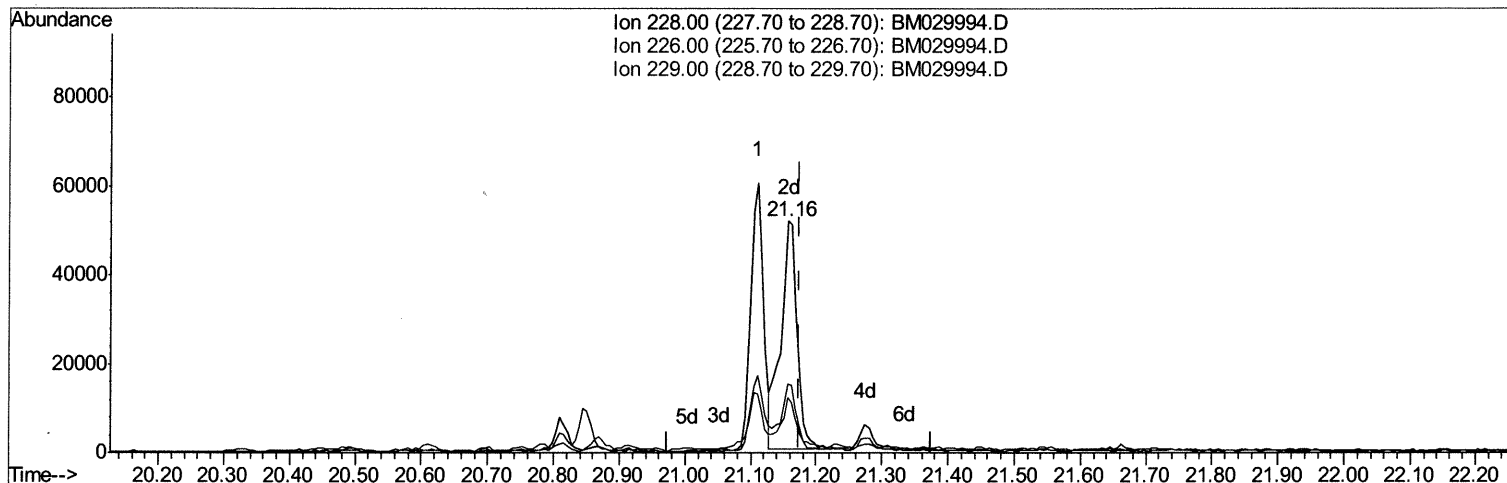

TIC: BM029994.D

(87) Chrysene

21.157min (-0.017) 2.32ng/ul m 05/13/21 JU

response 91057

Ion	Exp%	Act%
228.00	100	100
226.00	29.90	29.85
229.00	19.50	23.91#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029994.D
 Acq On : 12 May 2021 22:49
 Operator : CG/JU
 Sample : M2232-06
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG5A3

Manual Integrations
 APPROVED

Sohil
 5/13/2021 10:31:23 AM

Quant Time: May 13 02:41:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 13 01:09:15 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	137213	20.00	ng/ul	-0.01
20) Naphthalene-d8	10.32	136	583507	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.19	164	359440	20.00	ng/ul	-0.01
64) Phenanthrene-d10	16.93	188	678112	20.00	ng/ul	-0.01
79) Chrysene-d12	21.12	240	605159	20.00	ng/ul	-0.01
88) Perylene-d12	23.27	264	631644	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	6765	1.97	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	97871	7.67	ng/ul	0.00
9) Bis-(2-Chloroethyl) ether-d	6.89	67	73407	9.28	ng/ul	0.00
11) 2-Chlorophenol-d4	7.08	132	93671	9.51	ng/ul	0.00
15) 4-Methylphenol-d8	8.26	113	83439	7.91	ng/ul	0.00
21) Nitrobenzene-d5	8.70	128	40440	10.06	ng/ul	0.00
24) 2-Nitrophenol-d4	9.42	143	42432	9.35	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.96	165	75335	8.28	ng/ul	0.00
31) 4-Chloroaniline-d4	10.48	131	81653	5.90	ng/ul	0.00
46) Dimethylphthalate-d6	13.61	166	296803	10.65	ng/ul	-0.01
49) Acenaphthylene-d8	13.88	160	344605	9.76	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.48	143	11727m>	2.58	ng/ul>	0.05
60) Fluorene-d10	15.19	176	251766	10.64	ng/ul	-0.01
65) 4,6-Dinitro-2-methylphenol	15.33	200	19719	4.48	ng/ul	0.00
73) Anthracene-d10	17.03	188	386384	11.32	ng/ul	-0.01
81) Pyrene-d10	19.33	212	414399	13.35	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.14	264	389871	10.89	ng/ul	-0.01

Target Compounds

					Ovalue	
72) Phenanthrene	16.98	178	70142	1.754	ng/ul	99
80) Fluoranthene	19.00	202	172677	4.570	ng/ul	96
82) Pvrene	19.36	202	180229	4.533	ng/ul	97
85) Benzo(a)anthracene	21.11	228	80283	2.033	ng/ul	96
86) Bis(2-ethylhexyl)phthalate	21.05	149	24483	1.005	ng/ul	98
87) Chrysene	21.16	228	91057m>	2.316	ng/ul>	95
90) Benzo(b)fluoranthene	22.64	252	107621	2.627	ng/ul#	94
93) Benzo(a)pvrene	23.18	252	71155	1.912	ng/ul#	92
96) Benzo(a,h,i)perylene	26.07	276	39168	1.073	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed