

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029917.D
 Acq On : 10 May 2021 22:35
 Operator : CG/JU
 Sample : M2177-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG515

Manual Integrations
 APPROVED

mohammad
 5/11/2021 2:33:06 PM

Quant Time: May 11 02:26:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 01:19:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	149201	20.00	ng/ul	0.00
20) Naphthalene-d8	10.33	136	689483	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.20	164	464822	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.95	188	940238	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	814820	20.00	ng/ul	0.00
88) Perylene-d12	23.29	264	698754	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	5166	1.38	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.75	99	76539	5.52	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.90	67	52090	6.05	ng/ul	0.00
11) 2-Chlorophenol-d4	7.09	132	71116	6.64	ng/ul	0.00
15) 4-Methylphenol-d8	8.28	113	66035	5.75	ng/ul	0.00
21) Nitrobenzene-d5	8.71	128	33717	7.10	ng/ul	0.00
24) 2-Nitrophenol-d4	9.43	143	33385	6.23	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	60303	5.61	ng/ul	0.01
31) 4-Chloroaniline-d4	10.49	131	74511	4.55	ng/ul	0.01
46) Dimethylphthalate-d6	13.62	166	276222	7.67	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	327087	7.16	ng/ul	0.00
54) 4-Nitrophenol-d4	14.48	143	9379m	1.60	ng/ul	0.05
60) Fluorene-d10	15.20	176	243023	7.95	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	12919	2.12	ng/ul	0.00
73) Anthracene-d10	17.05	188	357388	7.55	ng/ul	0.00
81) Pyrene-d10	19.34	212	409512	9.80	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.15	264	309634	7.82	ng/ul	0.00

Target Compounds

					Ovalue
86) Bis(2-ethylhexyl)phthalate	21.06	149	58141	1.772	ng/ul 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029917.D
Acq On : 10 May 2021 22:35
Operator : CG/JU
Sample : M2177-09
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG515

Manual Integrations
APPROVED

mohammad
5/11/2021 2:33:06 PM

Quant Time: May 11 02:26:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 01:19:00 2021
Response via : Initial Calibration

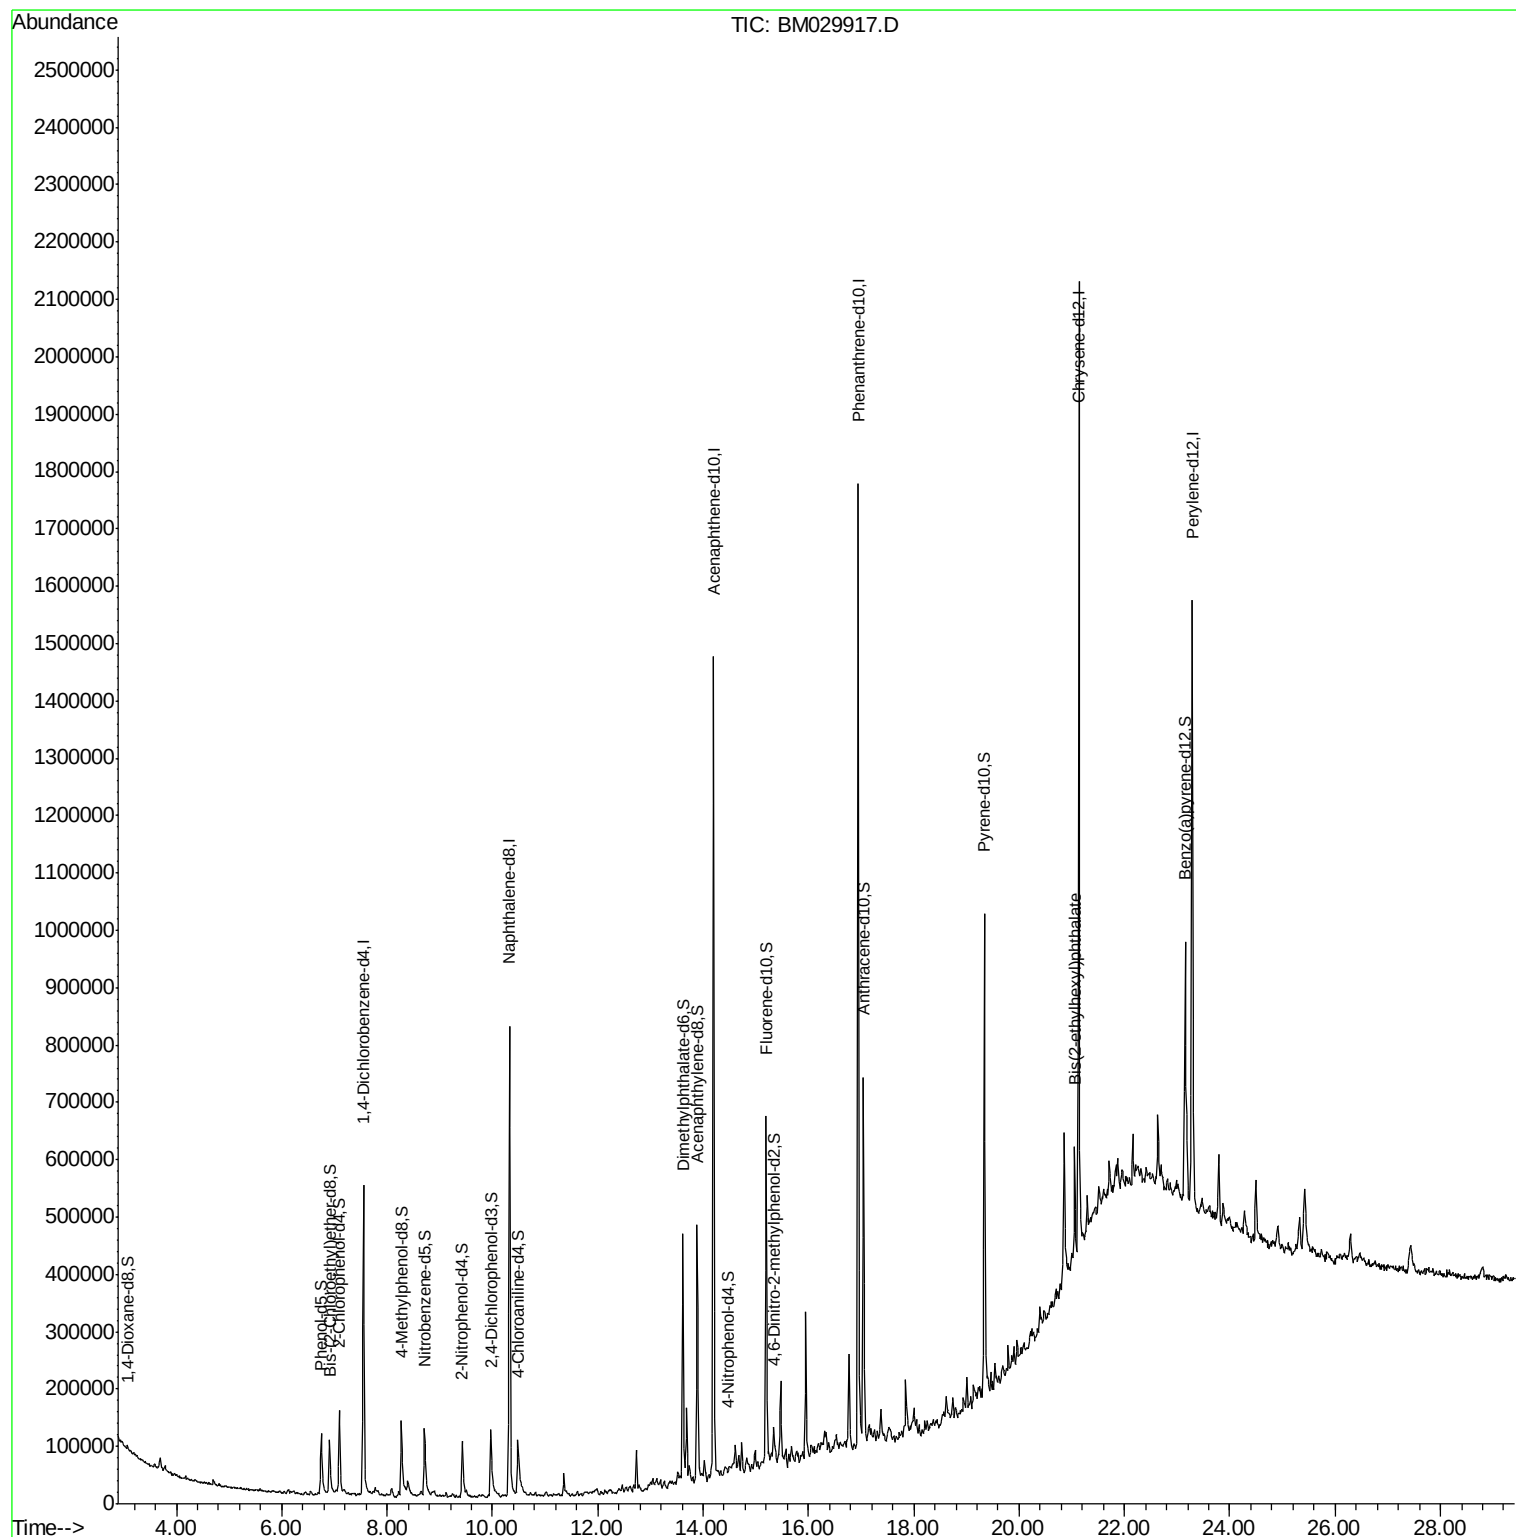

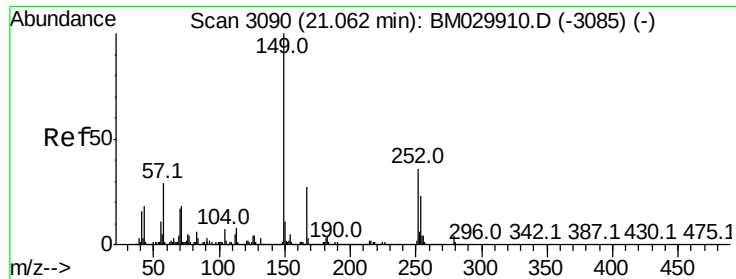

#86

Bis(2-ethylhexyl)phthalate

Concen: 1.772 ng/ul

RT: 21.06 min Scan# 3089

Delta R.T. -0.01 min

Lab File: BM029917.D


Acq: 10 May 2021 22:35

Instrument :

BNA_M

ClientSampleId :

BG515

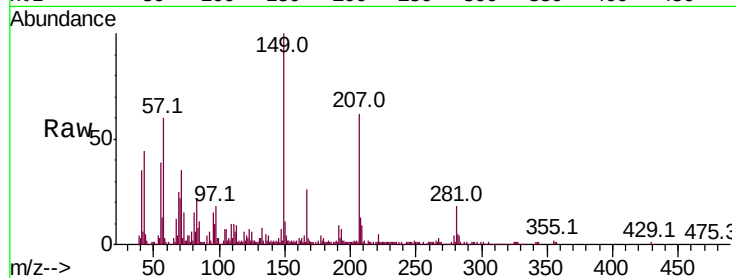

Tot Ion:	149	Resp:	58141
Ion Ratio	Lower	Upper	
149	100		
167	26.2	21.1	31.7
279	4.3	3.5	5.3

Manual Integrations
APPROVED

mohammad
5/11/2021 2:33:06 PM

