

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029924.D
 Acq On : 11 May 2021 02:48
 Operator : CG/JU
 Sample : M2177-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG576

Manual Integrations
 APPROVED

mohammad
 5/11/2021 2:33:29 PM

Quant Time: May 11 03:29:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 01:19:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	141622	20.00	ng/ul	0.00
20) Naphthalene-d8	10.33	136	655509	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.20	164	442183	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.94	188	889813	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	787820	20.00	ng/ul	0.00
88) Perylene-d12	23.28	264	671159	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	6336	1.79	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.75	99	92018	6.99	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.90	67	65962	8.08	ng/ul	0.00
11) 2-Chlorophenol-d4	7.09	132	84422	8.31	ng/ul	0.00
15) 4-Methylphenol-d8	8.27	113	72871	6.69	ng/ul	0.00
21) Nitrobenzene-d5	8.71	128	39925	8.84	ng/ul	0.00
24) 2-Nitrophenol-d4	9.43	143	41362	8.11	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	67758	6.63	ng/ul	0.01
31) 4-Chloroaniline-d4	10.49	131	87620	5.63	ng/ul	0.01
46) Dimethylphthalate-d6	13.62	166	311776	9.10	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	364452	8.39	ng/ul	0.00
54) 4-Nitrophenol-d4	14.49	143	11382m	2.04	ng/ul	0.06
60) Fluorene-d10	15.20	176	266448	9.16	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	14382	2.49	ng/ul	0.00
73) Anthracene-d10	17.04	188	392618	8.76	ng/ul	0.00
81) Pyrene-d10	19.34	212	439940	10.89	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.14	264	333396	8.76	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phthalate	21.06	149	33533	1.057	ng/ul	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029924.D
Acq On : 11 May 2021 02:48
Operator : CG/JU
Sample : M2177-10
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG576

Manual Integrations
APPROVED

mohammad
5/11/2021 2:33:29 PM

Quant Time: May 11 03:29:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 01:19:00 2021
Response via : Initial Calibration

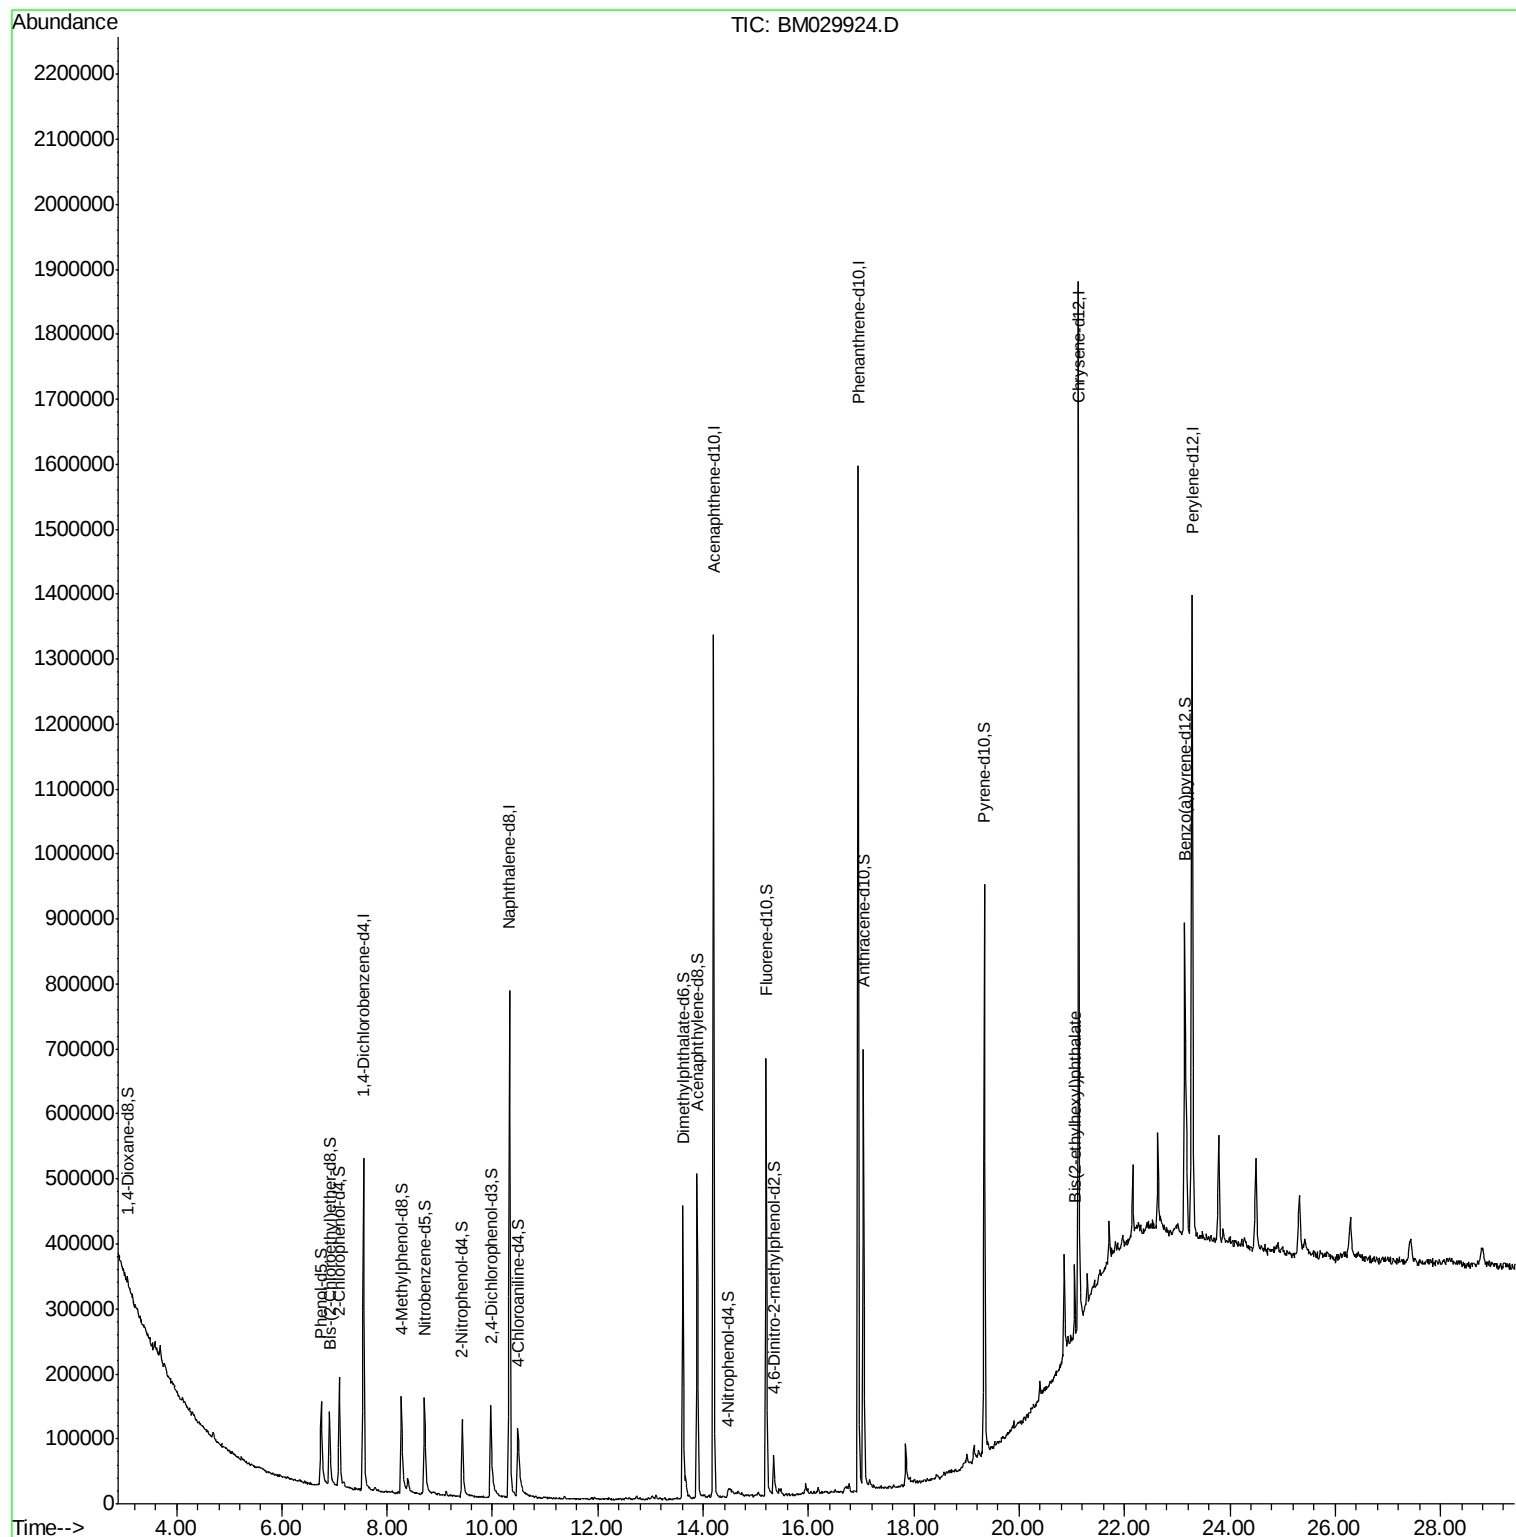

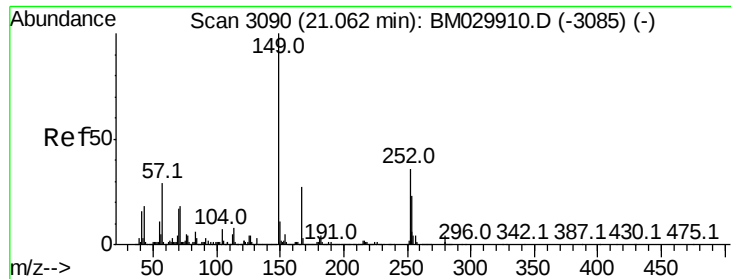

#86

Bis(2-ethylhexyl)phthalate

Concen: 1.057 ng/ul

RT: 21.06 min Scan# 3089

Delta R.T. -0.01 min

Lab File: BM029924.D

Acq: 11 May 2021 02:48

Instrument :

BNA_M

ClientSampleId :

BG576

Tot Ion:149 Resp: 33533

Ion Ratio Lower Upper

149 100

167 24.2 21.1 31.7

279 4.7 3.5 5.3

Manual Integrations

APPROVED

mohammad

5/11/2021 2:33:29 PM

