

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029934.D
 Acq On : 11 May 2021 09:23
 Operator : CG/JU
 Sample : M2197-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARF9

Quant Time: May 11 10:40:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 06:44:51 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	145335	20.00	ng/ul	0.00
20) Naphthalene-d8	10.32	136	642836	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.20	164	408827	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.95	188	826026	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	743473	20.00	ng/ul	0.00
88) Perylene-d12	23.29	264	652338	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	10285	2.83	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	6.74	99	84712	6.27	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.90	67	224214	26.75	ng/ul	0.00
11) 2-Chlorophenol-d4	7.09	132	238672	22.88	ng/ul	0.00
15) 4-Methylphenol-d8	8.26	113	149820	13.40	ng/ul	0.00
21) Nitrobenzene-d5	8.70	128	128771	29.07	ng/ul	0.00
24) 2-Nitrophenol-d4	9.42	143	141367	28.27	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.96	165	239304	23.87	ng/ul	0.00
31) 4-Chloroaniline-d4	10.49	131	24013	1.57	ng/ul	0.01
46) Dimethylphthalate-d6	13.62	166	1024935	32.34	ng/ul	0.00
49) Acenaphthylene-d8	13.89	160	1192835	29.70	ng/ul	0.00
54) 4-Nitrophenol-d4	14.45	143	12424	2.41	ng/ul	0.02
60) Fluorene-d10	15.19	176	867897	32.26	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.33	200	136577	25.46	ng/ul	0.00
73) Anthracene-d10	17.05	188	1570662	37.76	ng/ul	0.00
81) Pyrene-d10	19.34	212	1809175	47.44	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.15	264	1429072	38.65	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.66	163	41959	1.322	ng/ul	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029934.D
Acq On : 11 May 2021 09:23
Operator : CG/JU
Sample : M2197-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARF9

Quant Time: May 11 10:40:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 06:44:51 2021
Response via : Initial Calibration

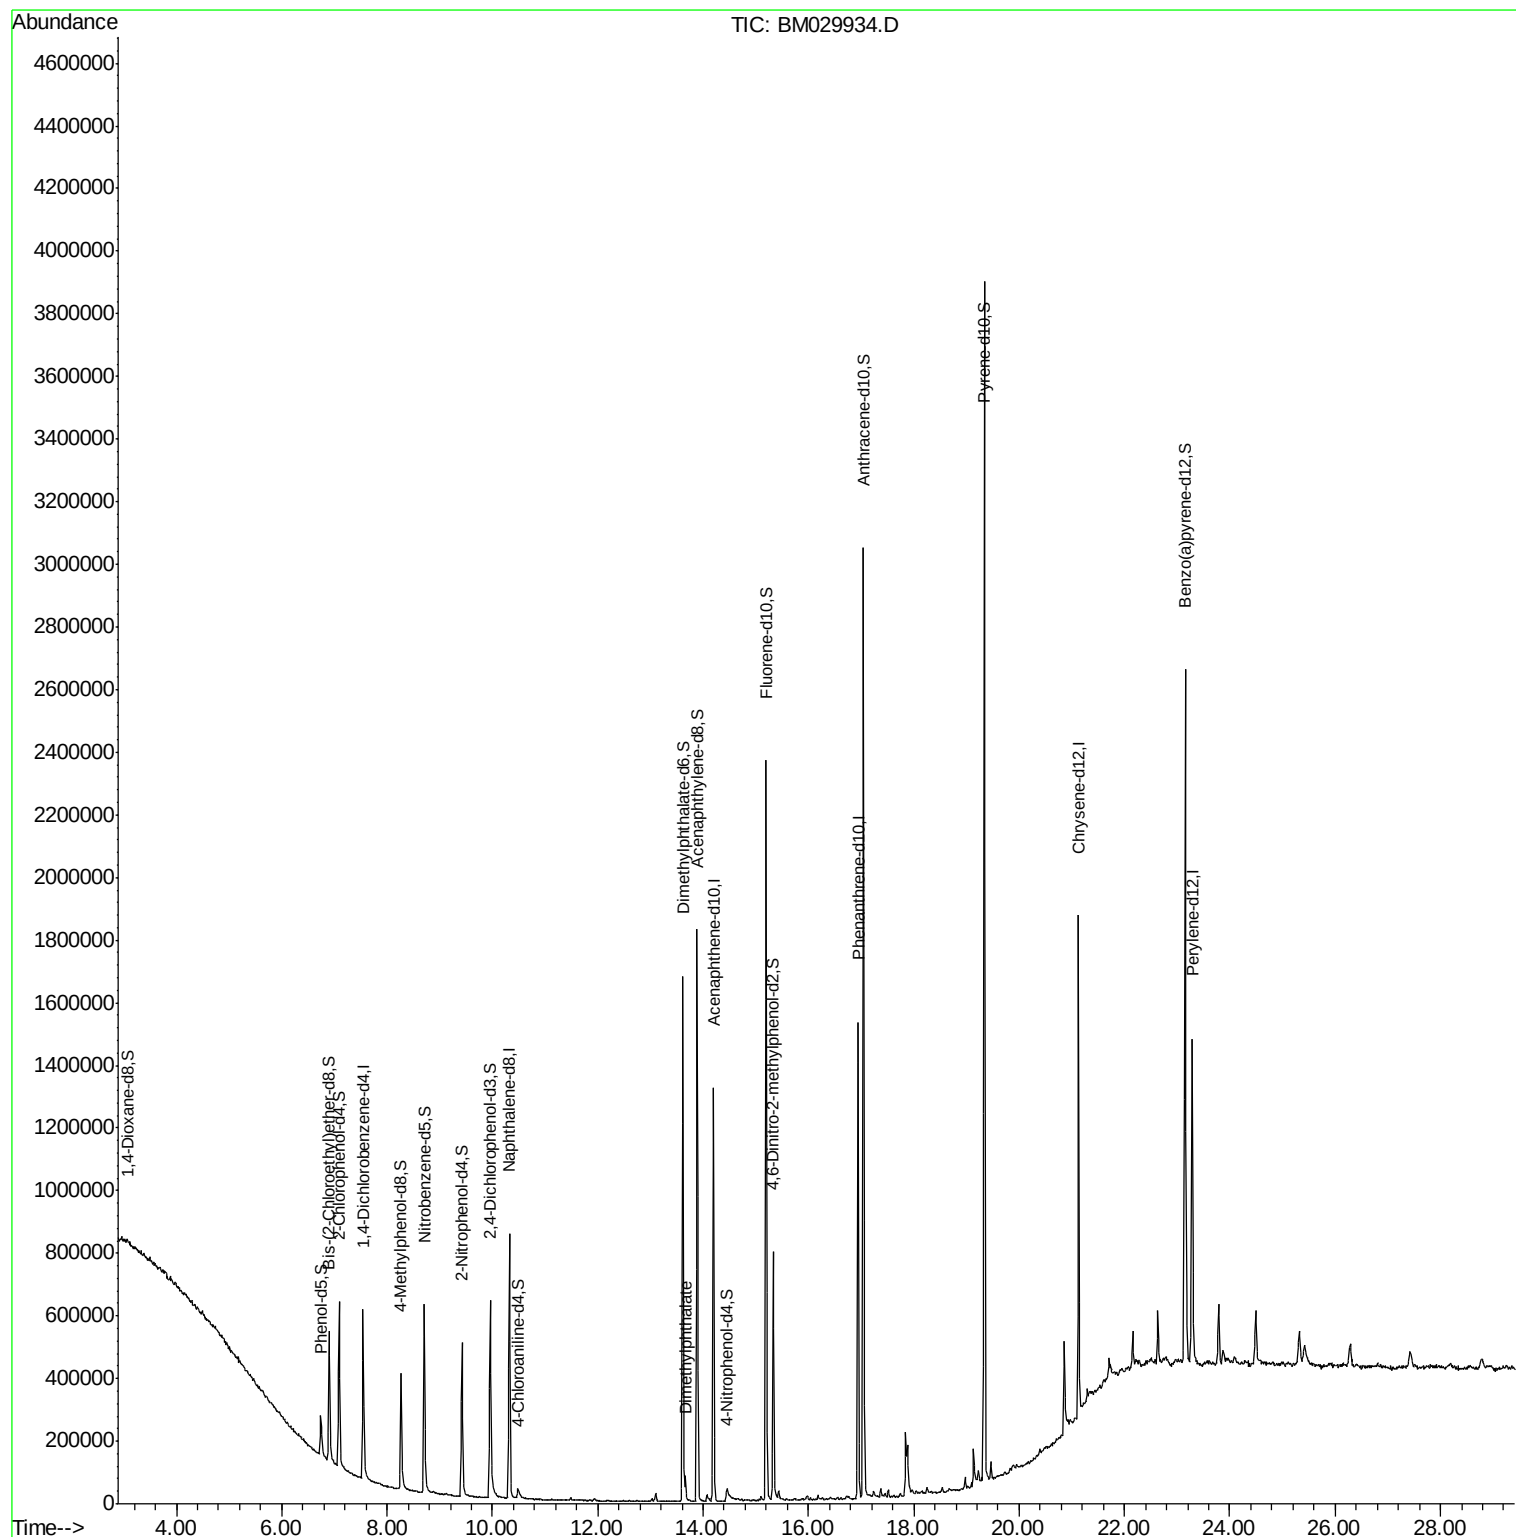

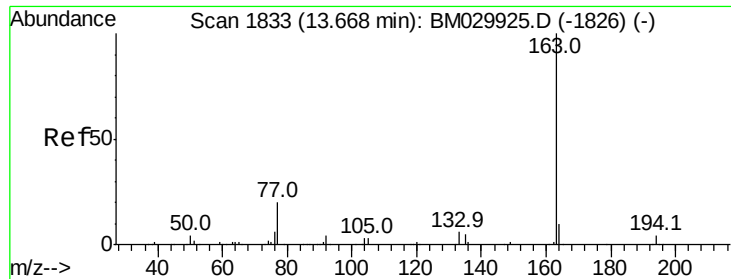

#47

Dimethylphthalate

Concen: 1.322 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM029934.D

Acq: 11 May 2021 09:23

Instrument :

BNA_M

ClientSampleId :

YARF9


Tot Ion:163 Resp: 41959

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.9 7.8 11.8

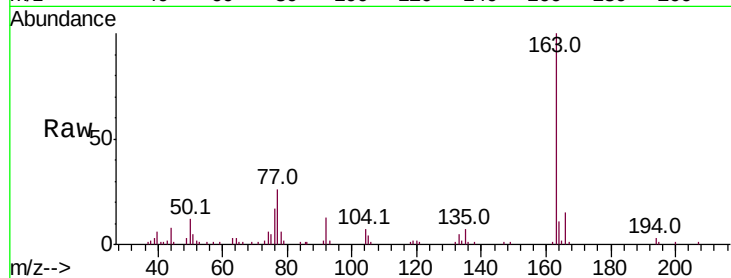

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

