

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029980.D
 Acq On : 12 May 2021 14:21
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Manual Integrations
 APPROVED

Sohil
 5/13/2021 10:30:39 AM

Quant Time: May 12 14:59:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 11 15:21:38 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	132532	20.00	ng/ul	0.00
20) Naphthalene-d8	10.32	136	568405	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.19	164	366355	20.00	ng/ul	-0.01
64) Phenanthrene-d10	16.94	188	706760	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	611375	20.00	ng/ul	0.00
88) Perylene-d12	23.28	264	608081	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	5938	1.79	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	113638	9.22	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.89	67	72049	9.43	ng/ul	0.00
11) 2-Chlorophenol-d4	7.08	132	95286	10.02	ng/ul	0.00
15) 4-Methylphenol-d8	8.27	113	89733	8.80	ng/ul	0.00
21) Nitrobenzene-d5	8.70	128	41553	10.61	ng/ul	0.00
24) 2-Nitrophenol-d4	9.42	143	45442	10.28	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.96	165	80054	9.03	ng/ul	0.00
31) 4-Chloroaniline-d4	10.48	131	95746	7.10	ng/ul	0.00
46) Dimethylphthalate-d6	13.61	166	337141	11.87	ng/ul	-0.01
49) Acenaphthylene-d8	13.88	160	396701	11.02	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.47	143	21434m	4.63	ng/ul	0.04
60) Fluorene-d10	15.19	176	296404	12.30	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.33	200	25122	5.47	ng/ul	0.00
73) Anthracene-d10	17.04	188	426478	11.98	ng/ul	0.00
81) Pyrene-d10	19.33	212	463255	14.77	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.14	264	444226	12.89	ng/ul	-0.01
Target Compounds						
82) Pvrene	19.36	202	41818	1.041	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029980.D
Acq On : 12 May 2021 14:21
Operator : CG/JU
Sample : M2177-03
Misc :
ALS Vial : 79 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG580

Manual Integrations
APPROVED

Sohil
5/13/2021 10:30:39 AM

Quant Time: May 12 14:59:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 11 15:21:38 2021
Response via : Initial Calibration

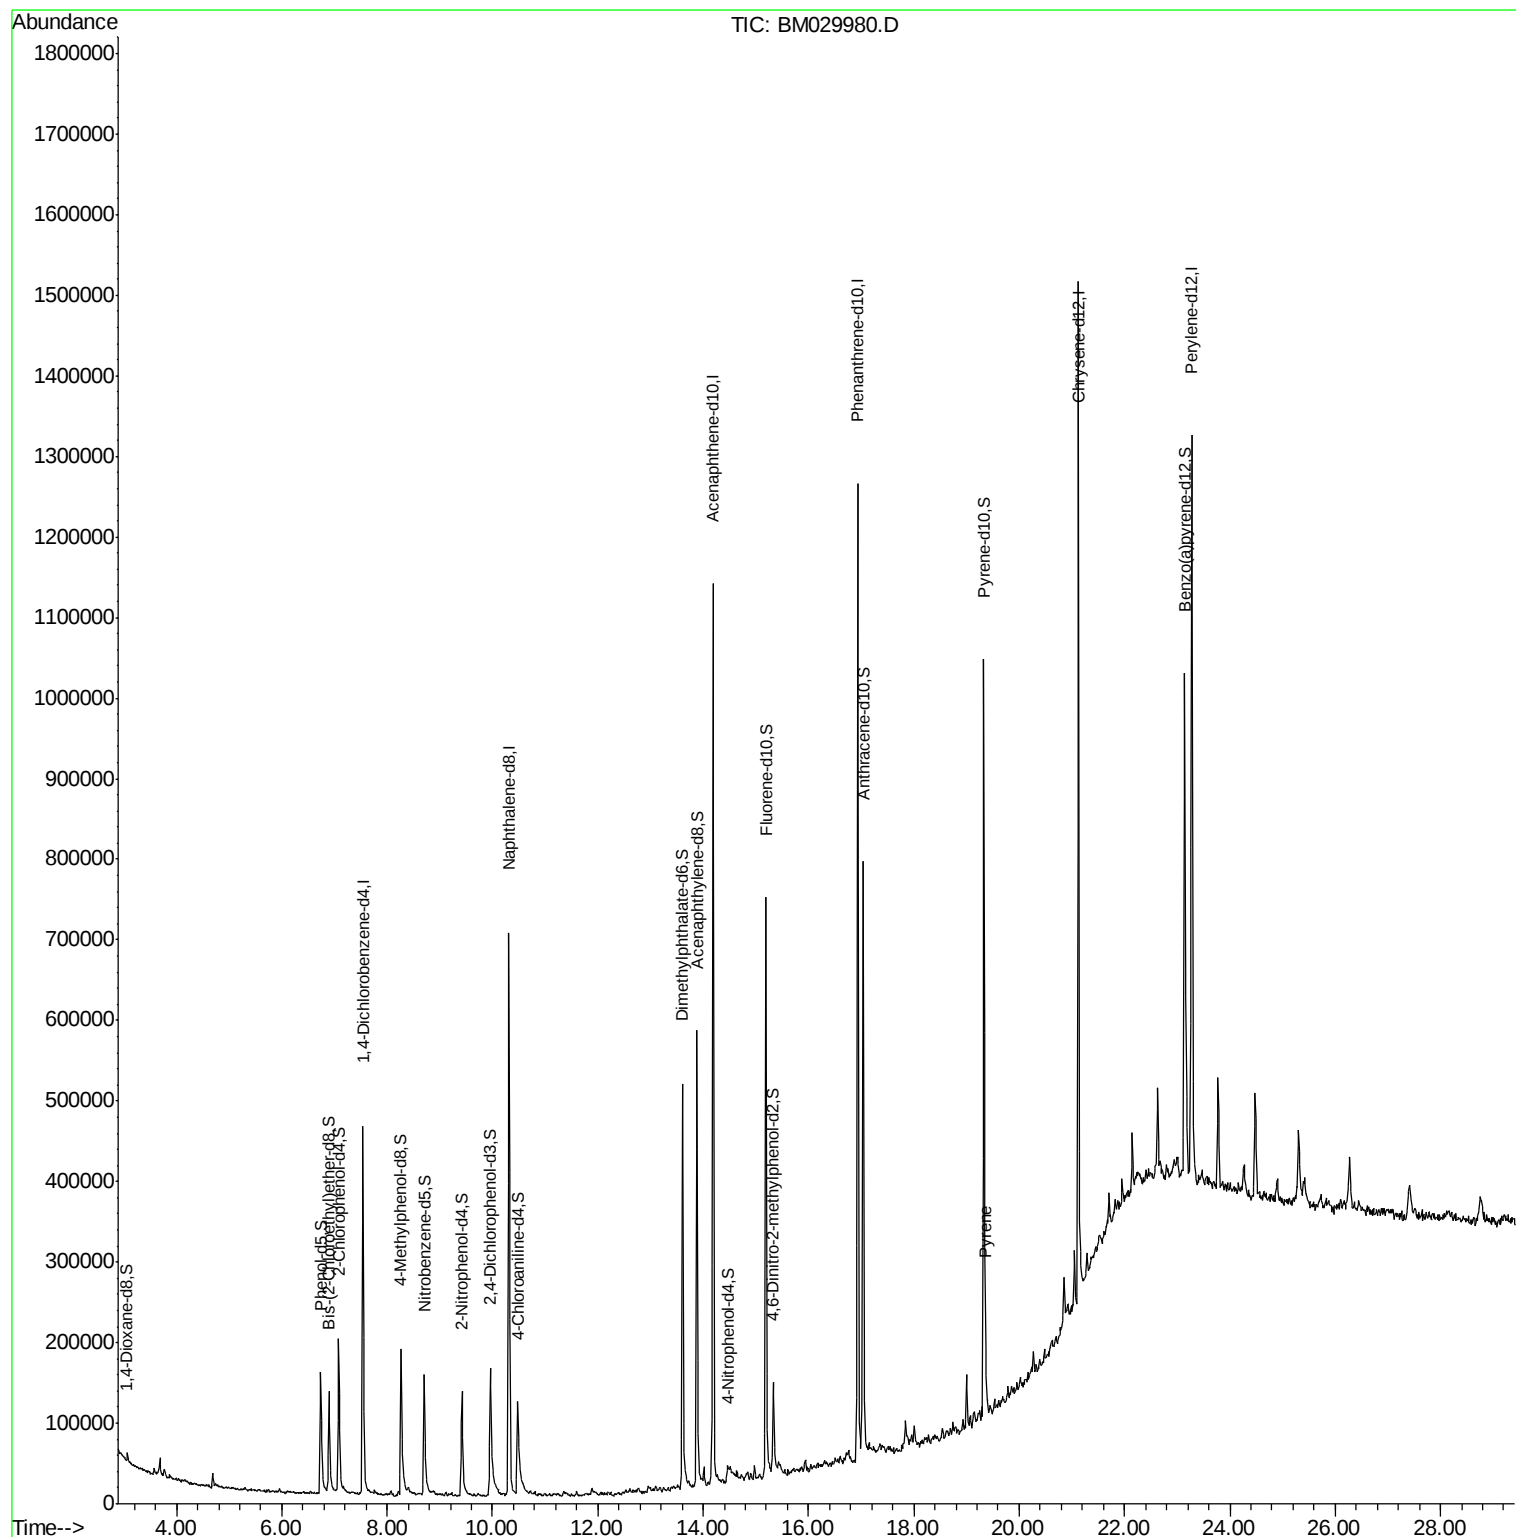

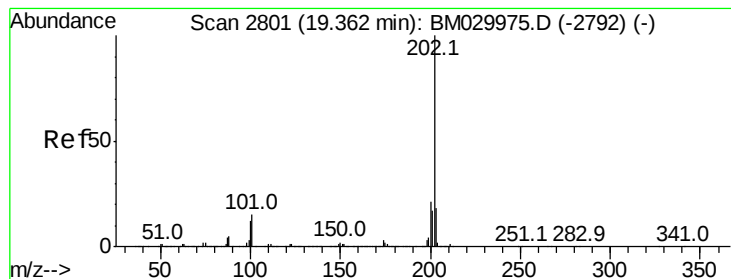

#82

Pvrene

Concen: 1.041 ng/ul

RT: 19.36 min Scan# 2801

Delta R.T. -0.01 min

Lab File: BM029980.D

Acq: 12 May 2021 14:21

Instrument :

BNA_M

ClientSampleId :

BG580

Tot Ion:	202	Resp:	41818
Ion Ratio	Lower	Upper	
202	100		
101	16.0	11.8	17.6
100	13.0	9.2	13.8

Manual Integrations
APPROVED

Sohil
5/13/2021 10:30:39 AM

