

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
 Data File : BM030009.D
 Acq On : 13 May 2021 13:45
 Operator : CG/JU
 Sample : M2377-02
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y8

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:49:54 PM

Quant Time: May 13 15:01:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 13 14:02:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	125813	20.00	ng/ul	0.00
20) Naphthalene-d8	10.31	136	569654	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.19	164	374207	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.93	188	712411	20.00	ng/ul	0.00
79) Chrysene-d12	21.13	240	516022	20.00	ng/ul	0.00
88) Perylene-d12	23.27	264	502673	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.07	96	4237	1.34	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	69393	5.93	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.89	67	238972	32.94	ng/ul	0.00
11) 2-Chlorophenol-d4	7.07	132	242069	26.81	ng/ul	0.00
15) 4-Methylphenol-d8	8.26	113	148018	15.30	ng/ul	0.00
21) Nitrobenzene-d5	8.70	128	146771	37.39	ng/ul	0.00
24) 2-Nitrophenol-d4	9.41	143	168674	38.07	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.95	165	263039	29.61	ng/ul	0.00
31) 4-Chloroaniline-d4	10.52	131	9736	0.72	ng/ul	0.05
46) Dimethylphthalate-d6	13.61	166	1103096	38.03	ng/ul	0.00
49) Acenaphthylene-d8	13.88	160	1350381	36.74	ng/ul	0.00
54) 4-Nitrophenol-d4	14.48	143	11484m	2.43	ng/ul	0.06
60) Fluorene-d10	15.19	176	950234	38.59	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.33	200	145533	31.45	ng/ul	0.00
73) Anthracene-d10	17.03	188	1437717	40.08	ng/ul	0.00
81) Pyrene-d10	19.33	212	1388660	52.46	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.14	264	1158067	40.64	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.66	163	32030	1.103	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030009.D
Acq On : 13 May 2021 13:45
Operator : CG/JU
Sample : M2377-02
Misc :
ALS Vial : 109 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG1Y8

Manual Integrations
APPROVED

mohammad
5/14/2021 12:49:54 PM

Quant Time: May 13 15:01:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 13 14:02:26 2021
Response via : Initial Calibration

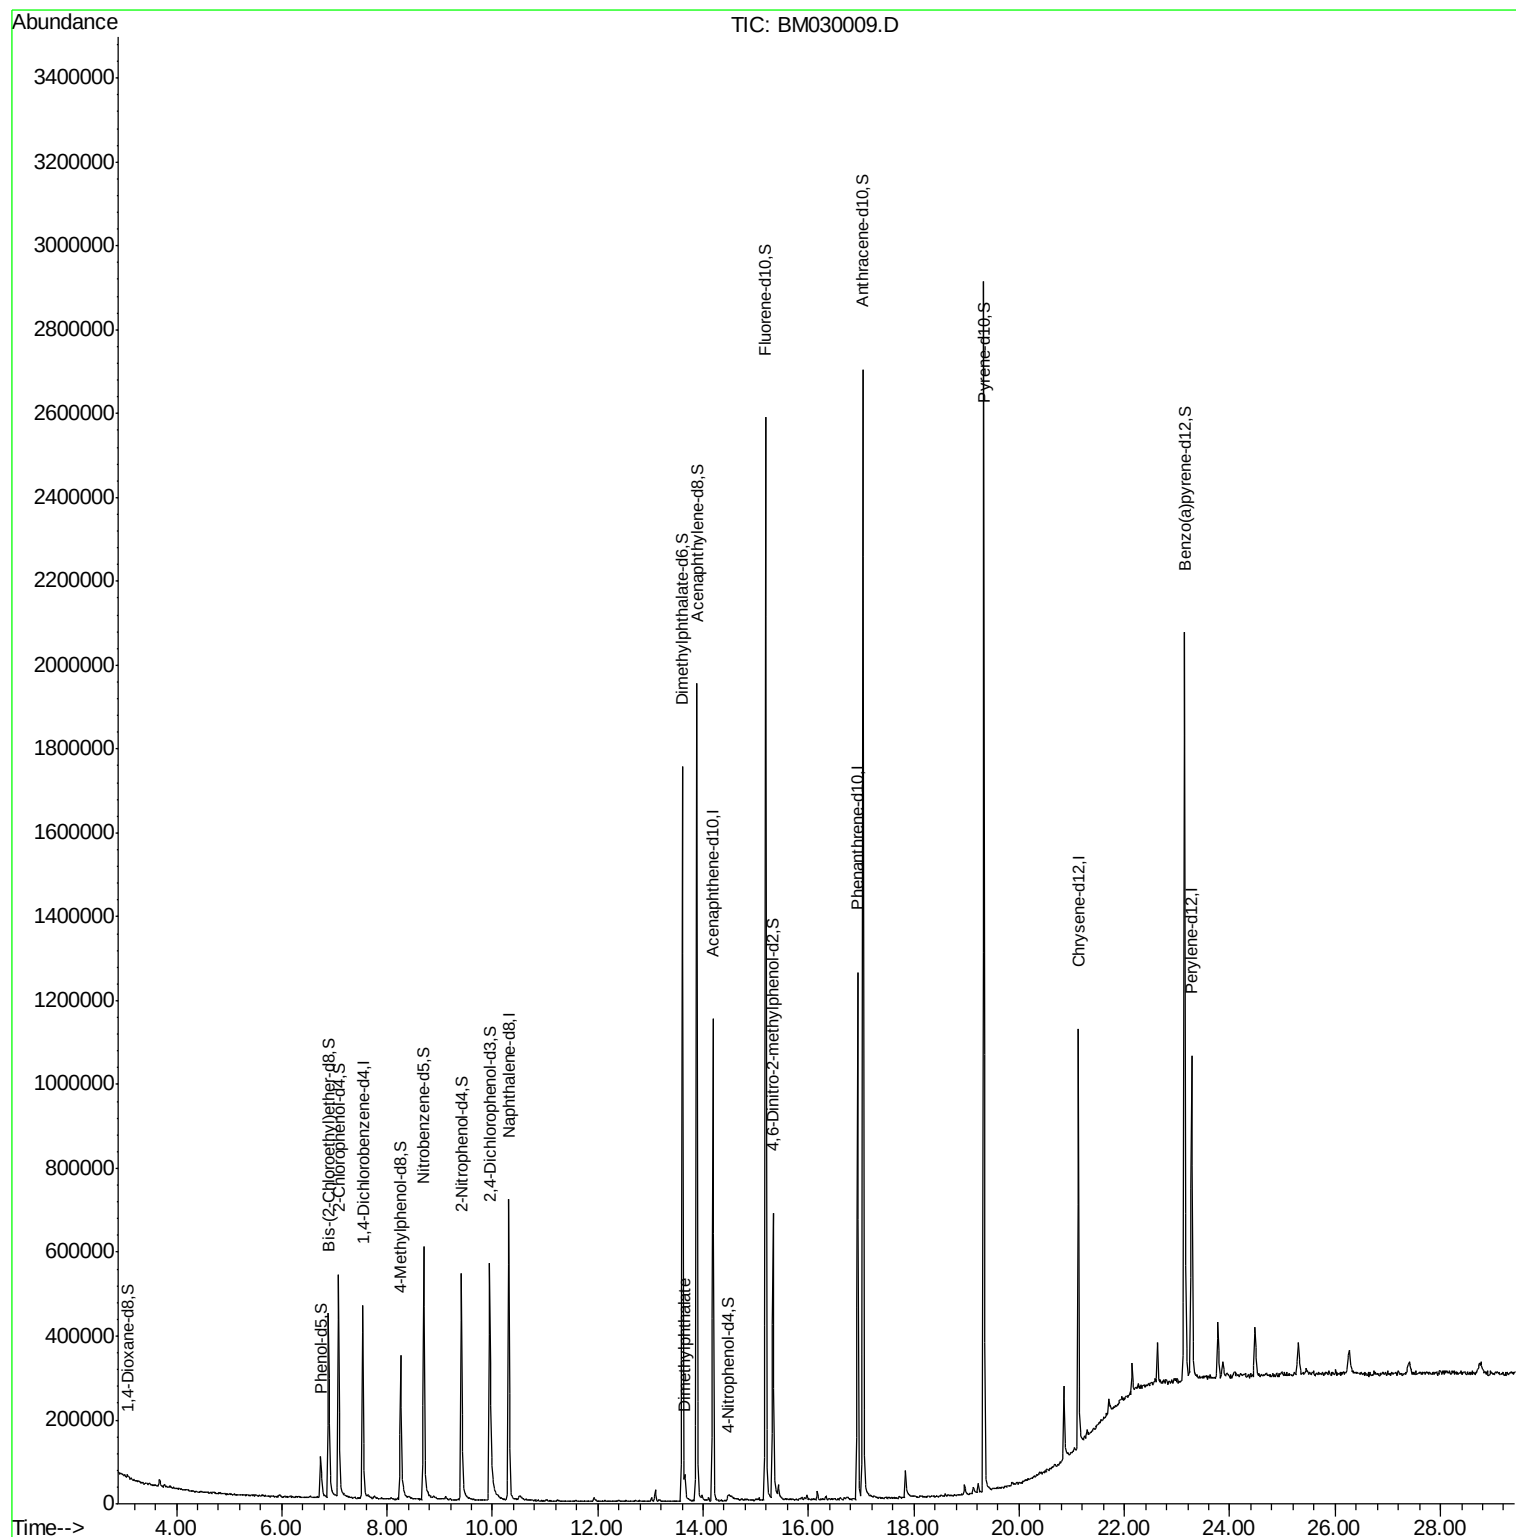

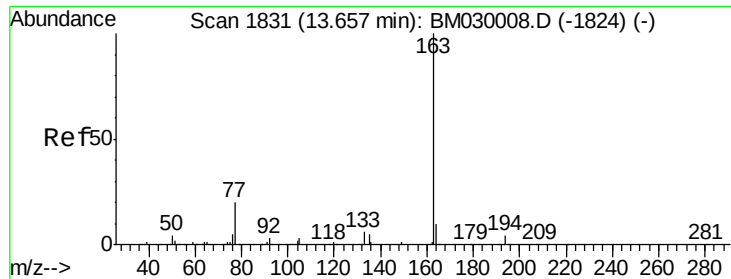

#47
 Dimethylphthalate
 Concen: 1.103 ng/ul
 RT: 13.66 min Scan# 1831
 Delta R.T. 0.00 min
 Lab File: BM030009.D
 Acq: 13 May 2021 13:45

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y8

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.9	3.4	5.0
164	10.1	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/14/2021 12:49:54 PM

