

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029903.D
 Acq On : 10 May 2021 09:42
 Operator : CG/JU
 Sample : PB136206BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK206

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	27	30	45	rVB2	35325	67225	1.70%	0.177%
2	3.481	99	101	123	rBV	248992	644582	16.27%	1.693%
3	3.781	150	152	156	rVB3	8971	9042	0.23%	0.024%
4	6.740	649	655	672	rBV	504959	924915	23.35%	2.430%
5	6.898	677	682	701	rVV	382904	702153	17.72%	1.845%
6	7.087	708	714	732	rBV	551789	968395	24.45%	2.544%
7	7.551	786	793	807	rBV	487831	834889	21.08%	2.193%
8	8.269	909	915	934	rBV	626199	1145117	28.91%	3.008%
9	8.710	983	990	1007	rBV	489043	894719	22.59%	2.351%
10	9.428	1105	1112	1129	rBV	390083	727893	18.37%	1.912%
11	9.963	1196	1203	1222	rBV	569903	1148039	28.98%	3.016%
12	10.328	1257	1265	1284	rBV	771702	1294789	32.68%	3.402%
13	10.475	1284	1290	1313	rBV	516543	1205082	30.42%	3.166%
14	11.951	1537	1541	1549	rBV4	4981	10160	0.26%	0.027%
15	13.621	1817	1825	1841	rBV	1351693	1956304	49.38%	5.139%
16	13.892	1864	1871	1888	rBV	1612077	2339629	59.06%	6.146%
17	14.198	1916	1923	1939	rBV	1250325	1829024	46.17%	4.805%
18	14.433	1957	1963	1995	rBV	176613	648171	16.36%	1.703%
19	15.198	2086	2093	2110	rBV	2083350	2949859	74.46%	7.750%
20	15.333	2110	2116	2130	rVV	474816	763457	19.27%	2.006%
21	15.439	2130	2134	2145	rVB	26627	50622	1.28%	0.133%
22	15.986	2222	2227	2236	rVB5	6527	12429	0.31%	0.033%
23	16.739	2351	2355	2357	rBV3	4347	5409	0.14%	0.014%
24	16.945	2384	2390	2401	rBV	1487205	2132503	53.83%	5.602%
25	17.045	2401	2407	2434	rVB	2278093	3332393	84.12%	8.754%
26	18.980	2732	2736	2744	rBV	18705	28829	0.73%	0.076%
27	19.227	2775	2778	2783	rBV	16002	23299	0.59%	0.061%
28	19.298	2787	2790	2791	rBV3	3782	4390	0.11%	0.012%
29	19.345	2791	2798	2811	rBV	2920951	3961440	100.00%	10.407%
30	21.133	3097	3102	3118	rBV	1695235	2330215	58.82%	6.122%
31	23.150	3439	3445	3460	rVB2	1715269	3215964	81.18%	8.449%
32	23.286	3462	3468	3477	rBV2	998449	1904096	48.07%	5.002%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029903.D
Acq On : 10 May 2021 09:42
Operator : CG/JU
Sample : PB136206BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK206

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION


Sum of corrected areas: 38065033

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029903.D
Acq On : 10 May 2021 09:42
Operator : CG/JU
Sample : PB136206BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

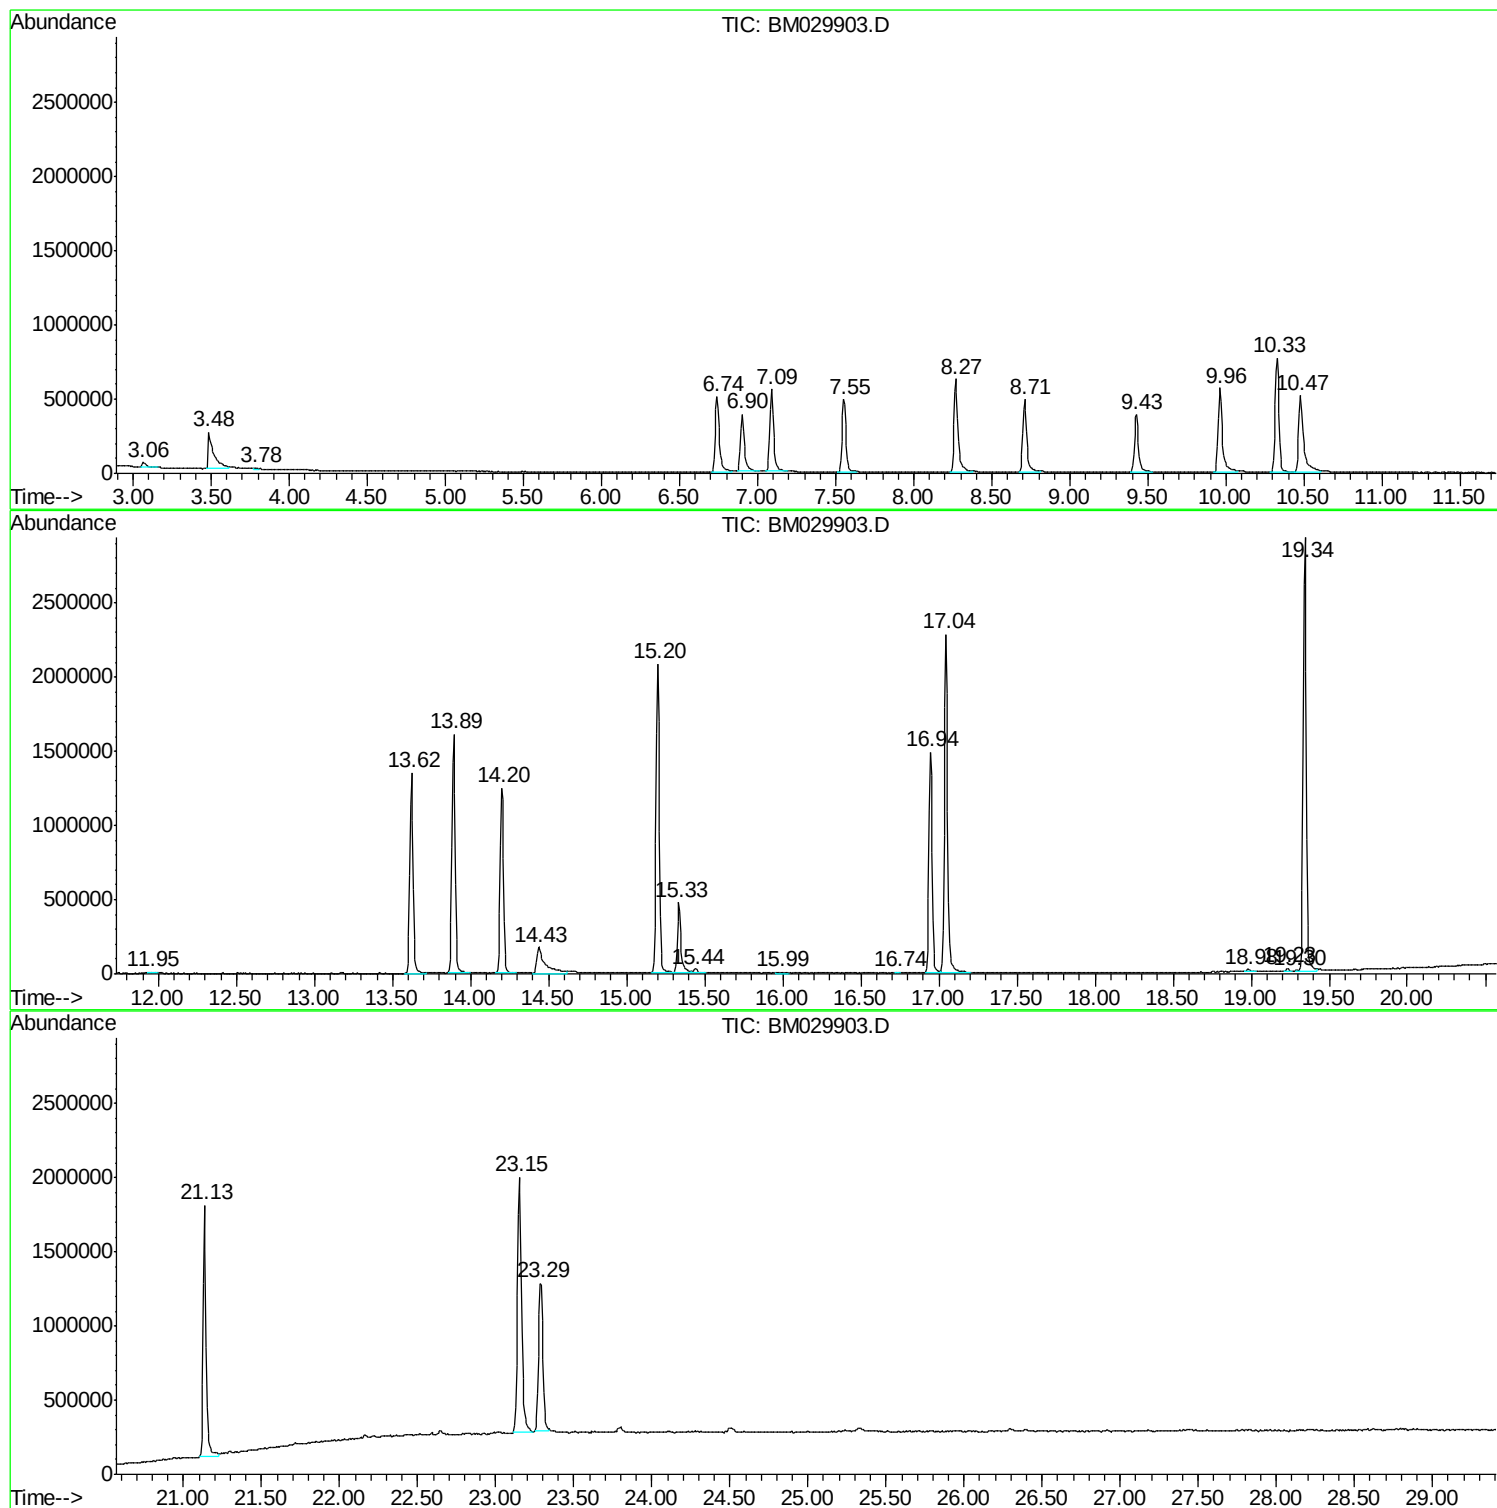

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029903.D
Acq On : 10 May 2021 09:42
Operator : CG/JU
Sample : PB136206BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029903.D
Acq On : 10 May 2021 09:42
Operator : CG/JU
Sample : PB136206BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK206

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc