

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029913.D
 Acq On : 10 May 2021 20:11
 Operator : CG/JU
 Sample : M2177-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG579

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.551	110	113	114	rBV	18921	22326	0.80%	0.094%
2	3.693	134	137	143	rVB2	20040	29028	1.04%	0.123%
3	4.698	304	308	313	rBV5	7691	13606	0.49%	0.057%
4	5.163	384	387	389	rBV3	2856	3498	0.13%	0.015%
5	5.969	521	524	527	rBV5	1956	2928	0.10%	0.012%
6	6.545	619	622	629	rVB6	3297	6273	0.22%	0.027%
7	6.745	651	656	676	rBV	134986	335193	12.01%	1.416%
8	6.904	678	683	698	rVV	63848	133095	4.77%	0.562%
9	7.092	709	715	727	rBV	124336	237671	8.51%	1.004%
10	7.181	727	730	741	rVB7	7625	16554	0.59%	0.070%
11	7.386	763	765	772	rBV8	2354	4097	0.15%	0.017%
12	7.551	786	793	812	rBV	473258	859593	30.79%	3.631%
13	7.775	827	831	840	rVB4	9097	13540	0.49%	0.057%
14	8.028	873	874	879	rVB4	2718	3229	0.12%	0.014%
15	8.086	879	884	888	rBV5	6348	10956	0.39%	0.046%
16	8.216	899	906	909	rBV5	5661	8847	0.32%	0.037%
17	8.281	912	917	931	rVV	82048	202841	7.27%	0.857%
18	8.398	933	937	952	rVB4	20155	57084	2.04%	0.241%
19	8.716	983	991	1009	rBV	74351	185590	6.65%	0.784%
20	8.910	1018	1024	1028	rVB6	5451	10759	0.39%	0.045%
21	8.986	1033	1037	1041	rVB7	1767	2799	0.10%	0.012%
22	9.069	1046	1051	1054	rVB6	4044	5700	0.20%	0.024%
23	9.128	1054	1061	1065	rBV5	4445	8781	0.31%	0.037%
24	9.198	1067	1073	1078	rVV2	8730	14653	0.52%	0.062%
25	9.245	1078	1081	1089	rVB7	4441	9844	0.35%	0.042%
26	9.433	1105	1113	1121	rBV	59583	128481	4.60%	0.543%
27	9.510	1121	1126	1130	rVB8	5491	11092	0.40%	0.047%
28	9.816	1174	1178	1181	rBV5	2743	3642	0.13%	0.015%
29	9.922	1193	1196	1199	rBV5	2680	4820	0.17%	0.020%
30	9.975	1199	1205	1225	rVV	108911	313470	11.23%	1.324%
31	10.198	1239	1243	1248	rVB5	7756	12208	0.44%	0.052%
32	10.327	1258	1265	1277	rBV	750975	1306060	46.78%	5.518%
33	10.504	1288	1295	1313	rBV2	52343	179860	6.44%	0.760%
34	10.733	1328	1334	1336	rBV7	3154	3812	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029913.D
 Acq On : 10 May 2021 20:11
 Operator : CG/JU
 Sample : M2177-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG579

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

35	10.863	1351	1356	1362	rVB5	4939	9820	0.35%	0.041%
36	11.010	1377	1381	1386	rVB8	4171	5166	0.19%	0.022%
37	11.222	1415	1417	1422	rVB5	3455	3465	0.12%	0.015%
38	11.298	1427	1430	1436	rVB7	2858	4539	0.16%	0.019%
39	11.404	1439	1448	1449	rBV8	5874	10354	0.37%	0.044%
40	11.422	1449	1451	1456	rVB5	5454	6057	0.22%	0.026%
41	11.504	1460	1465	1466	rBV5	2535	3709	0.13%	0.016%
42	11.604	1479	1482	1488	rVB6	6440	11337	0.41%	0.048%
43	11.757	1504	1508	1510	rBV5	2622	4276	0.15%	0.018%
44	11.798	1510	1515	1518	rVV7	2699	5086	0.18%	0.021%
45	12.074	1557	1562	1563	rBV4	3976	5529	0.20%	0.023%
46	12.092	1563	1565	1568	rVB4	2835	2793	0.10%	0.012%
47	12.139	1568	1573	1576	rBV7	3286	7264	0.26%	0.031%
48	12.480	1628	1631	1636	rVB7	2755	4001	0.14%	0.017%
49	12.545	1636	1642	1646	rBV8	5746	12471	0.45%	0.053%
50	12.621	1650	1655	1660	rVV7	4812	9664	0.35%	0.041%
51	12.692	1660	1667	1670	rVV9	4490	9125	0.33%	0.039%
52	12.792	1680	1684	1685	rBV4	3965	4599	0.16%	0.019%
53	12.874	1696	1698	1702	rVB5	3089	3426	0.12%	0.014%
54	12.968	1708	1714	1718	rBV6	9113	15380	0.55%	0.065%
55	13.116	1733	1739	1740	rBV6	5394	7672	0.27%	0.032%
56	13.245	1757	1761	1763	rBV4	4713	7552	0.27%	0.032%
57	13.515	1805	1807	1810	rBV4	4192	4924	0.18%	0.021%
58	13.621	1819	1825	1831	rBV	298882	467092	16.73%	1.973%
59	13.721	1840	1842	1843	rBV2	2928	2826	0.10%	0.012%
60	13.804	1854	1856	1860	rVB5	2634	2939	0.11%	0.012%
61	13.892	1864	1871	1883	rBV	587523	915438	32.79%	3.867%
62	14.027	1890	1894	1898	rVB6	15801	23670	0.85%	0.100%
63	14.098	1902	1906	1912	rBV8	13308	27832	1.00%	0.118%
64	14.157	1912	1916	1917	rBV4	10693	11991	0.43%	0.051%
65	14.198	1917	1923	1931	rVB	1217482	1823622	65.32%	7.704%
66	14.374	1950	1953	1954	rBV2	4223	5202	0.19%	0.022%
67	14.486	1967	1972	1973	rBV5	6419	9789	0.35%	0.041%
68	14.557	1982	1984	1992	rVB9	10402	15398	0.55%	0.065%
69	14.651	1997	2000	2004	rVB6	9822	13948	0.50%	0.059%
70	14.827	2015	2030	2034	rBV2	36913	162611	5.82%	0.687%
71	14.986	2054	2057	2064	rVB6	21601	30313	1.09%	0.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
 Data File : BM029913.D
 Acq On : 10 May 2021 20:11
 Operator : CG/JU
 Sample : M2177-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG579

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

72	15.198	2087	2093	2100	rBV	465940	709345	25.41%	2.997%
73	15.339	2113	2117	2126	rBV4	55332	105773	3.79%	0.447%
74	15.927	2213	2217	2220	rBV5	15582	25394	0.91%	0.107%
75	16.704	2346	2349	2357	rBV3	30026	60672	2.17%	0.256%
76	16.945	2384	2390	2395	rBV	1452041	2148508	76.96%	9.077%
77	16.986	2395	2397	2401	rVV	103051	131521	4.71%	0.556%
78	17.045	2402	2407	2418	rVB	776040	1226658	43.94%	5.182%
79	17.856	2541	2545	2553	rVB9	46526	95102	3.41%	0.402%
80	19.009	2737	2741	2749	rVB	236611	315129	11.29%	1.331%
81	19.345	2792	2798	2801	rBV	1878743	2791695	100.00%	11.794%
82	20.027	2912	2914	2920	rVB	67890	80822	2.90%	0.341%
83	20.856	3053	3055	3064	rVB5	95011	145209	5.20%	0.613%
84	21.062	3086	3090	3094	rVB	208595	230070	8.24%	0.972%
85	21.133	3096	3102	3106	rBV	1855125	2530398	90.64%	10.690%
86	22.644	3356	3359	3364	rBV2	187189	277504	9.94%	1.172%
87	23.150	3440	3445	3460	rVB2	1246094	2785347	99.77%	11.767%
88	23.285	3463	3468	3482	rVB2	1143436	2179017	78.05%	9.205%


Sum of corrected areas: 23670974

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051021\
Data File : BM029913.D
Acq On : 10 May 2021 20:11
Operator : CG/JU
Sample : M2177-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG579

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

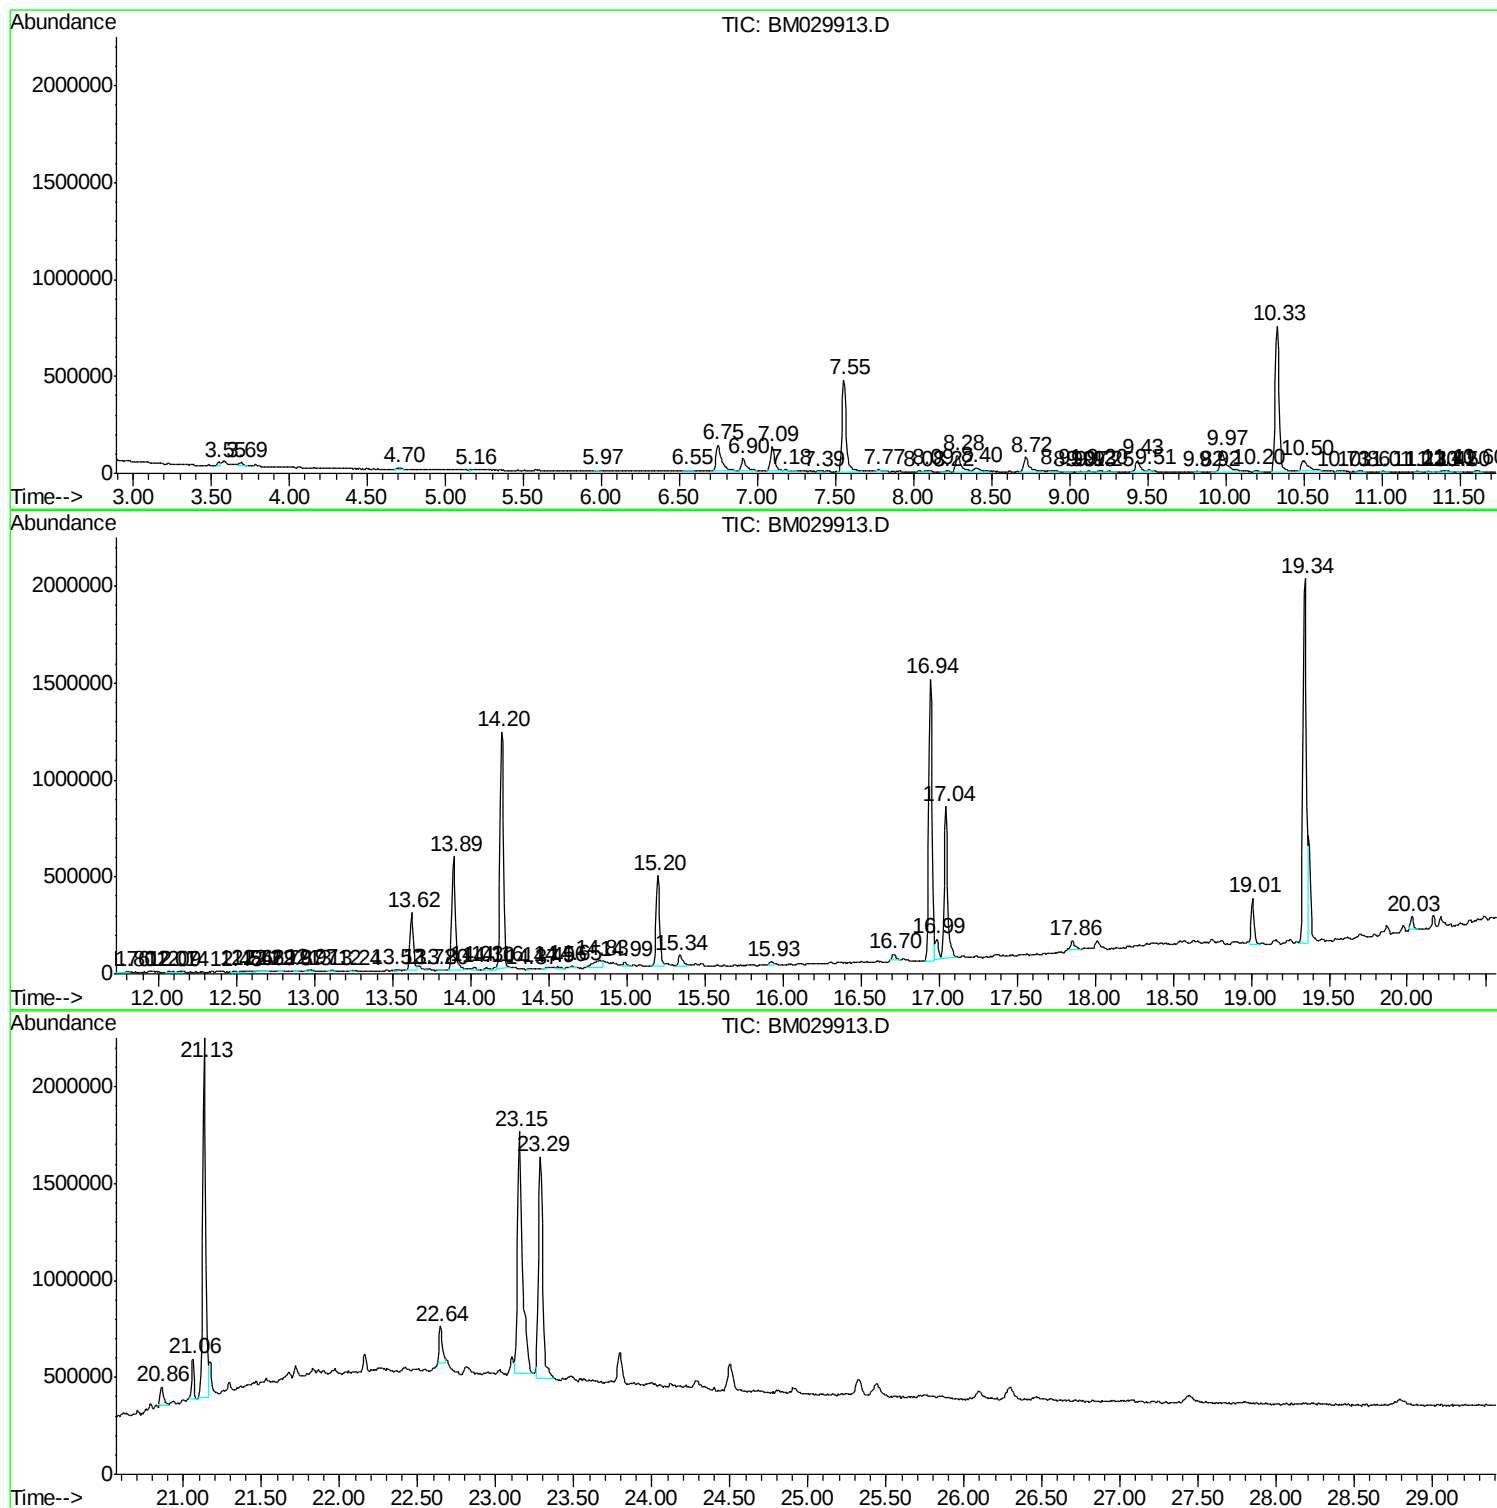

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM029913.D
Acq On : 10 May 2021 20:11
Operator : CG/JU
Sample : M2177-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG579

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM029913.D
Acq On : 10 May 2021 20:11
Operator : CG/JU
Sample : M2177-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG579

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc