

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029916.D
 Acq On : 10 May 2021 21:59
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	133	137	145	rVB	25847	43362	1.86%	0.306%
2	4.693	304	307	313	rBV	18077	28564	1.23%	0.201%
3	5.963	520	523	529	rVB6	5081	7831	0.34%	0.055%
4	6.263	572	574	578	rBV3	2287	2670	0.11%	0.019%
5	6.757	652	658	672	rBV	35463	108218	4.65%	0.763%
6	6.910	676	684	693	rBV	31090	73433	3.16%	0.518%
7	7.098	709	716	727	rBV	53917	114312	4.91%	0.806%
8	7.175	727	729	733	rBV5	3871	6226	0.27%	0.044%
9	7.551	786	793	813	rBV	515774	904852	38.88%	6.377%
10	7.775	827	831	835	rBV5	5222	6953	0.30%	0.049%
11	8.081	880	883	891	rVB2	5533	9677	0.42%	0.068%
12	8.222	903	907	911	rBV4	5586	6378	0.27%	0.045%
13	8.281	912	917	928	rBV2	36409	96145	4.13%	0.678%
14	8.410	935	939	944	rBV6	6015	10266	0.44%	0.072%
15	8.622	971	975	978	rBV6	1914	3293	0.14%	0.023%
16	8.722	984	992	1005	rBV	37059	105121	4.52%	0.741%
17	8.857	1012	1015	1016	rBV3	2174	2376	0.10%	0.017%
18	8.898	1020	1022	1026	rVB5	4115	4204	0.18%	0.030%
19	8.998	1037	1039	1045	rVB6	2509	4475	0.19%	0.032%
20	9.122	1054	1060	1064	rVB8	5328	8878	0.38%	0.063%
21	9.239	1079	1080	1085	rVB4	3904	5337	0.23%	0.038%
22	9.304	1087	1091	1095	rVB6	3069	4623	0.20%	0.033%
23	9.433	1104	1113	1122	rBV3	31450	79442	3.41%	0.560%
24	9.645	1146	1149	1153	rBV5	3126	3915	0.17%	0.028%
25	9.922	1189	1196	1201	rBV5	4417	10677	0.46%	0.075%
26	9.998	1201	1209	1218	rBV4	26989	93899	4.03%	0.662%
27	10.328	1257	1265	1281	rBV	792243	1396910	60.02%	9.846%
28	10.510	1290	1296	1298	rBV4	15503	30759	1.32%	0.217%
29	10.622	1313	1315	1322	rVB8	4100	5757	0.25%	0.041%
30	10.733	1332	1334	1337	rVB4	3118	2449	0.11%	0.017%
31	10.810	1342	1347	1353	rVB8	5384	10797	0.46%	0.076%
32	10.998	1371	1379	1383	rBV8	3814	7922	0.34%	0.056%
33	11.069	1388	1391	1393	rBV4	3071	3904	0.17%	0.028%
34	11.157	1402	1406	1409	rBV5	2071	3392	0.15%	0.024%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029916.D
 Acq On : 10 May 2021 21:59
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

35	11.222	1415	1417	1420	rBV4	2046	2357	0.10%	0.017%
36	11.375	1437	1443	1444	rBV5	4623	8065	0.35%	0.057%
37	11.498	1461	1464	1465	rBV3	3161	3608	0.16%	0.025%
38	11.510	1465	1466	1470	rVB4	4435	4273	0.18%	0.030%
39	11.604	1477	1482	1487	rBV8	5599	12075	0.52%	0.085%
40	11.739	1500	1505	1508	rBV7	2676	4430	0.19%	0.031%
41	11.898	1526	1532	1537	rBV5	9620	18932	0.81%	0.133%
42	11.957	1541	1542	1549	rVB7	5197	8230	0.35%	0.058%
43	12.016	1549	1552	1553	rVB3	3116	2711	0.12%	0.019%
44	12.063	1553	1560	1564	rBV10	6210	12753	0.55%	0.090%
45	12.133	1569	1572	1574	rBV4	2897	4036	0.17%	0.028%
46	12.257	1591	1593	1596	rVB3	2547	2822	0.12%	0.020%
47	12.380	1610	1614	1615	rBV4	3810	4211	0.18%	0.030%
48	12.474	1627	1630	1633	rBV4	3380	5406	0.23%	0.038%
49	12.545	1636	1642	1647	rBV8	7434	16058	0.69%	0.113%
50	12.616	1651	1654	1660	rVB7	7808	10190	0.44%	0.072%
51	12.680	1662	1665	1666	rBV3	2412	2646	0.11%	0.019%
52	12.733	1672	1674	1676	rVV3	3489	2498	0.11%	0.018%
53	12.786	1678	1683	1688	rVB9	6709	11680	0.50%	0.082%
54	12.886	1695	1700	1701	rBV5	2832	3382	0.15%	0.024%
55	12.910	1701	1704	1707	rVV4	2924	3361	0.14%	0.024%
56	12.963	1709	1713	1717	rBV5	9155	15110	0.65%	0.106%
57	13.004	1717	1720	1722	rVV4	4041	4573	0.20%	0.032%
58	13.174	1747	1749	1752	rBV4	2312	3164	0.14%	0.022%
59	13.257	1758	1763	1770	rBV10	7285	16319	0.70%	0.115%
60	13.333	1774	1776	1781	rVB5	4459	5638	0.24%	0.040%
61	13.416	1783	1790	1792	rBV8	6717	13115	0.56%	0.092%
62	13.621	1819	1825	1831	rBV	193996	320486	13.77%	2.259%
63	13.892	1863	1871	1878	rBV	190705	302908	13.02%	2.135%
64	14.027	1890	1894	1900	rVB3	30306	45731	1.97%	0.322%
65	14.098	1904	1906	1908	rBV3	4605	4034	0.17%	0.028%
66	14.157	1913	1916	1917	rBV3	13735	12673	0.54%	0.089%
67	14.198	1917	1923	1934	rVB	1334453	2010029	86.37%	14.167%
68	14.527	1974	1979	1982	rBV6	12087	22663	0.97%	0.160%
69	14.651	1998	2000	2004	rVB4	12328	12430	0.53%	0.088%
70	14.915	2042	2045	2052	rVB8	10196	16168	0.69%	0.114%
71	14.986	2053	2057	2061	rBV6	21547	29645	1.27%	0.209%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029916.D
Acq On : 10 May 2021 21:59
Operator : CG/JU
Sample : M2177-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG580

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION

72	15.198	2088	2093	2109	rBV	266085	436744	18.77%	3.078%
73	15.345	2114	2118	2127	rBV	20841	44071	1.89%	0.311%
74	15.951	2215	2221	2225	rBV5	18396	36578	1.57%	0.258%
75	16.945	2384	2390	2401	rBV	1596620	2327250	100.00%	16.403%
76	17.045	2402	2407	2418	rVB2	289636	475688	20.44%	3.353%
77	17.851	2541	2544	2549	rBV6	37682	51872	2.23%	0.366%
78	19.009	2737	2741	2746	rBV	92259	128983	5.54%	0.909%
79	19.339	2793	2797	2801	rBV2	377839	563780	24.23%	3.974%
80	21.133	3097	3102	3113	rBV	1533740	2159671	92.80%	15.222%
81	23.286	3462	3468	3480	rVB2	951539	1778136	76.41%	12.532%


Sum of corrected areas: 14188200

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029916.D
Acq On : 10 May 2021 21:59
Operator : CG/JU
Sample : M2177-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG580

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

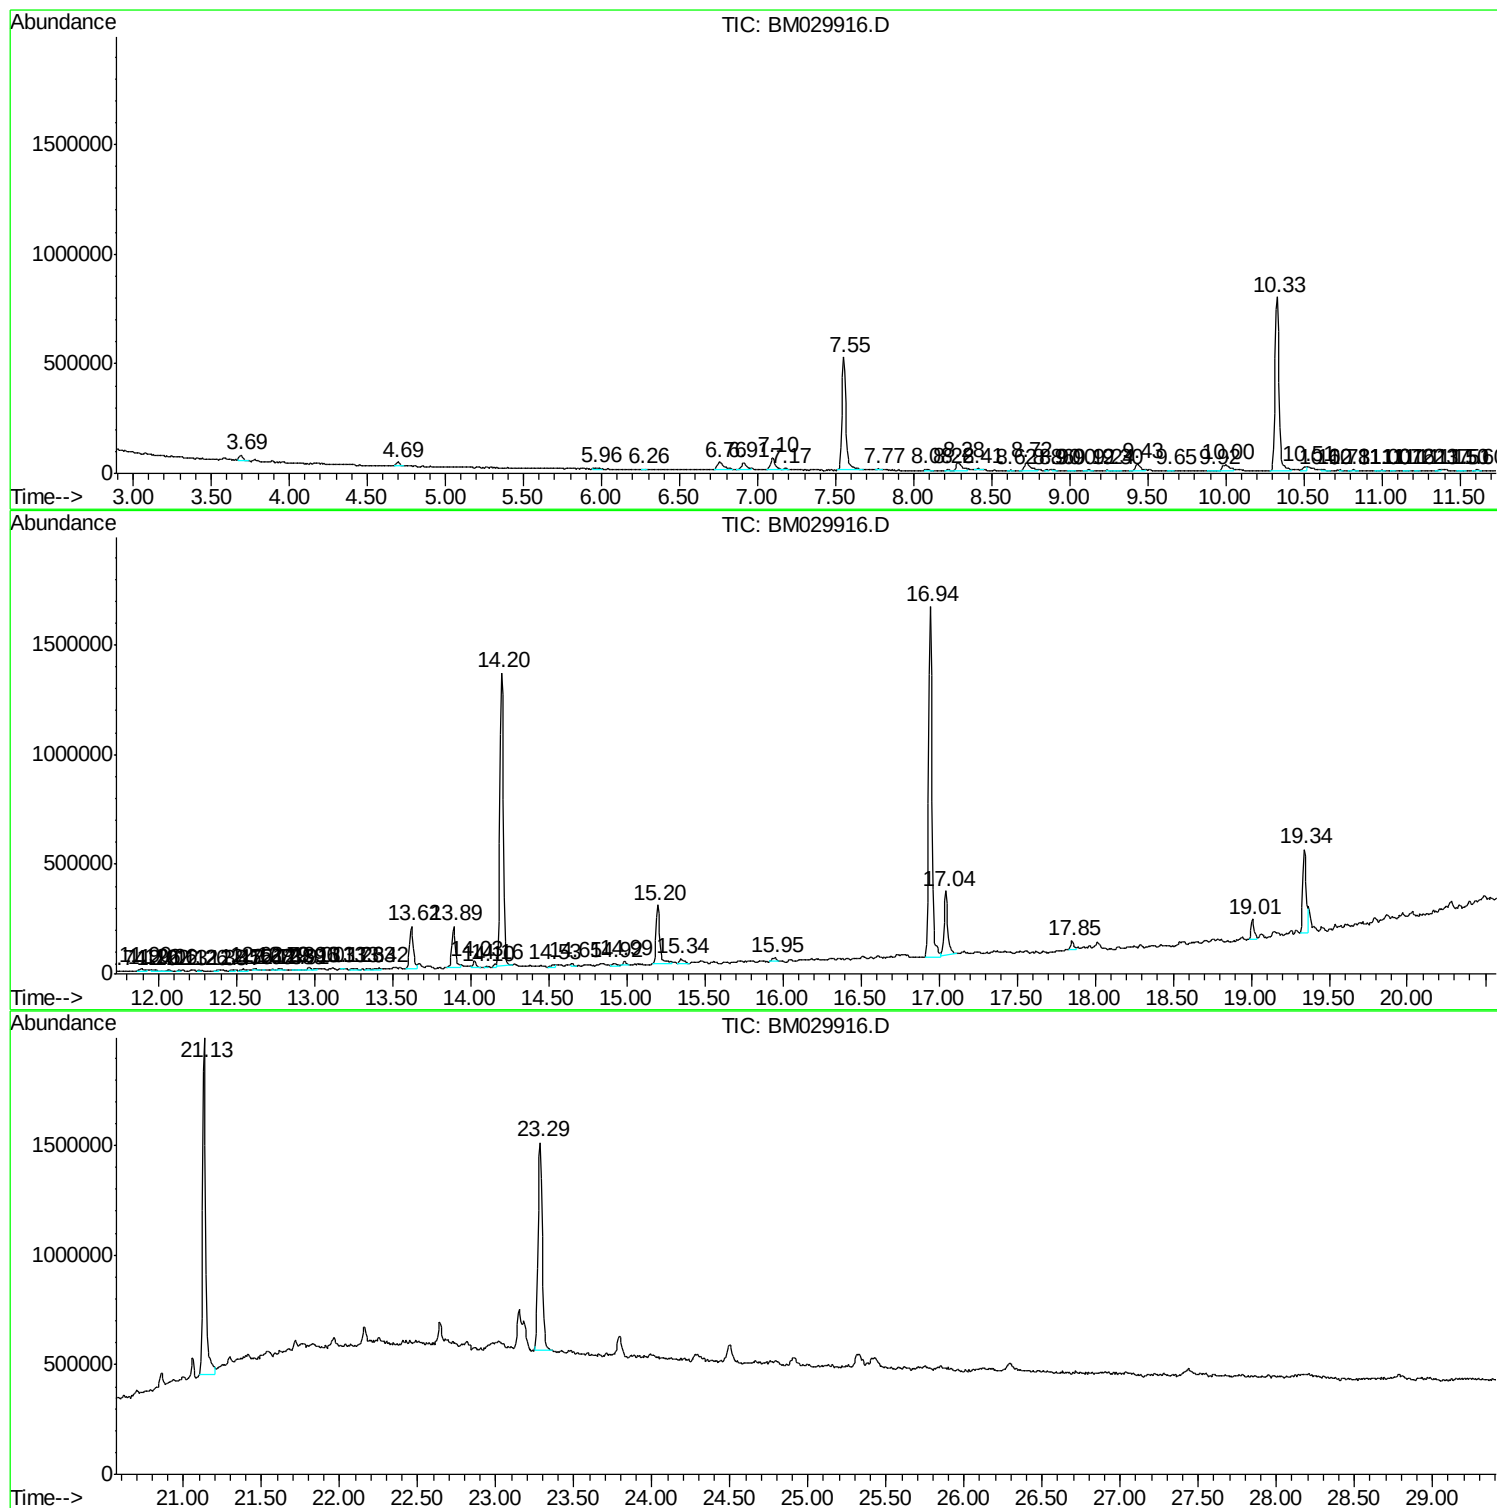

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\\
Data_File : BM029916.D
Acq_On : 10 May, 2021 21:599
Operator : CG/JUU
Sample : M2177-033
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
BG580

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SEAM-EPA-BM050721.M
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
