

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029919.D
 Acq On : 10 May 2021 23:47
 Operator : CG/JU
 Sample : M2177-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG578

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.546	620	622	628	rVB4	4230	6902	0.30%	0.038%
2	6.746	651	656	668	rBV2	78437	192690	8.27%	1.065%
3	6.904	677	683	694	rBV	70035	145062	6.23%	0.802%
4	7.093	709	715	726	rBV	112874	216479	9.29%	1.196%
5	7.181	727	730	739	rVB7	7620	15418	0.66%	0.085%
6	7.551	787	793	811	rBV	529404	913709	39.22%	5.050%
7	7.740	820	825	827	rBV5	3113	3424	0.15%	0.019%
8	7.769	827	830	835	rBV5	6434	9327	0.40%	0.052%
9	7.893	849	851	855	rVB5	2263	2512	0.11%	0.014%
10	7.975	863	865	872	rVB6	2332	4150	0.18%	0.023%
11	8.087	880	884	893	rVB5	8220	17381	0.75%	0.096%
12	8.198	901	903	904	rBV2	2802	2442	0.10%	0.013%
13	8.216	904	906	910	rBV5	4068	5412	0.23%	0.030%
14	8.275	911	916	933	rBV	95830	224622	9.64%	1.241%
15	8.404	933	938	945	rVB7	8508	20414	0.88%	0.113%
16	8.522	956	958	963	rVB6	2602	3227	0.14%	0.018%
17	8.716	985	991	1001	rBV	90133	204718	8.79%	1.131%
18	8.857	1010	1015	1017	rBV5	4702	7454	0.32%	0.041%
19	8.898	1019	1022	1027	rVB5	4911	7796	0.33%	0.043%
20	9.122	1056	1060	1064	rVB6	3511	6590	0.28%	0.036%
21	9.239	1075	1080	1088	rVV8	4490	9787	0.42%	0.054%
22	9.304	1088	1091	1097	rVB6	3160	4952	0.21%	0.027%
23	9.434	1104	1113	1123	rBV	74351	173289	7.44%	0.958%
24	9.745	1163	1166	1168	rBV3	2113	2835	0.12%	0.016%
25	9.922	1191	1196	1199	rBV6	2744	3955	0.17%	0.022%
26	9.975	1199	1205	1225	rBV	79377	232675	9.99%	1.286%
27	10.328	1257	1265	1277	rBV	810975	1416399	60.79%	7.828%
28	10.445	1282	1285	1287	rVV4	3001	4102	0.18%	0.023%
29	10.492	1287	1293	1316	rVV	66224	212485	9.12%	1.174%
30	10.810	1344	1347	1350	rBV4	4424	4637	0.20%	0.026%
31	10.881	1358	1359	1368	rVB8	2612	3713	0.16%	0.021%
32	11.004	1376	1380	1382	rBV4	2074	2545	0.11%	0.014%
33	11.163	1405	1407	1410	rVB4	2553	2355	0.10%	0.013%
34	11.357	1434	1440	1445	rBV	15361	26371	1.13%	0.146%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029919.D
 Acq On : 10 May 2021 23:47
 Operator : CG/JU
 Sample : M2177-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG578

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

35	11.504	1464	1465	1470	rVB5	2306	2695	0.12%	0.015%
36	11.610	1476	1483	1489	rBV9	4764	8806	0.38%	0.049%
37	11.680	1491	1495	1497	rVB4	2198	2769	0.12%	0.015%
38	11.739	1500	1505	1507	rBV5	2778	3910	0.17%	0.022%
39	11.945	1537	1540	1541	rBV3	3512	2732	0.12%	0.015%
40	12.069	1556	1561	1563	rBV5	3392	5493	0.24%	0.030%
41	12.133	1568	1572	1575	rVV5	2305	3855	0.17%	0.021%
42	12.163	1575	1577	1581	rVV5	2652	2684	0.12%	0.015%
43	12.228	1583	1588	1591	rVV6	4021	7663	0.33%	0.042%
44	12.251	1591	1592	1599	rVB7	3310	4082	0.18%	0.023%
45	12.463	1624	1628	1636	rVB8	6294	14208	0.61%	0.079%
46	12.616	1649	1654	1659	rVB8	4928	9089	0.39%	0.050%
47	12.686	1662	1666	1669	rBV3	5865	7705	0.33%	0.043%
48	12.733	1669	1674	1679	rVV	29689	42813	1.84%	0.237%
49	12.780	1679	1682	1689	rVB8	4959	10905	0.47%	0.060%
50	12.916	1700	1705	1709	rBV7	2602	4310	0.18%	0.024%
51	12.963	1709	1713	1716	rBV7	5056	7648	0.33%	0.042%
52	13.004	1716	1720	1723	rVV4	4242	6897	0.30%	0.038%
53	13.045	1723	1727	1731	rVV7	6509	10848	0.47%	0.060%
54	13.116	1734	1739	1744	rVB7	6872	14041	0.60%	0.078%
55	13.186	1749	1751	1757	rVB6	7448	10679	0.46%	0.059%
56	13.239	1757	1760	1761	rBV3	3703	3976	0.17%	0.022%
57	13.345	1772	1778	1780	rBV6	4342	7626	0.33%	0.042%
58	13.622	1819	1825	1830	rBV	324307	492719	21.15%	2.723%
59	13.692	1830	1837	1842	rVV2	50818	114185	4.90%	0.631%
60	13.733	1842	1844	1852	rVB7	10981	20055	0.86%	0.111%
61	13.886	1862	1870	1882	rBV	343075	566303	24.31%	3.130%
62	14.022	1890	1893	1897	rBV4	12378	15105	0.65%	0.083%
63	14.104	1903	1907	1912	rBV7	4958	9344	0.40%	0.052%
64	14.198	1913	1923	1932	rBV	1358356	2051780	88.07%	11.339%
65	14.333	1944	1946	1950	rVB5	5365	6354	0.27%	0.035%
66	14.421	1958	1961	1962	rBV3	5085	4690	0.20%	0.026%
67	14.516	1971	1977	1979	rBV7	9152	16876	0.72%	0.093%
68	14.610	1990	1993	1999	rVB4	15132	23393	1.00%	0.129%
69	14.733	2010	2014	2022	rVB7	22114	36461	1.56%	0.202%
70	14.827	2025	2030	2031	rBV5	8975	14303	0.61%	0.079%
71	14.904	2042	2043	2045	rBV2	5402	4821	0.21%	0.027%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029919.D
 Acq On : 10 May 2021 23:47
 Operator : CG/JU
 Sample : M2177-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG578

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

72	14.986	2053	2057	2061	rBV6	14348	21704	0.93%	0.120%
73	15.039	2064	2066	2070	rVB5	8439	8570	0.37%	0.047%
74	15.198	2087	2093	2107	rBV	447324	694098	29.79%	3.836%
75	15.339	2113	2117	2127	rVB8	31789	72489	3.11%	0.401%
76	15.474	2136	2140	2146	rVB	49417	77243	3.32%	0.427%
77	15.627	2163	2166	2170	rBV5	7585	10864	0.47%	0.060%
78	15.680	2171	2175	2177	rBV5	9511	13494	0.58%	0.075%
79	15.774	2186	2191	2193	rBV6	10246	17935	0.77%	0.099%
80	15.851	2202	2204	2207	rBV4	4308	5721	0.25%	0.032%
81	15.951	2214	2221	2226	rBV	89586	155580	6.68%	0.860%
82	16.057	2234	2239	2240	rBV5	10302	15942	0.68%	0.088%
83	16.239	2267	2270	2271	rBV3	7751	7575	0.33%	0.042%
84	16.310	2278	2282	2284	rBV4	12290	19588	0.84%	0.108%
85	16.498	2312	2314	2316	rBV3	7796	7974	0.34%	0.044%
86	16.668	2341	2343	2345	rBV3	6356	7684	0.33%	0.042%
87	16.768	2357	2360	2368	rVB	59017	98133	4.21%	0.542%
88	16.945	2384	2390	2401	rBV	1562859	2329818	100.00%	12.876%
89	17.045	2401	2407	2419	rVB	459971	722529	31.01%	3.993%
90	17.374	2460	2463	2468	rVB3	16963	26151	1.12%	0.145%
91	17.851	2542	2544	2547	rBV4	14918	16794	0.72%	0.093%
92	19.339	2792	2797	2806	rBV	596714	900480	38.65%	4.977%
93	20.856	3053	3055	3061	rVB3	88801	98117	4.21%	0.542%
94	21.056	3086	3089	3096	rBV	180123	207453	8.90%	1.146%
95	21.127	3097	3101	3112	rVV	1559044	2149612	92.27%	11.880%
96	23.150	3440	3445	3458	rVB3	327367	816275	35.04%	4.511%
97	23.286	3462	3468	3483	rVB2	975492	1911015	82.02%	10.561%


Sum of corrected areas: 18094490

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029919.D
Acq On : 10 May 2021 23:47
Operator : CG/JU
Sample : M2177-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG578

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

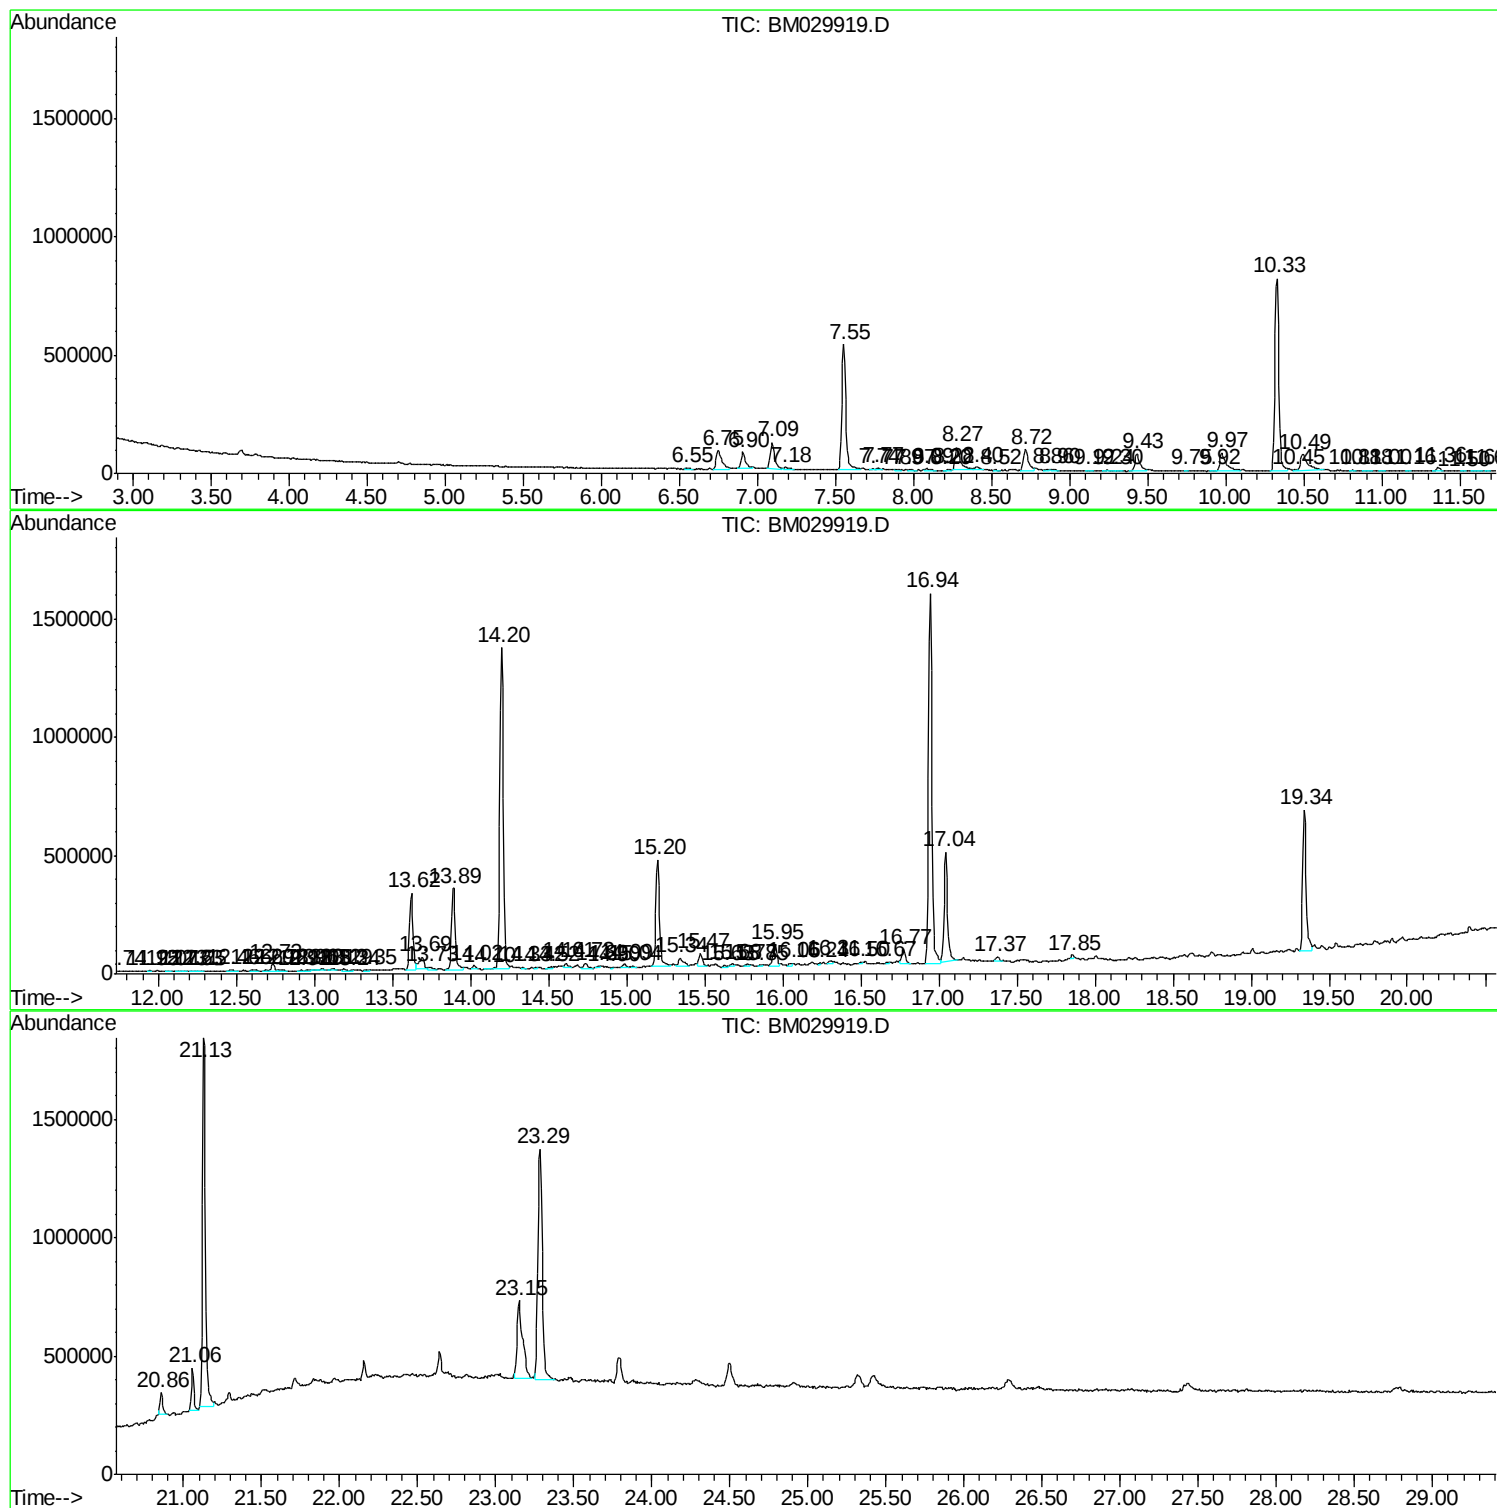

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\\
Data_File : BM029919.D
Acq_On : 10 May, 2021 23:477
Operator : CG/JUU
Sample : M2177-144
Misc :
ALS_Vial : 18 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
BG578

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SEAM-EPA-BM050721.M
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
