

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029939.D
 Acq On : 11 May 2021 12:24
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.740	651	655	671	rVB	196451	418734	27.00%	2.530%
2	6.899	679	682	693	rVB2	144533	249764	16.10%	1.509%
3	7.087	710	714	725	rVB2	206593	373705	24.09%	2.258%
4	7.552	787	793	803	rVB	414564	698601	45.04%	4.222%
5	8.269	910	915	931	rVB	203718	407052	26.24%	2.460%
6	8.710	984	990	1005	rVB	155660	302655	19.51%	1.829%
7	9.422	1106	1111	1122	rBV	117643	221554	14.28%	1.339%
8	9.740	1163	1165	1167	rBV3	3586	3785	0.24%	0.023%
9	9.963	1197	1203	1218	rBV	181603	379231	24.45%	2.292%
10	10.322	1257	1264	1276	rBV	593950	1012466	65.28%	6.118%
11	10.481	1285	1291	1307	rBV	118130	297158	19.16%	1.796%
12	10.728	1328	1333	1336	rVB7	5267	10116	0.65%	0.061%
13	10.810	1345	1347	1352	rVB4	3602	3595	0.23%	0.022%
14	10.881	1356	1359	1361	rBV4	1960	1775	0.11%	0.011%
15	10.945	1365	1370	1373	rVB5	2560	3726	0.24%	0.023%
16	10.981	1373	1376	1377	rBV3	2705	1942	0.13%	0.012%
17	10.998	1377	1379	1380	rBV2	2245	1876	0.12%	0.011%
18	11.116	1396	1399	1402	rVB4	2478	2976	0.19%	0.018%
19	11.151	1402	1405	1407	rBV4	4137	4037	0.26%	0.024%
20	11.351	1436	1439	1440	rBV3	3283	2394	0.15%	0.014%
21	11.369	1440	1442	1444	rVV3	1842	1725	0.11%	0.010%
22	11.516	1459	1467	1469	rBV6	3351	7186	0.46%	0.043%
23	11.610	1480	1483	1488	rVB7	3198	5159	0.33%	0.031%
24	11.763	1507	1509	1510	rVV2	2175	1573	0.10%	0.010%
25	11.781	1510	1512	1518	rVB7	3417	5453	0.35%	0.033%
26	11.851	1518	1524	1525	rBV6	2406	4111	0.27%	0.025%
27	11.887	1525	1530	1536	rVV6	6126	15519	1.00%	0.094%
28	11.934	1536	1538	1540	rVV3	3392	3053	0.20%	0.018%
29	11.957	1540	1542	1549	rVB6	3256	6363	0.41%	0.038%
30	12.004	1549	1550	1555	rVB5	2161	2162	0.14%	0.013%
31	12.069	1555	1561	1562	rBV6	3429	5543	0.36%	0.033%
32	12.081	1562	1563	1568	rVB4	1902	1812	0.12%	0.011%
33	12.139	1568	1573	1574	rBV5	2255	3030	0.20%	0.018%
34	12.163	1574	1577	1581	rVB6	2722	4318	0.28%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029939.D
 Acq On : 11 May 2021 12:24
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

35	12.210	1581	1585	1587	rBV4	3531	5522	0.36%	0.033%
36	12.339	1599	1607	1609	rVB8	1433	2310	0.15%	0.014%
37	12.387	1611	1615	1618	rBV6	2586	3108	0.20%	0.019%
38	12.475	1625	1630	1631	rBV5	2446	2570	0.17%	0.016%
39	12.486	1631	1632	1637	rVB5	2309	1929	0.12%	0.012%
40	12.534	1637	1640	1645	rBV6	4434	6980	0.45%	0.042%
41	12.616	1650	1654	1662	rVB6	5473	9027	0.58%	0.055%
42	12.692	1662	1667	1669	rVB5	3527	5306	0.34%	0.032%
43	12.734	1669	1674	1677	rBV5	3823	6634	0.43%	0.040%
44	12.786	1677	1683	1687	rBV6	4842	8392	0.54%	0.051%
45	12.969	1708	1714	1716	rBV5	7160	11936	0.77%	0.072%
46	12.998	1716	1719	1723	rVV6	2863	3817	0.25%	0.023%
47	13.116	1735	1739	1744	rVB7	5133	7167	0.46%	0.043%
48	13.169	1744	1748	1750	rBV4	4120	5128	0.33%	0.031%
49	13.192	1750	1752	1757	rVB6	5168	6504	0.42%	0.039%
50	13.234	1757	1759	1760	rBV2	2580	1739	0.11%	0.011%
51	13.263	1760	1764	1767	rVB5	3571	5509	0.36%	0.033%
52	13.334	1775	1776	1779	rVB3	3100	2446	0.16%	0.015%
53	13.363	1779	1781	1784	rVB3	1677	1824	0.12%	0.011%
54	13.416	1784	1790	1792	rBV7	4534	7258	0.47%	0.044%
55	13.498	1801	1804	1806	rBV4	3272	3752	0.24%	0.023%
56	13.616	1817	1824	1831	rBV	486020	724427	46.71%	4.378%
57	13.733	1840	1844	1851	rVB5	8981	20090	1.30%	0.121%
58	13.804	1853	1856	1858	rVB4	2371	2686	0.17%	0.016%
59	13.886	1860	1870	1883	rBV	571621	863091	55.65%	5.216%
60	14.022	1889	1893	1898	rVB4	16173	21620	1.39%	0.131%
61	14.104	1902	1907	1910	rBV5	7035	12570	0.81%	0.076%
62	14.157	1912	1916	1917	rBV4	9770	10248	0.66%	0.062%
63	14.198	1917	1923	1931	rVB	960414	1368433	88.23%	8.270%
64	14.363	1948	1951	1952	rBV2	3023	3345	0.22%	0.020%
65	14.451	1962	1966	1973	rBV5	19278	47930	3.09%	0.290%
66	14.516	1975	1977	1979	rVV3	3752	3420	0.22%	0.021%
67	14.651	1997	2000	2004	rVB6	6850	7647	0.49%	0.046%
68	14.733	2011	2014	2020	rBV6	4840	8656	0.56%	0.052%
69	14.833	2027	2031	2033	rBV5	5832	8891	0.57%	0.054%
70	14.910	2041	2044	2051	rBV8	7182	14993	0.97%	0.091%
71	14.986	2051	2057	2061	rBV6	16817	25612	1.65%	0.155%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029939.D
 Acq On : 11 May 2021 12:24
 Operator : CG/JU
 Sample : M2177-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG580

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

72	15.075	2070	2072	2073	rBV2	4184	3366	0.22%	0.020%
73	15.139	2081	2083	2085	rBV2	2607	2466	0.16%	0.015%
74	15.198	2086	2093	2102	rBV	690515	1048391	67.59%	6.336%
75	15.333	2111	2116	2127	rVB3	55533	107254	6.92%	0.648%
76	15.416	2127	2130	2131	rBV3	5156	5325	0.34%	0.032%
77	15.433	2131	2133	2137	rVV5	6743	7674	0.49%	0.046%
78	15.551	2151	2153	2157	rBV4	4249	5171	0.33%	0.031%
79	15.616	2161	2164	2171	rVB8	4921	6956	0.45%	0.042%
80	15.680	2172	2175	2176	rBV3	4708	5098	0.33%	0.031%
81	15.875	2206	2208	2212	rBV5	4142	5075	0.33%	0.031%
82	15.933	2214	2218	2219	rBV4	10935	14957	0.96%	0.090%
83	16.045	2235	2237	2242	rVB5	6310	9071	0.58%	0.055%
84	16.174	2257	2259	2264	rVB6	6467	8048	0.52%	0.049%
85	16.280	2275	2277	2278	rBV2	3943	2125	0.14%	0.013%
86	16.510	2312	2316	2317	rBV3	5976	7935	0.51%	0.048%
87	16.945	2384	2390	2401	rBV	1081221	1551008	100.00%	9.373%
88	17.039	2401	2406	2418	rVV2	701740	1076298	69.39%	6.504%
89	17.851	2541	2544	2549	rBV7	20283	27444	1.77%	0.166%
90	18.016	2569	2572	2577	rVB4	19270	29523	1.90%	0.178%
91	19.010	2737	2741	2746	rBV	55859	78759	5.08%	0.476%
92	19.339	2792	2797	2812	rBV	845632	1237434	79.78%	7.478%
93	21.133	3097	3102	3113	rBV	882634	1226778	79.10%	7.414%
94	23.151	3439	3445	3459	rVB	471169	1108963	71.50%	6.702%
95	23.286	3462	3468	3483	rVB	646668	1256003	80.98%	7.590%


Sum of corrected areas: 16547788

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029939.D
Acq On : 11 May 2021 12:24
Operator : CG/JU
Sample : M2177-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BG580

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

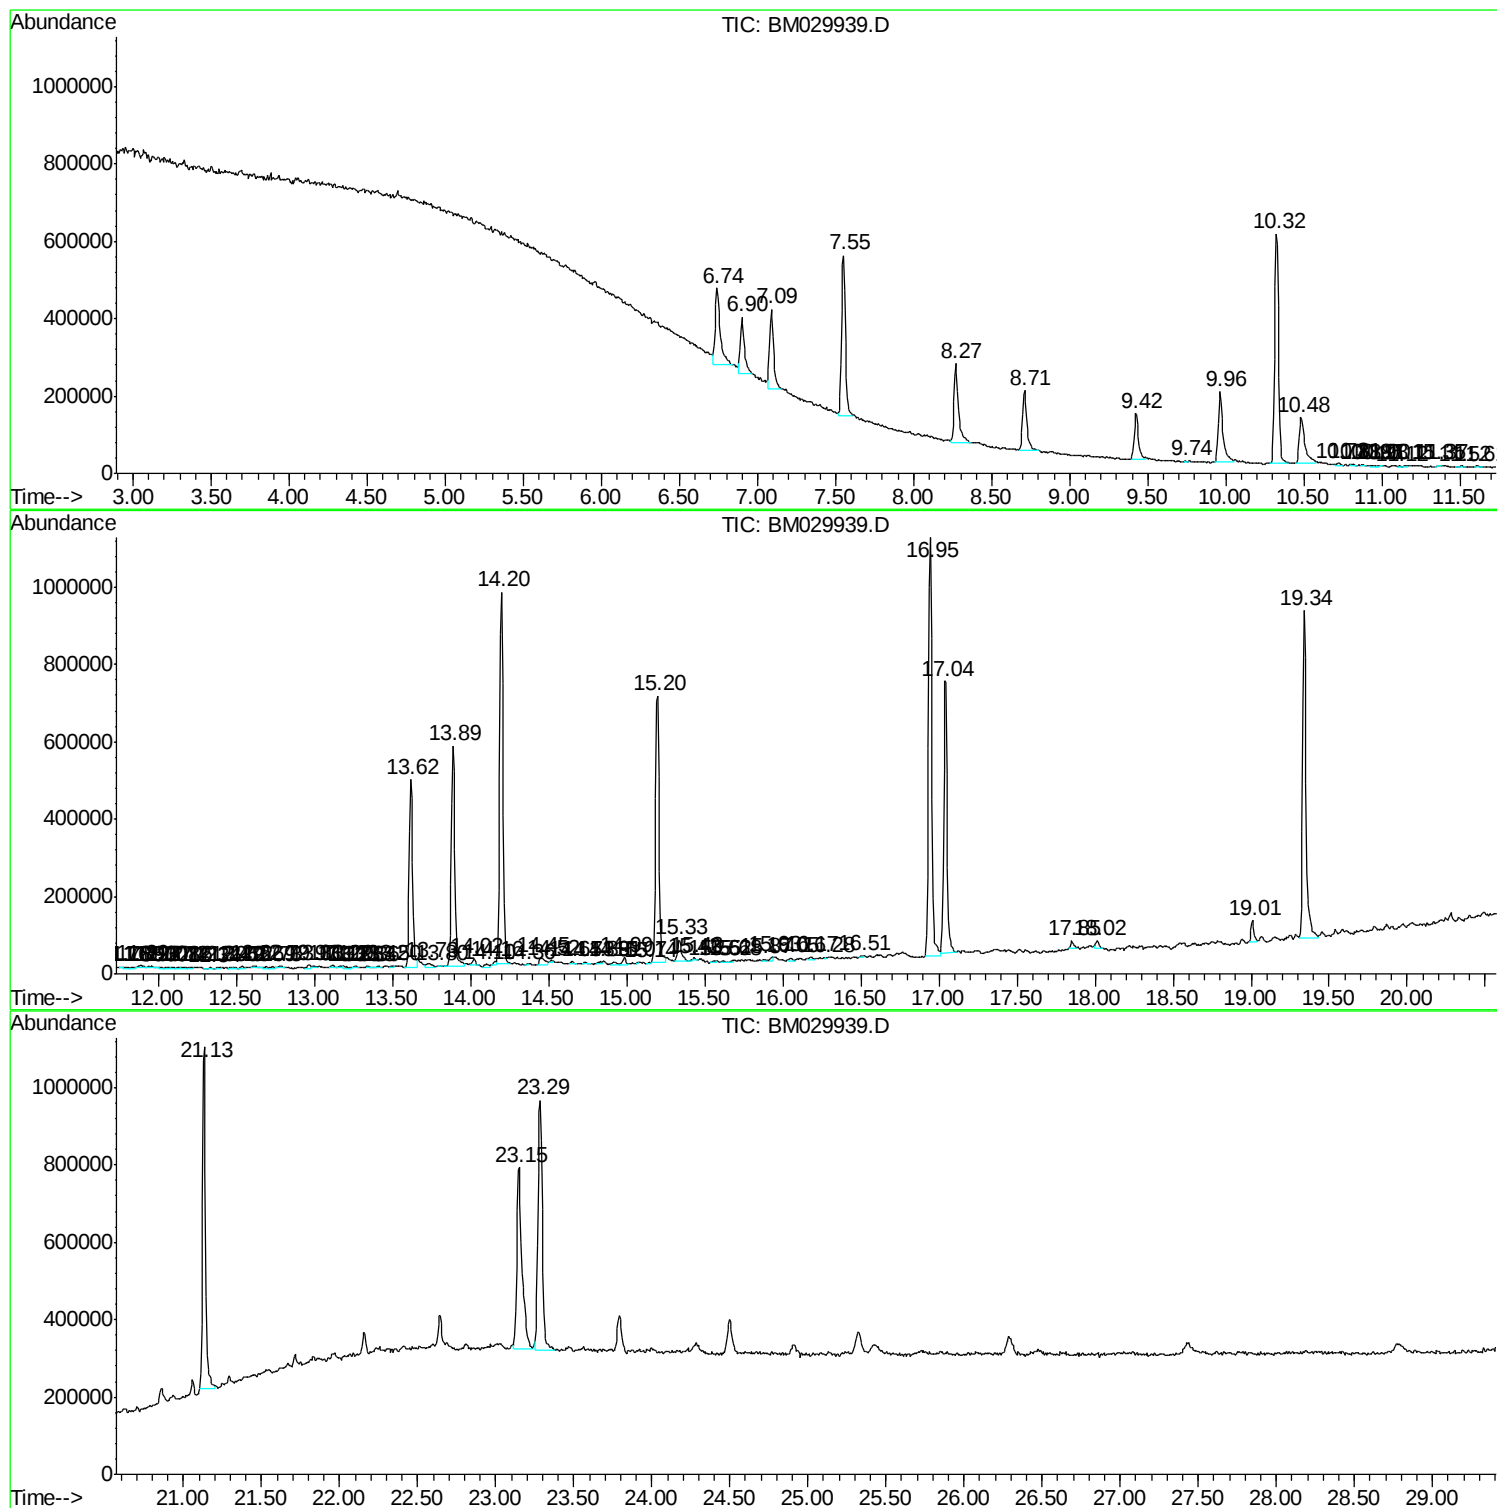

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\\
Data_File : BM029939.D
Acq_On : 11_May, 2021_ 12:244
Operator : CG/JUU
Sample : M2177-033
Misc :
ALS_Vial : 38 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
BG580

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SEAM-EPA-BM050721.M
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
