

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029949.D
 Acq On : 11 May 2021 19:00
 Operator : CG/JU
 Sample : M2341-10
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.781	148	152	158	rVB6	7264	11530	0.61%	0.130%
2	6.816	665	668	670	rBV4	1858	1903	0.10%	0.021%
3	6.881	676	679	681	rBV4	1409	2140	0.11%	0.024%
4	7.545	786	792	819	rBV	377510	738400	39.01%	8.310%
5	8.075	879	882	884	rBV3	1613	1933	0.10%	0.022%
6	8.716	987	991	996	rVB6	1463	2866	0.15%	0.032%
7	10.322	1257	1264	1284	rBV	503665	1055594	55.76%	11.879%
8	10.598	1310	1311	1314	rBV3	2323	2354	0.12%	0.026%
9	11.986	1545	1547	1551	rBV3	1486	2018	0.11%	0.023%
10	14.198	1916	1923	1942	rBV	927796	1547289	81.74%	17.412%
11	14.339	1945	1947	1952	rVB5	1820	2232	0.12%	0.025%
12	14.557	1981	1984	1988	rVB4	1864	2296	0.12%	0.026%
13	14.668	2002	2003	2006	rBV3	2036	2272	0.12%	0.026%
14	15.145	2080	2084	2088	rBV6	1079	2006	0.11%	0.023%
15	16.186	2257	2261	2263	rBV3	1869	2572	0.14%	0.029%
16	16.339	2283	2287	2289	rBV4	1716	2342	0.12%	0.026%
17	16.651	2336	2340	2342	rBV4	1466	2052	0.11%	0.023%
18	16.739	2351	2355	2362	rVB3	3472	5896	0.31%	0.066%
19	16.945	2384	2390	2408	rBV	1001303	1728851	91.33%	19.455%
20	17.574	2495	2497	2501	rBV4	1431	1954	0.10%	0.022%
21	17.856	2541	2545	2546	rBV4	3214	2975	0.16%	0.033%
22	17.874	2546	2548	2552	rBV4	2812	4725	0.25%	0.053%
23	18.503	2653	2655	2658	rBV4	1802	2192	0.12%	0.025%
24	19.145	2762	2764	2767	rBV3	3474	4435	0.23%	0.050%
25	21.133	3097	3102	3117	rBV	1206798	1893033	100.00%	21.303%
26	23.286	3462	3468	3481	rVB2	953467	1860348	98.27%	20.935%


Sum of corrected areas: 8886208

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029949.D
Acq On : 11 May 2021 19:00
Operator : CG/JU
Sample : M2341-10
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

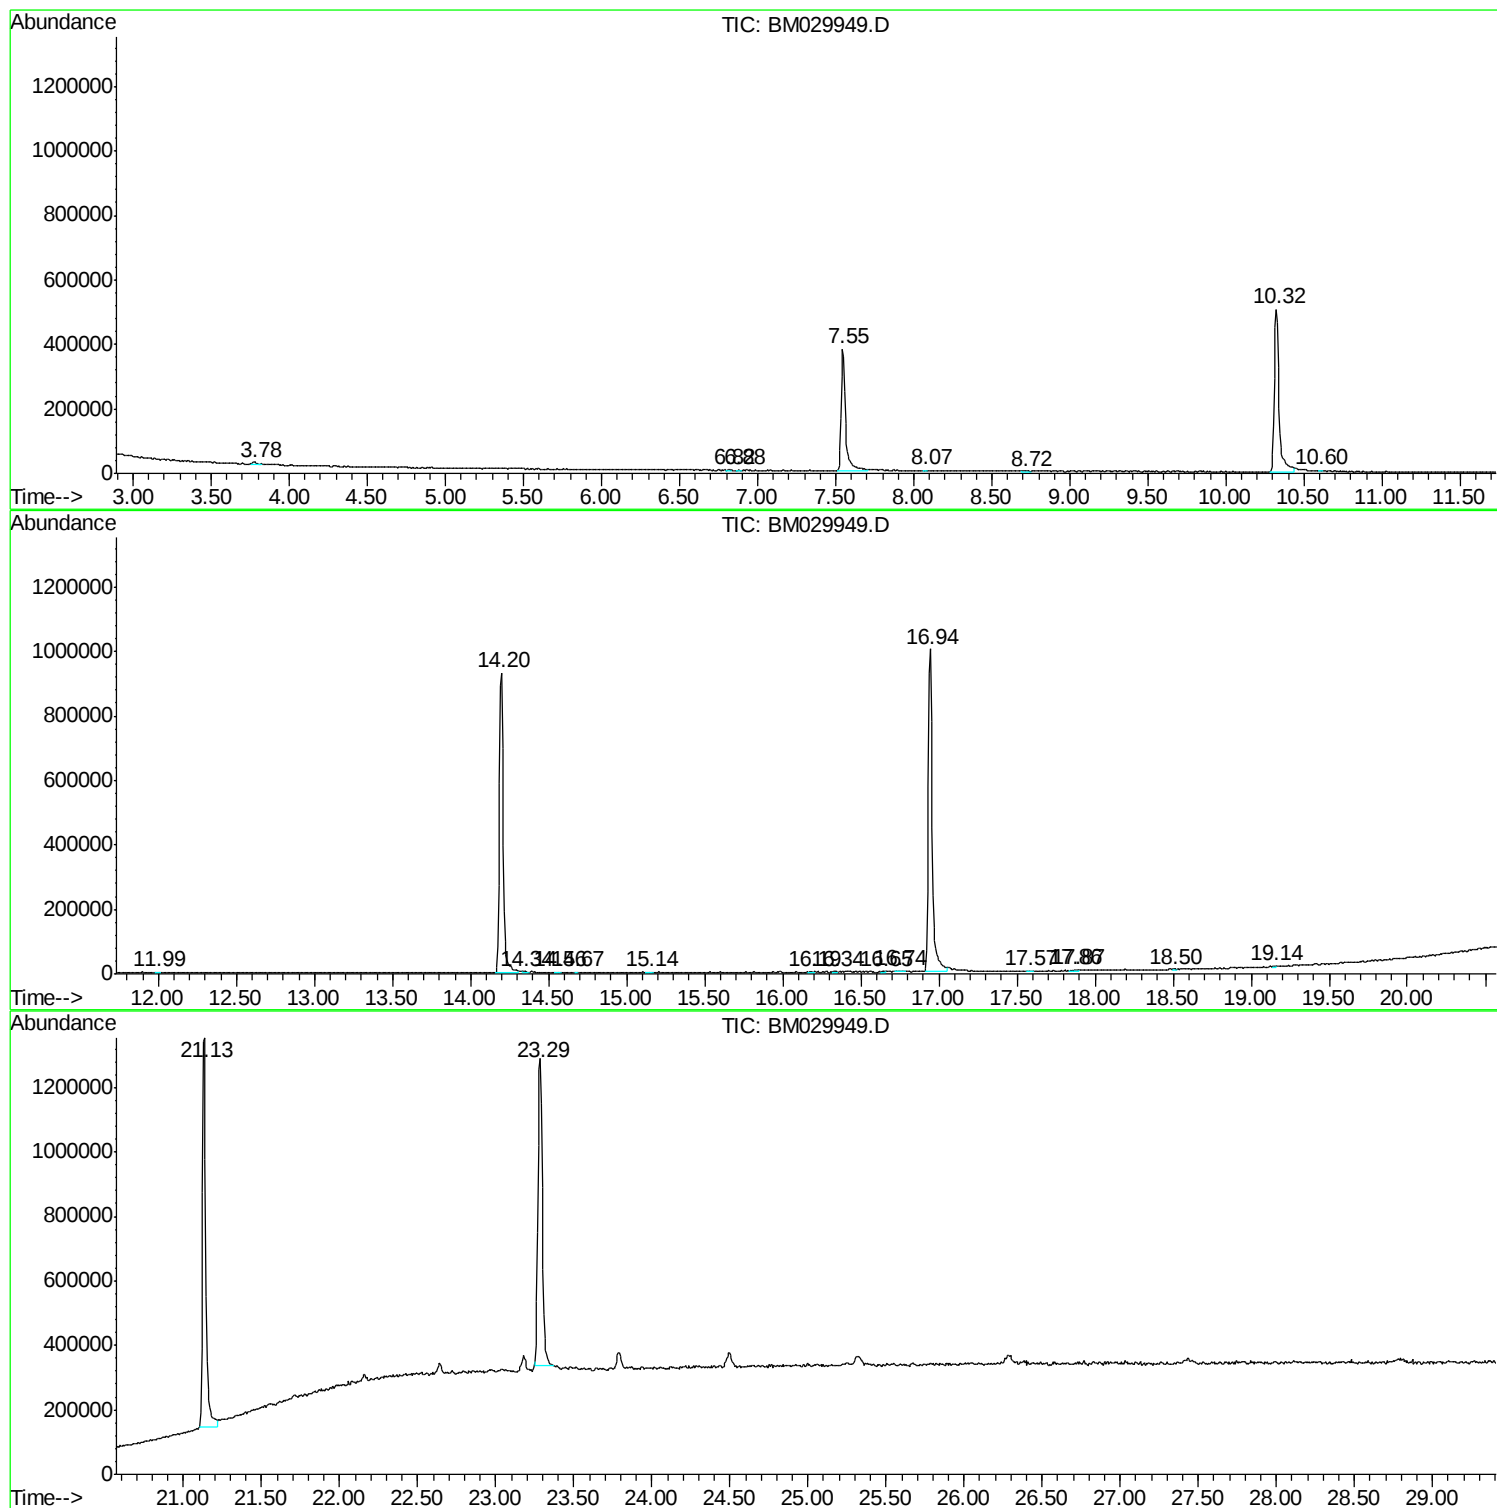

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029949.D
Acq On : 11 May 2021 19:00
Operator : CG/JU
Sample : M2341-10
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029949.D
Acq On : 11 May 2021 19:00
Operator : CG/JU
Sample : M2341-10
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc