

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029972.D
 Acq On : 12 May 2021 09:25
 Operator : CG/JU
 Sample : M2194-02
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	26	29	35	rVB	28156	35988	0.92%	0.099%
2	3.687	131	136	142	rVB	20759	33115	0.85%	0.091%
3	3.769	148	150	155	rVB2	9310	10952	0.28%	0.030%
4	3.875	166	168	173	rVB5	6909	9283	0.24%	0.025%
5	4.693	304	307	312	rVB3	5138	7801	0.20%	0.021%
6	5.622	460	465	478	rVB	39802	74147	1.89%	0.203%
7	5.951	518	521	525	rVB5	6034	7689	0.20%	0.021%
8	6.734	649	654	668	rBV	115029	247422	6.32%	0.679%
9	6.893	675	681	698	rBV	426933	788245	20.14%	2.162%
10	7.081	706	713	725	rBV	535695	937594	23.95%	2.572%
11	7.540	784	791	805	rBV	504349	857429	21.91%	2.352%
12	7.757	825	828	834	rVB3	2574	4724	0.12%	0.013%
13	8.263	907	914	934	rBV	358959	721102	18.42%	1.978%
14	8.698	981	988	1004	rBV	582099	1072631	27.40%	2.942%
15	9.416	1102	1110	1125	rBV	498821	917587	23.44%	2.517%
16	9.739	1158	1165	1170	rBV7	5444	9522	0.24%	0.026%
17	9.951	1195	1201	1222	rBV	595520	1304649	33.33%	3.579%
18	10.316	1255	1263	1274	rBV	776874	1291933	33.01%	3.544%
19	10.498	1288	1294	1303	rBV3	19975	60556	1.55%	0.166%
20	10.992	1376	1378	1384	rBV6	2688	4005	0.10%	0.011%
21	11.328	1432	1435	1441	rVB7	2112	4036	0.10%	0.011%
22	11.433	1446	1453	1457	rBV6	3681	7885	0.20%	0.022%
23	11.933	1533	1538	1542	rBV4	5724	11988	0.31%	0.033%
24	12.804	1681	1686	1690	rVB5	3502	5505	0.14%	0.015%
25	13.057	1721	1729	1733	rBV9	5260	10555	0.27%	0.029%
26	13.504	1801	1805	1808	rBV3	3954	5024	0.13%	0.014%
27	13.610	1817	1823	1836	rBV	1584842	2313976	59.12%	6.348%
28	13.880	1862	1869	1885	rBV	1833033	2622196	66.99%	7.193%
29	14.010	1887	1891	1894	rVB6	5415	8890	0.23%	0.024%
30	14.192	1912	1922	1933	rBV	1187831	1759406	44.95%	4.826%
31	14.298	1937	1940	1943	rVV4	3702	4229	0.11%	0.012%
32	14.463	1962	1968	1976	rBV4	24398	76710	1.96%	0.210%
33	14.639	1995	1998	2002	rVB6	2880	3988	0.10%	0.011%
34	14.792	2021	2024	2029	rVB7	3156	4657	0.12%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
 Data File : BM029972.D
 Acq On : 12 May 2021 09:25
 Operator : CG/JU
 Sample : M2194-02
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

35	15.057	2067	2069	2074	rVB6	5887	7064	0.18%	0.019%
36	15.110	2074	2078	2082	rBV6	6818	12272	0.31%	0.034%
37	15.186	2085	2091	2105	rBV	2183491	3319246	84.80%	9.105%
38	15.327	2109	2115	2128	rVV	657268	1011843	25.85%	2.776%
39	15.427	2129	2132	2143	rVB	30410	58450	1.49%	0.160%
40	15.757	2184	2188	2189	rBV3	4479	5539	0.14%	0.015%
41	15.939	2215	2219	2221	rBV5	3588	6557	0.17%	0.018%
42	15.974	2223	2225	2230	rVB6	9205	10950	0.28%	0.030%
43	16.251	2269	2272	2273	rBV3	5085	4566	0.12%	0.013%
44	16.445	2302	2305	2309	rVB6	8254	11923	0.30%	0.033%
45	16.663	2339	2342	2347	rBV6	8549	14042	0.36%	0.039%
46	16.721	2349	2352	2356	rVV4	6592	11373	0.29%	0.031%
47	16.939	2382	2389	2399	rBV	1294183	1889150	48.27%	5.182%
48	17.039	2399	2406	2425	rVV	2427814	3642956	93.07%	9.993%
49	17.845	2539	2543	2549	rBV5	23939	36690	0.94%	0.101%
50	18.809	2705	2707	2712	rVB6	5379	4153	0.11%	0.011%
51	18.968	2730	2734	2739	rBV	28340	45298	1.16%	0.124%
52	19.133	2759	2762	2765	rBV5	20501	26324	0.67%	0.072%
53	19.221	2774	2777	2781	rBV	20870	25032	0.64%	0.069%
54	19.274	2784	2786	2790	rBV4	6654	9465	0.24%	0.026%
55	19.333	2790	2796	2806	rBV	2825336	3914053	100.00%	10.737%
56	21.127	3096	3101	3111	rBV	1247915	1772067	45.27%	4.861%
57	23.144	3437	3444	3458	rVB2	1907863	3650198	93.26%	10.013%
58	23.274	3460	3466	3476	rVB2	916074	1728970	44.17%	4.743%


Sum of corrected areas: 36453600

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051021\
Data File : BM029972.D
Acq On : 12 May 2021 09:25
Operator : CG/JU
Sample : M2194-02
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARG8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

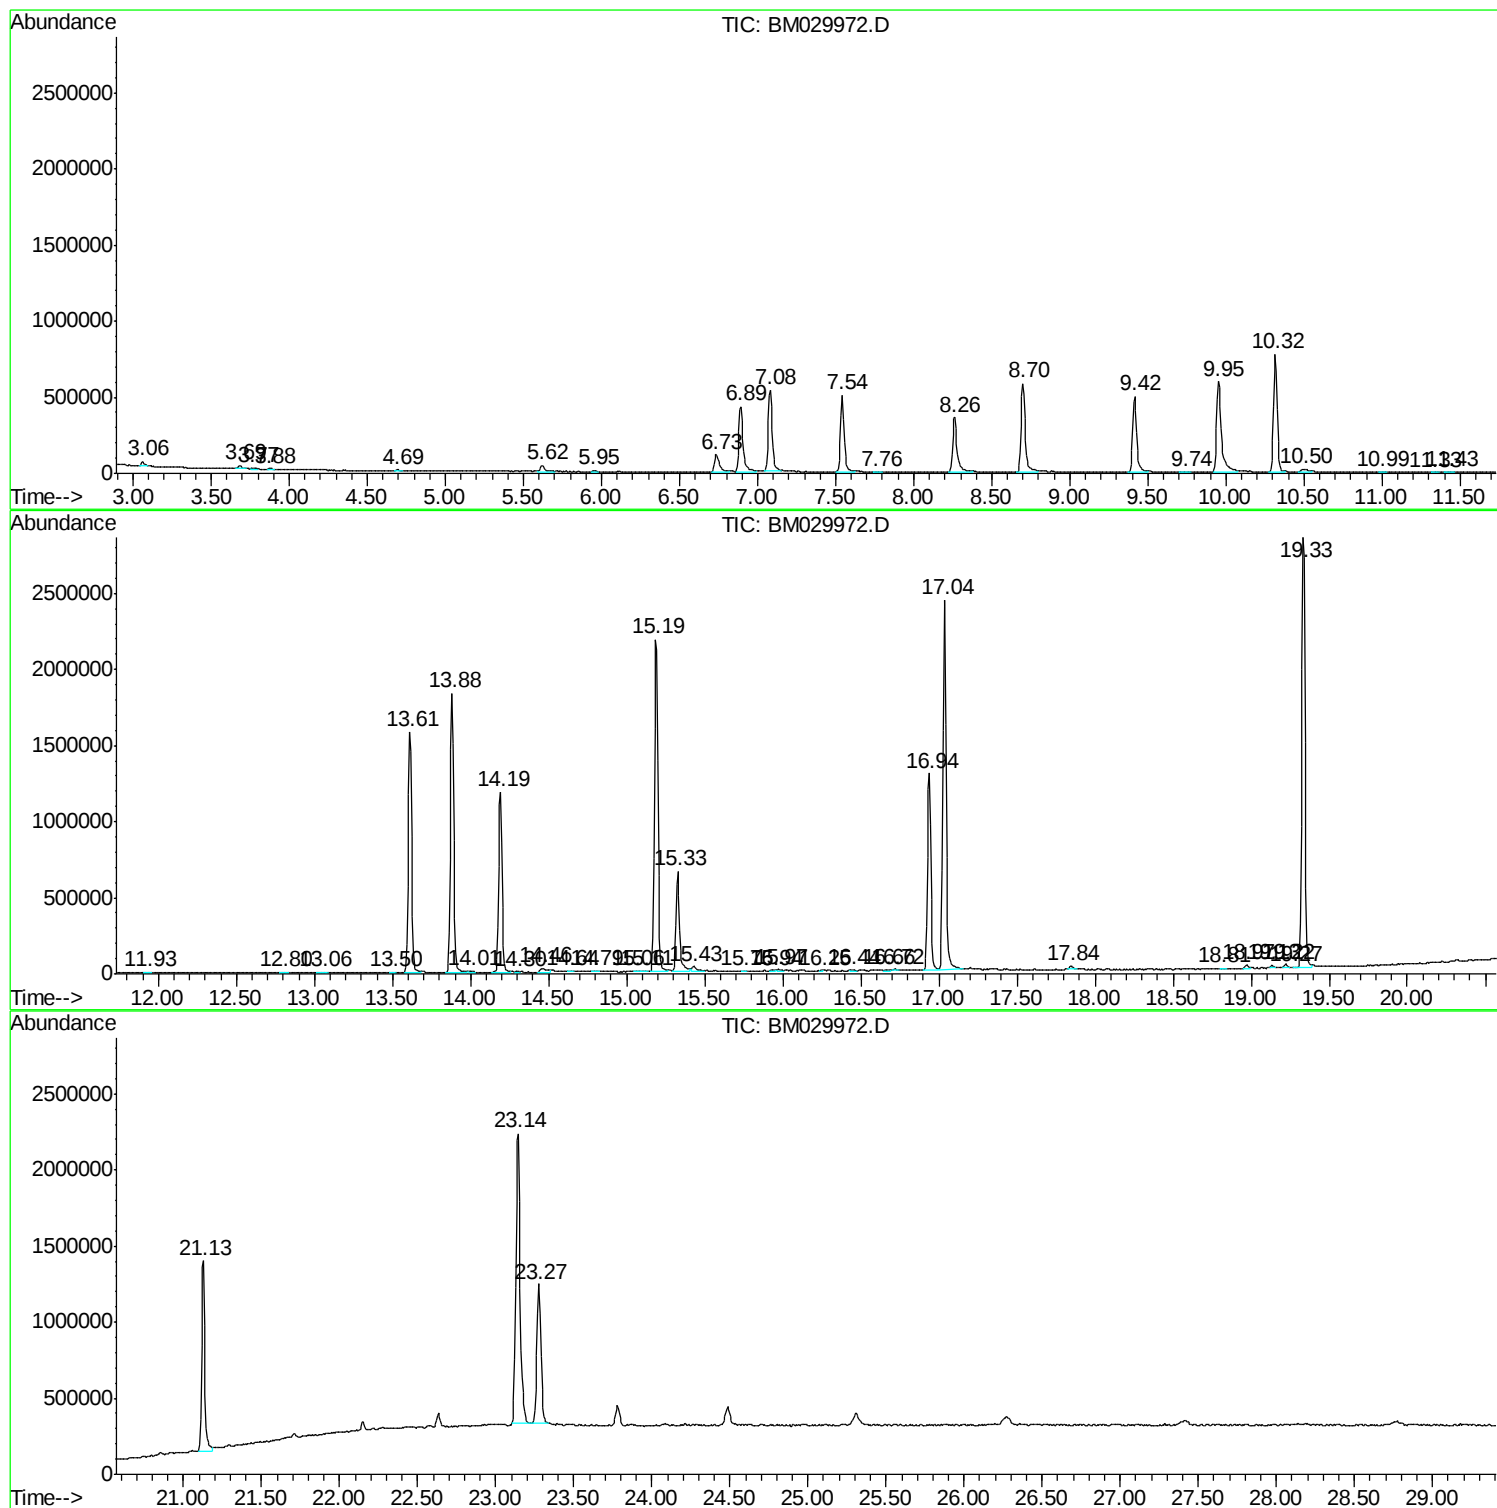

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029972.D
Acq On : 12 May 2021 09:25
Operator : CG/JU
Sample : M2194-02
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARG8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051021\
Data File : BM029972.D
Acq On : 12 May 2021 09:25
Operator : CG/JU
Sample : M2194-02
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARG8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc