

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
 Data File : BM030003.D
 Acq On : 13 May 2021 08:36
 Operator : CG/JU
 Sample : PB136264BL
 Misc :
 ALS Vial : 103 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK264

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	26	29	40	rVB	54326	86223	1.86%	0.170%
2	3.469	97	99	125	rBV	470245	1088784	23.46%	2.148%
3	6.728	646	653	673	rBV	819142	1461548	31.49%	2.883%
4	6.887	674	680	695	rVV	640380	1093568	23.56%	2.157%
5	7.075	706	712	727	rBV	933635	1528750	32.94%	3.015%
6	7.540	784	791	811	rBV	615420	1047302	22.57%	2.066%
7	8.257	906	913	930	rBV	1006852	1804136	38.87%	3.558%
8	8.692	981	987	1009	rBV	828103	1492355	32.16%	2.944%
9	9.410	1101	1109	1126	rBV	714690	1269245	27.35%	2.503%
10	9.945	1192	1200	1219	rBV	970868	1846339	39.78%	3.642%
11	10.310	1255	1262	1271	rBV	928164	1563682	33.69%	3.084%
12	10.463	1281	1288	1310	rBV	893566	1854585	39.96%	3.658%
13	11.922	1532	1536	1544	rBV2	13450	24070	0.52%	0.047%
14	13.610	1816	1823	1841	rBV	2191346	3039786	65.50%	5.996%
15	13.880	1862	1869	1886	rBV	2391184	3528333	76.03%	6.959%
16	14.186	1915	1921	1939	rVB	1428111	2170230	46.76%	4.281%
17	14.427	1955	1962	1990	rBV	345403	1052868	22.69%	2.077%
18	15.186	2079	2091	2109	rBV	3066122	4319949	93.08%	8.521%
19	15.327	2109	2115	2128	rVV	789858	1227817	26.46%	2.422%
20	15.427	2128	2132	2139	rVB2	36911	59072	1.27%	0.117%
21	15.616	2160	2164	2169	rVB4	5193	7853	0.17%	0.015%
22	15.763	2182	2189	2192	rBV6	3330	7124	0.15%	0.014%
23	15.880	2203	2209	2213	rBV7	3004	6363	0.14%	0.013%
24	15.974	2220	2225	2229	rVB5	9915	14539	0.31%	0.029%
25	16.427	2298	2302	2307	rVB4	5627	9321	0.20%	0.018%
26	16.615	2331	2334	2341	rVB6	3971	6585	0.14%	0.013%
27	16.727	2346	2353	2357	rBV4	6250	11049	0.24%	0.022%
28	16.804	2363	2366	2369	rBV4	4043	4677	0.10%	0.009%
29	16.933	2382	2388	2399	rBV	1625848	2332586	50.26%	4.601%
30	17.033	2399	2405	2425	rVV2	3119379	4527044	97.55%	8.929%
31	17.498	2481	2484	2488	rVB6	5536	6441	0.14%	0.013%
32	18.451	2642	2646	2648	rBV3	5211	5411	0.12%	0.011%
33	18.968	2730	2734	2740	rBV2	26099	40860	0.88%	0.081%
34	19.221	2773	2777	2780	rBV	23673	28891	0.62%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030003.D
Acq On : 13 May 2021 08:36
Operator : CG/JU
Sample : PB136264BL
Misc :
ALS Vial : 103 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION

35	19.333	2790	2796	2805	rBV	3457893	4640922	100.00%	9.154%
36	21.127	3096	3101	3111	rBV	1414306	1917844	41.32%	3.783%
37	23.144	3437	3444	3459	rBV2	2017533	3715387	80.06%	7.328%
38	23.280	3461	3467	3479	rVB	1005928	1858030	40.04%	3.665%


Sum of corrected areas: 50699569

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030003.D
Acq On : 13 May 2021 08:36
Operator : CG/JU
Sample : PB136264BL
Misc :
ALS Vial : 103 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

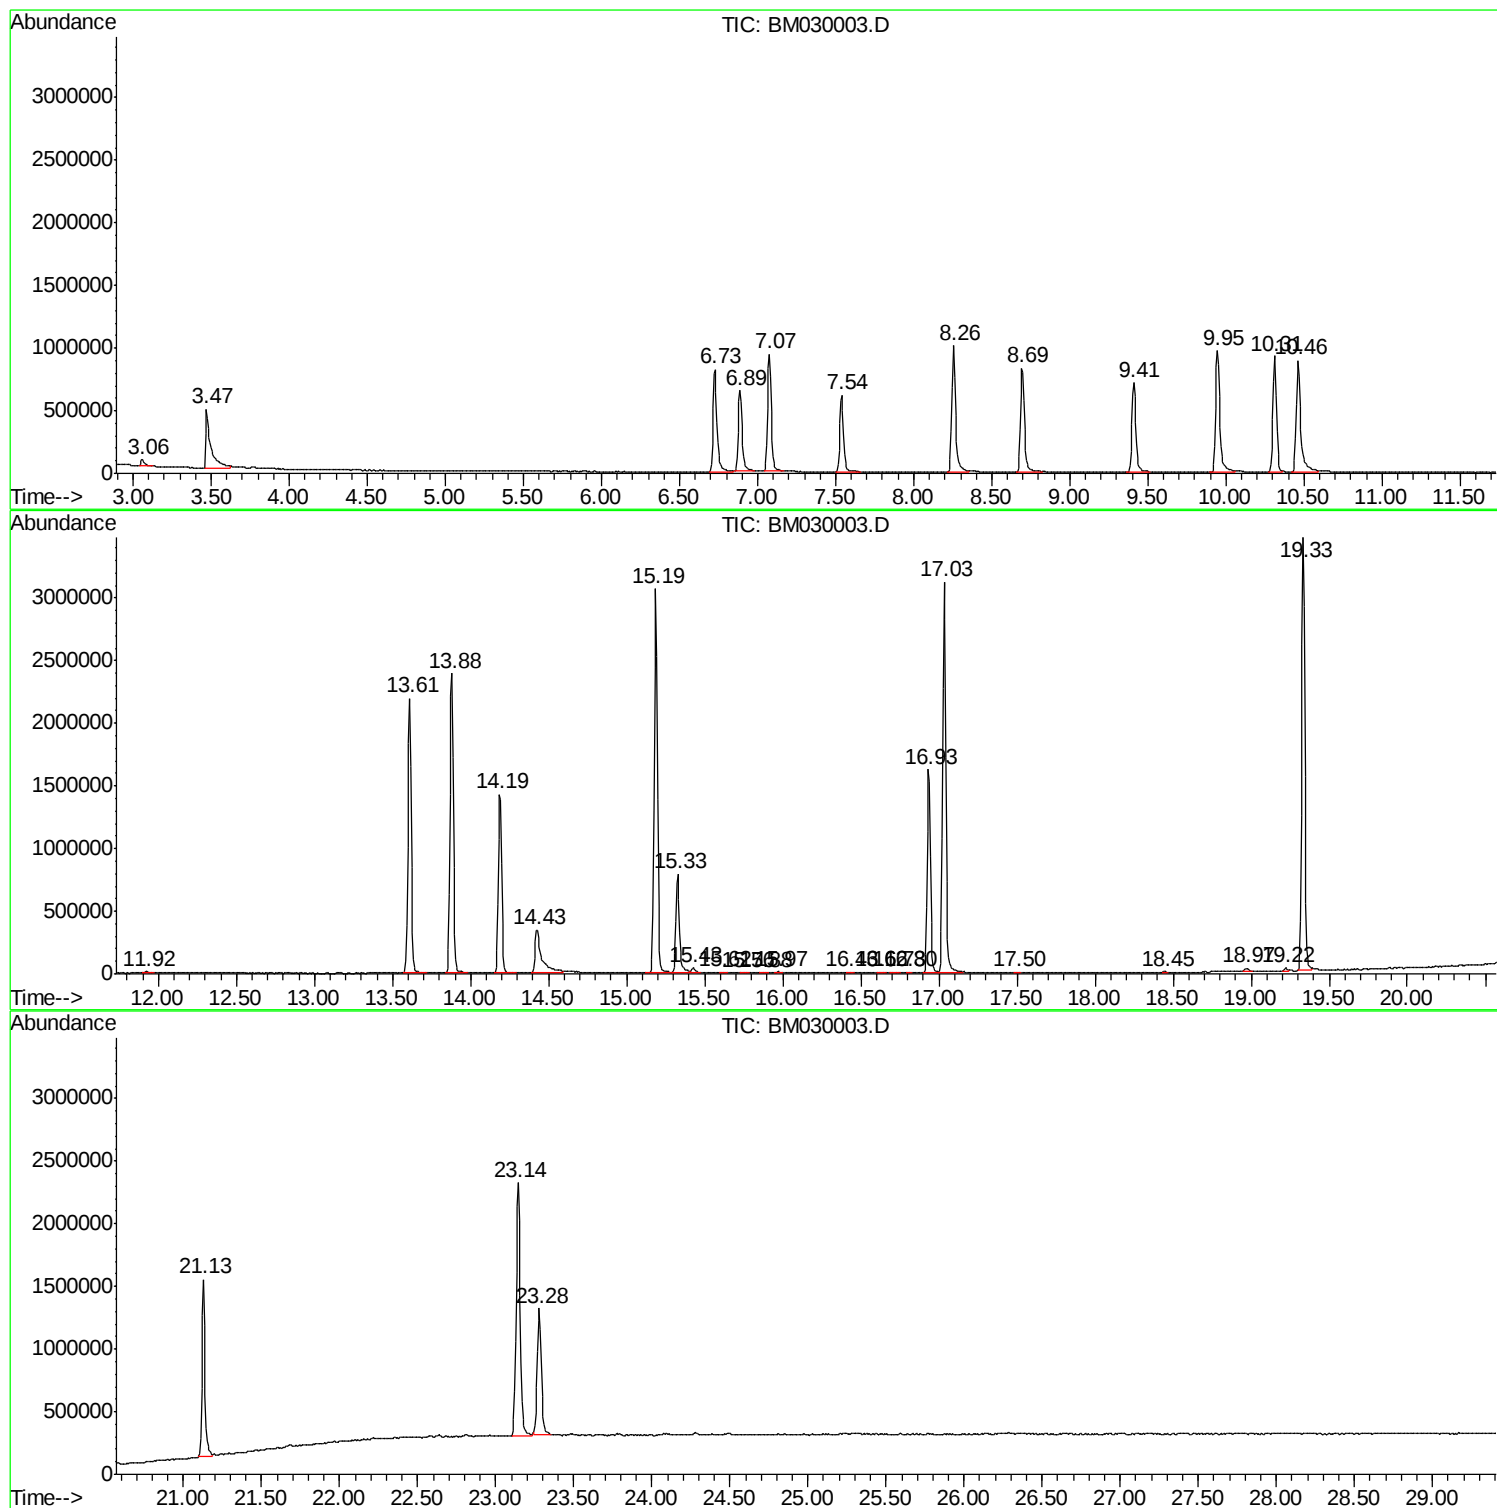

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030003.D
Acq On : 13 May 2021 08:36
Operator : CG/JU
Sample : PB136264BL
Misc :
ALS Vial : 103 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030003.D
Acq On : 13 May 2021 08:36
Operator : CG/JU
Sample : PB136264BL
Misc :
ALS Vial : 103 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK264

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc