

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
 Data File : BM030005.D
 Acq On : 13 May 2021 10:41
 Operator : CG/JU
 Sample : PB136351BL
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK351

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.057	26	29	35	rBV	45768	60606	1.62%	0.145%
2	3.469	97	99	124	rBV	373088	856137	22.89%	2.042%
3	6.728	647	653	671	rBV	682337	1223970	32.72%	2.919%
4	6.887	674	680	701	rVV	531897	932462	24.93%	2.224%
5	7.075	706	712	736	rVB	768329	1313167	35.11%	3.131%
6	7.540	784	791	802	rBV	526753	877965	23.47%	2.094%
7	8.257	906	913	935	rBV	814141	1520634	40.66%	3.626%
8	8.698	981	988	1014	rBV	676233	1279556	34.21%	3.051%
9	9.410	1103	1109	1128	rBV	585546	1066696	28.52%	2.544%
10	9.945	1194	1200	1221	rBV	758214	1509537	40.36%	3.600%
11	10.310	1255	1262	1272	rBV	774763	1324138	35.40%	3.158%
12	10.463	1281	1288	1314	rBV	667586	1516574	40.55%	3.616%
13	10.928	1362	1367	1370	rBV4	2037	4238	0.11%	0.010%
14	11.933	1532	1538	1546	rBV4	7607	17457	0.47%	0.042%
15	13.610	1816	1823	1834	rBV	1756792	2464962	65.90%	5.878%
16	13.880	1862	1869	1882	rBV	1917415	2878876	76.97%	6.865%
17	14.186	1915	1921	1938	rBV	1175182	1781623	47.63%	4.248%
18	14.433	1956	1963	1985	rBV	212355	729589	19.51%	1.740%
19	15.186	2084	2091	2107	rBV	2431005	3502876	93.65%	8.353%
20	15.327	2109	2115	2128	rVV	623212	969794	25.93%	2.313%
21	15.433	2128	2133	2139	rVB	27506	50985	1.36%	0.122%
22	15.974	2219	2225	2229	rBV5	7598	13253	0.35%	0.032%
23	16.621	2330	2335	2339	rBV6	2963	4543	0.12%	0.011%
24	16.939	2382	2389	2399	rBV	1242513	1855044	49.60%	4.424%
25	17.033	2399	2405	2430	rVB2	2399749	3601532	96.29%	8.588%
26	18.898	2718	2722	2725	rVB5	3116	4125	0.11%	0.010%
27	18.974	2730	2735	2741	rBV	19746	36407	0.97%	0.087%
28	19.227	2774	2778	2782	rBV	15467	20081	0.54%	0.048%
29	19.333	2790	2796	2816	rBV	2703645	3740270	100.00%	8.919%
30	21.127	3096	3101	3113	rBV	1190506	1675330	44.79%	3.995%
31	23.144	3437	3444	3457	rBV2	1885761	3424313	91.55%	8.166%
32	23.280	3461	3467	3476	rVB2	909812	1678920	44.89%	4.004%

LSC Area Percent Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030005.D
Acq On : 13 May 2021 10:41
Operator : CG/JU
Sample : PB136351BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK351

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Title : SVOA CALIBRATION


Sum of corrected areas: 41935660

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030005.D
Acq On : 13 May 2021 10:41
Operator : CG/JU
Sample : PB136351BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK351

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

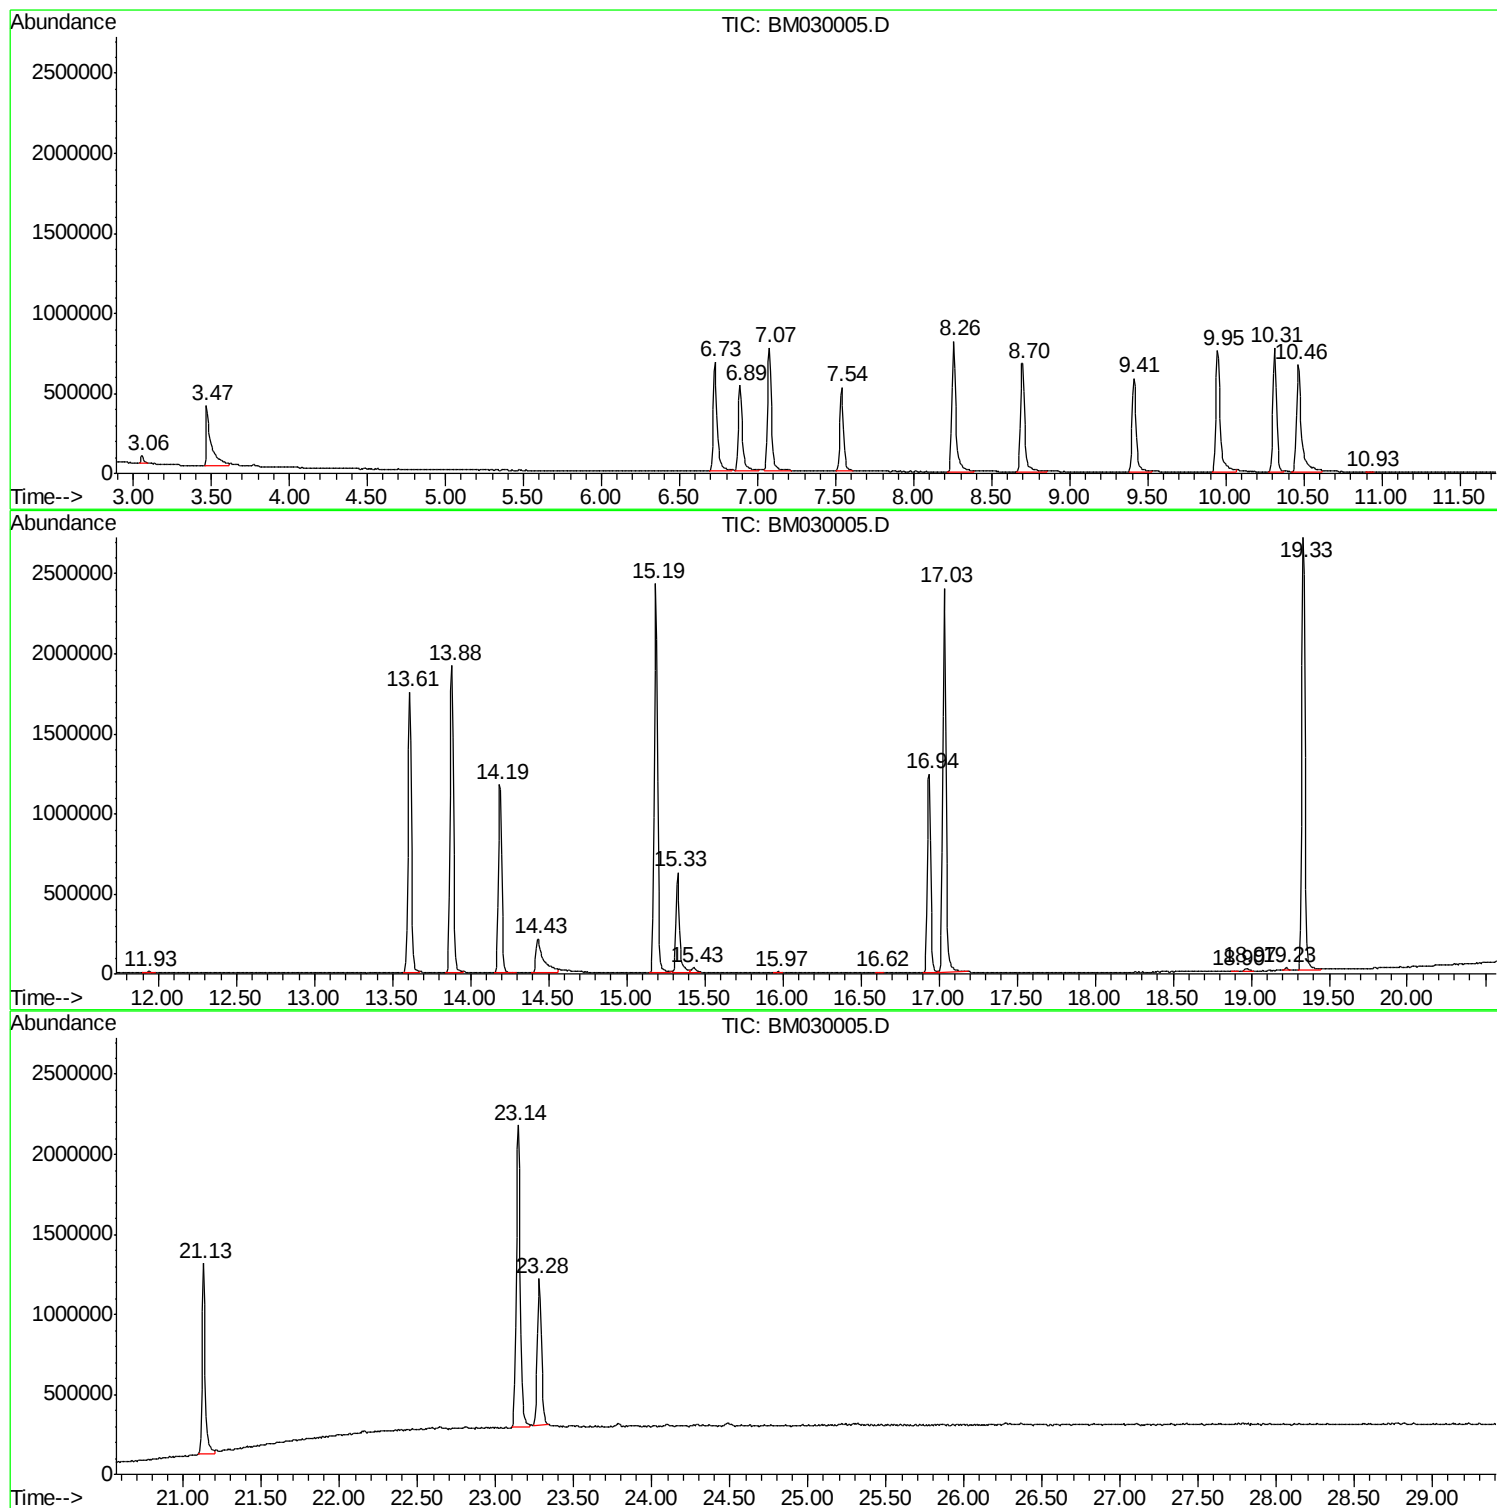

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030005.D
Acq On : 13 May 2021 10:41
Operator : CG/JU
Sample : PB136351BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK351

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051021\
Data File : BM030005.D
Acq On : 13 May 2021 10:41
Operator : CG/JU
Sample : PB136351BL
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK351

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc