

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051022\
 Data File : BM034966.D
 Acq On : 10 May 2022 16:48
 Operator : CG/JU
 Sample : PB144571BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	43	47	56	rVB	55910	77085	1.66%	0.147%
2	3.775	113	117	135	rBV	704541	1083398	23.33%	2.062%
3	4.111	170	174	182	rVB	18899	30646	0.66%	0.058%
4	7.081	672	679	696	rVB	824657	1278381	27.53%	2.434%
5	7.246	701	707	720	rVB	633251	1014458	21.85%	1.931%
6	7.452	734	742	753	rBV	866137	1351780	29.11%	2.573%
7	7.922	814	822	830	rBV	816819	1292693	27.84%	2.461%
8	8.622	933	941	954	rBV	1018340	1648050	35.49%	3.137%
9	9.075	1011	1018	1031	rBV	842011	1357512	29.23%	2.584%
10	9.804	1134	1142	1152	rBV	674668	1130312	24.34%	2.152%
11	10.340	1226	1233	1249	rBV	997135	1642126	35.36%	3.126%
12	10.722	1289	1298	1308	rBV	1197635	1966191	42.34%	3.743%
13	10.851	1313	1320	1330	rBV	1045633	1782226	38.38%	3.393%
14	12.310	1561	1568	1574	rBV2	18742	31323	0.67%	0.060%
15	12.904	1664	1669	1674	rBV7	2356	5833	0.13%	0.011%
16	13.963	1842	1849	1867	rBV	2143041	2920909	62.90%	5.560%
17	14.245	1889	1897	1905	rBV	2260084	3177176	68.42%	6.048%
18	14.551	1943	1949	1961	rVV	1937624	2872530	61.86%	5.468%
19	14.645	1961	1965	1969	rVB5	4040	5641	0.12%	0.011%
20	14.739	1974	1981	2001	rBV	816856	1308358	28.18%	2.491%
21	15.369	2084	2088	2093	rVB6	4266	5773	0.12%	0.011%
22	15.545	2111	2118	2125	rBV	2926935	4117595	88.67%	7.838%
23	15.657	2130	2137	2148	rBV	931418	1275164	27.46%	2.427%
24	15.781	2154	2158	2163	rVB2	32252	47185	1.02%	0.090%
25	16.328	2247	2251	2258	rVB3	8773	13264	0.29%	0.025%
26	16.810	2331	2333	2338	rVB4	4508	6044	0.13%	0.012%
27	16.969	2358	2360	2366	rBV5	3727	5373	0.12%	0.010%
28	17.292	2409	2415	2425	rBV	2384082	3346253	72.06%	6.370%
29	17.392	2425	2432	2448	rVB	3189417	4452557	95.89%	8.476%
30	18.198	2564	2569	2573	rBV7	6258	10871	0.23%	0.021%
31	18.463	2612	2614	2619	rBV6	2698	4722	0.10%	0.009%
32	18.833	2675	2677	2681	rVB4	4537	4799	0.10%	0.009%
33	19.192	2734	2738	2739	rBV4	4229	5366	0.12%	0.010%
34	19.251	2743	2748	2753	rBV2	33540	48865	1.05%	0.093%
35	19.316	2755	2759	2763	rBV	29567	42945	0.92%	0.082%
36	19.686	2815	2822	2836	rBV	3448216	4643591	100.00%	8.839%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051022\
Data File : BM034966.D
Acq On : 10 May 2022 16:48
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Title : SVOA CALIBRATION

37	21.474	3121	3126	3133	rBV	2211043	2770311	59.66%	5.274%
38	23.704	3498	3505	3514	rBV2	1757370	3379946	72.79%	6.434%
39	23.856	3525	3531	3542	rVB2	1167536	2375167	51.15%	4.521%


Sum of corrected areas: 52532419

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051022\
Data File : BM034966.D
Acq On : 10 May 2022 16:48
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

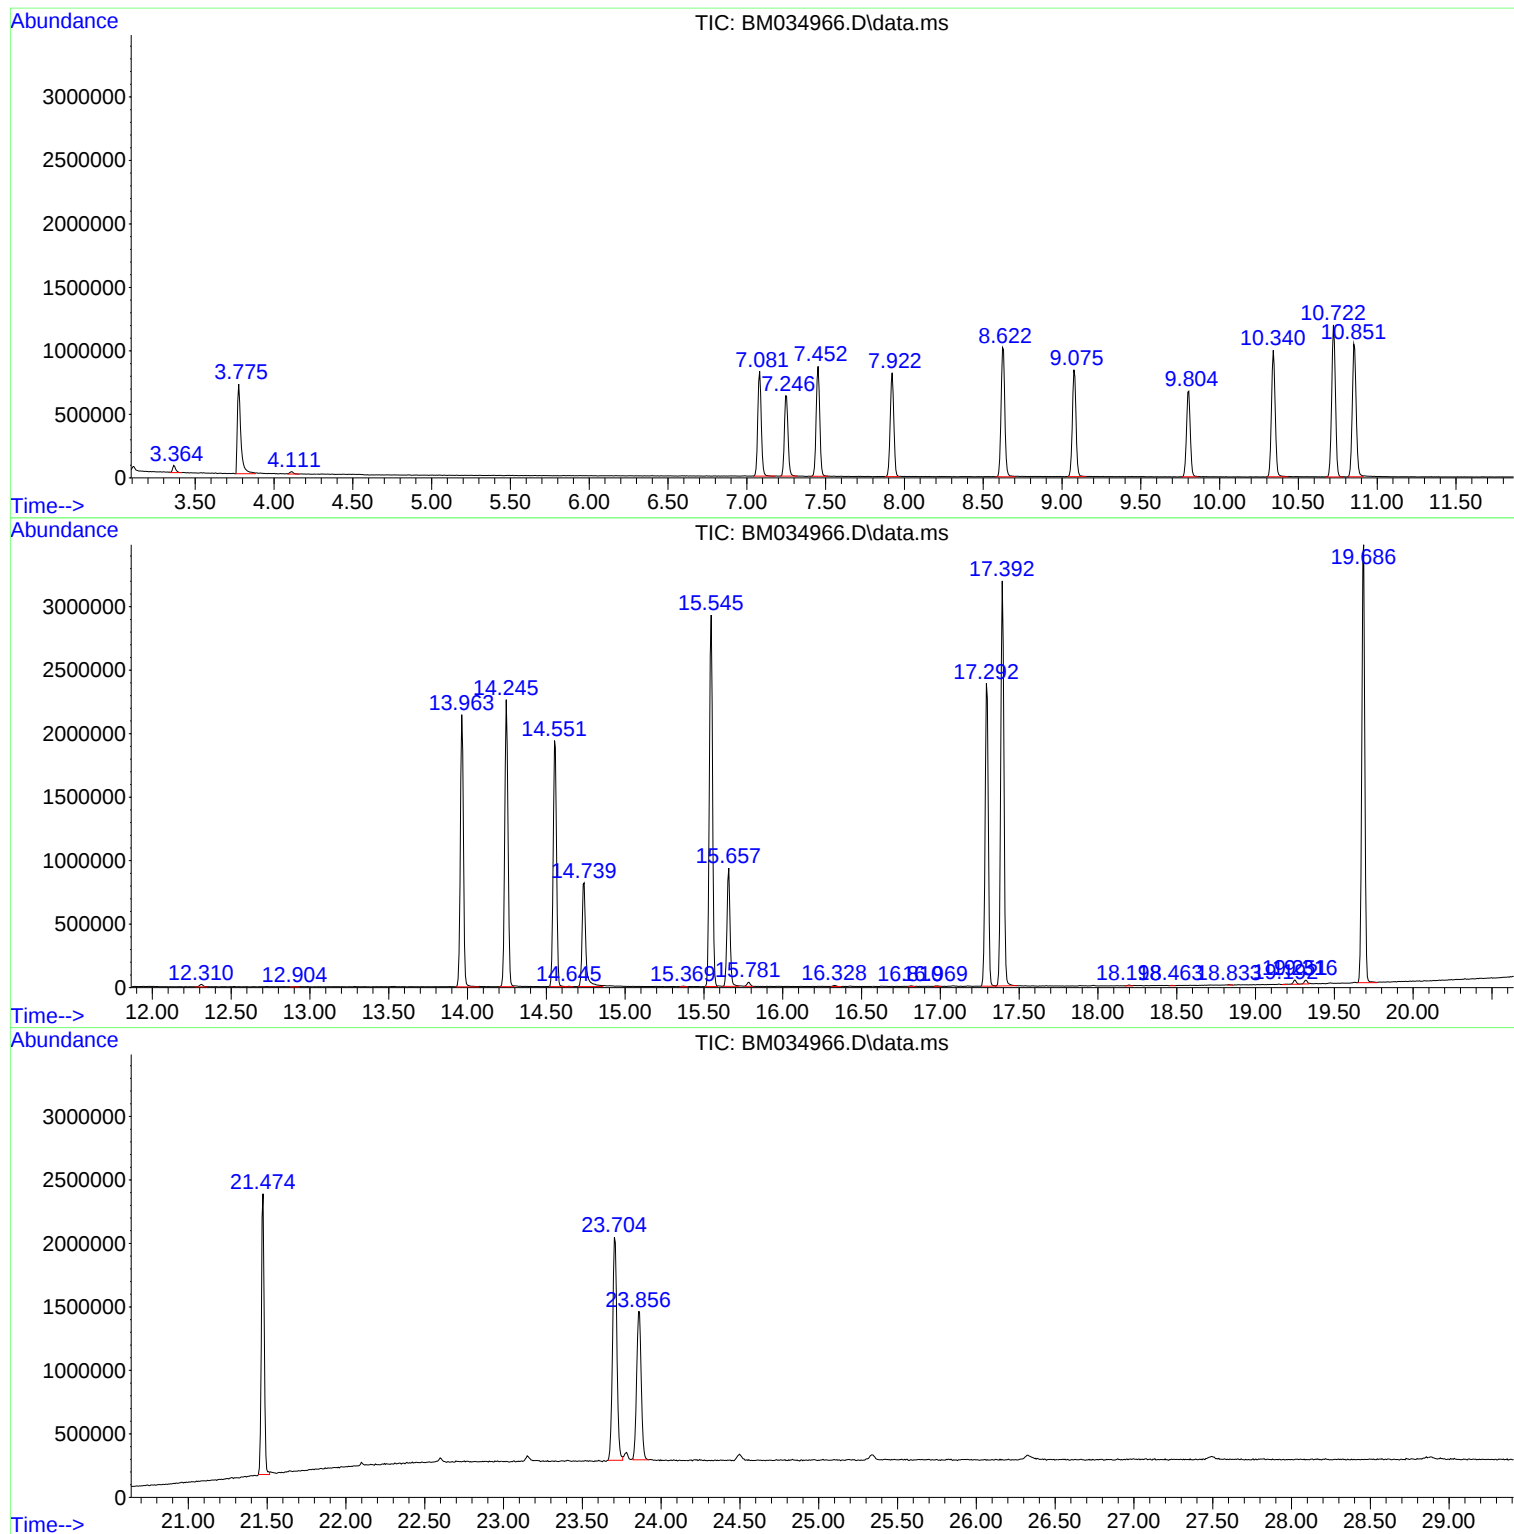

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051022\
Data File : BM034966.D
Acq On : 10 May 2022 16:48
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051022\
Data File : BM034966.D
Acq On : 10 May 2022 16:48
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------