

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005382.D
 Acq On : 11 May 2016 10:13
 Operator : UM/SJ
 Sample : H2888-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WX9

Quant Time: May 12 03:31:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 02:20:05 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	113408	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	576851	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	377837	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	871680	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	780743	20.00	ng/ul	0.00
83) Perylene-d12	23.61	264	644880	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	8983	3.72	ng/uL	0.00
5) Phenol-d5	6.93	99	224509	21.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	141090	24.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	178226	22.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	197548	23.24	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	98408	23.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	115709	24.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	196293	22.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	286965	27.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	739690	24.42	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	844819	23.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	115845	20.95	ng/ul	0.00
57) Fluorene-d10	15.40	176	610518	23.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	117987	24.06	ng/ul	0.00
70) Anthracene-d10	17.25	188	962028	24.97	ng/ul	0.00
76) Pyrene-d10	19.55	212	1046277	29.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	743843	26.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.86	163	138620	4.58	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005382.D
Acq On : 11 May 2016 10:13
Operator : UM/SJ
Sample : H2888-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WX9

Quant Time: May 12 03:31:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 02:20:05 2016
Response via : Initial Calibration

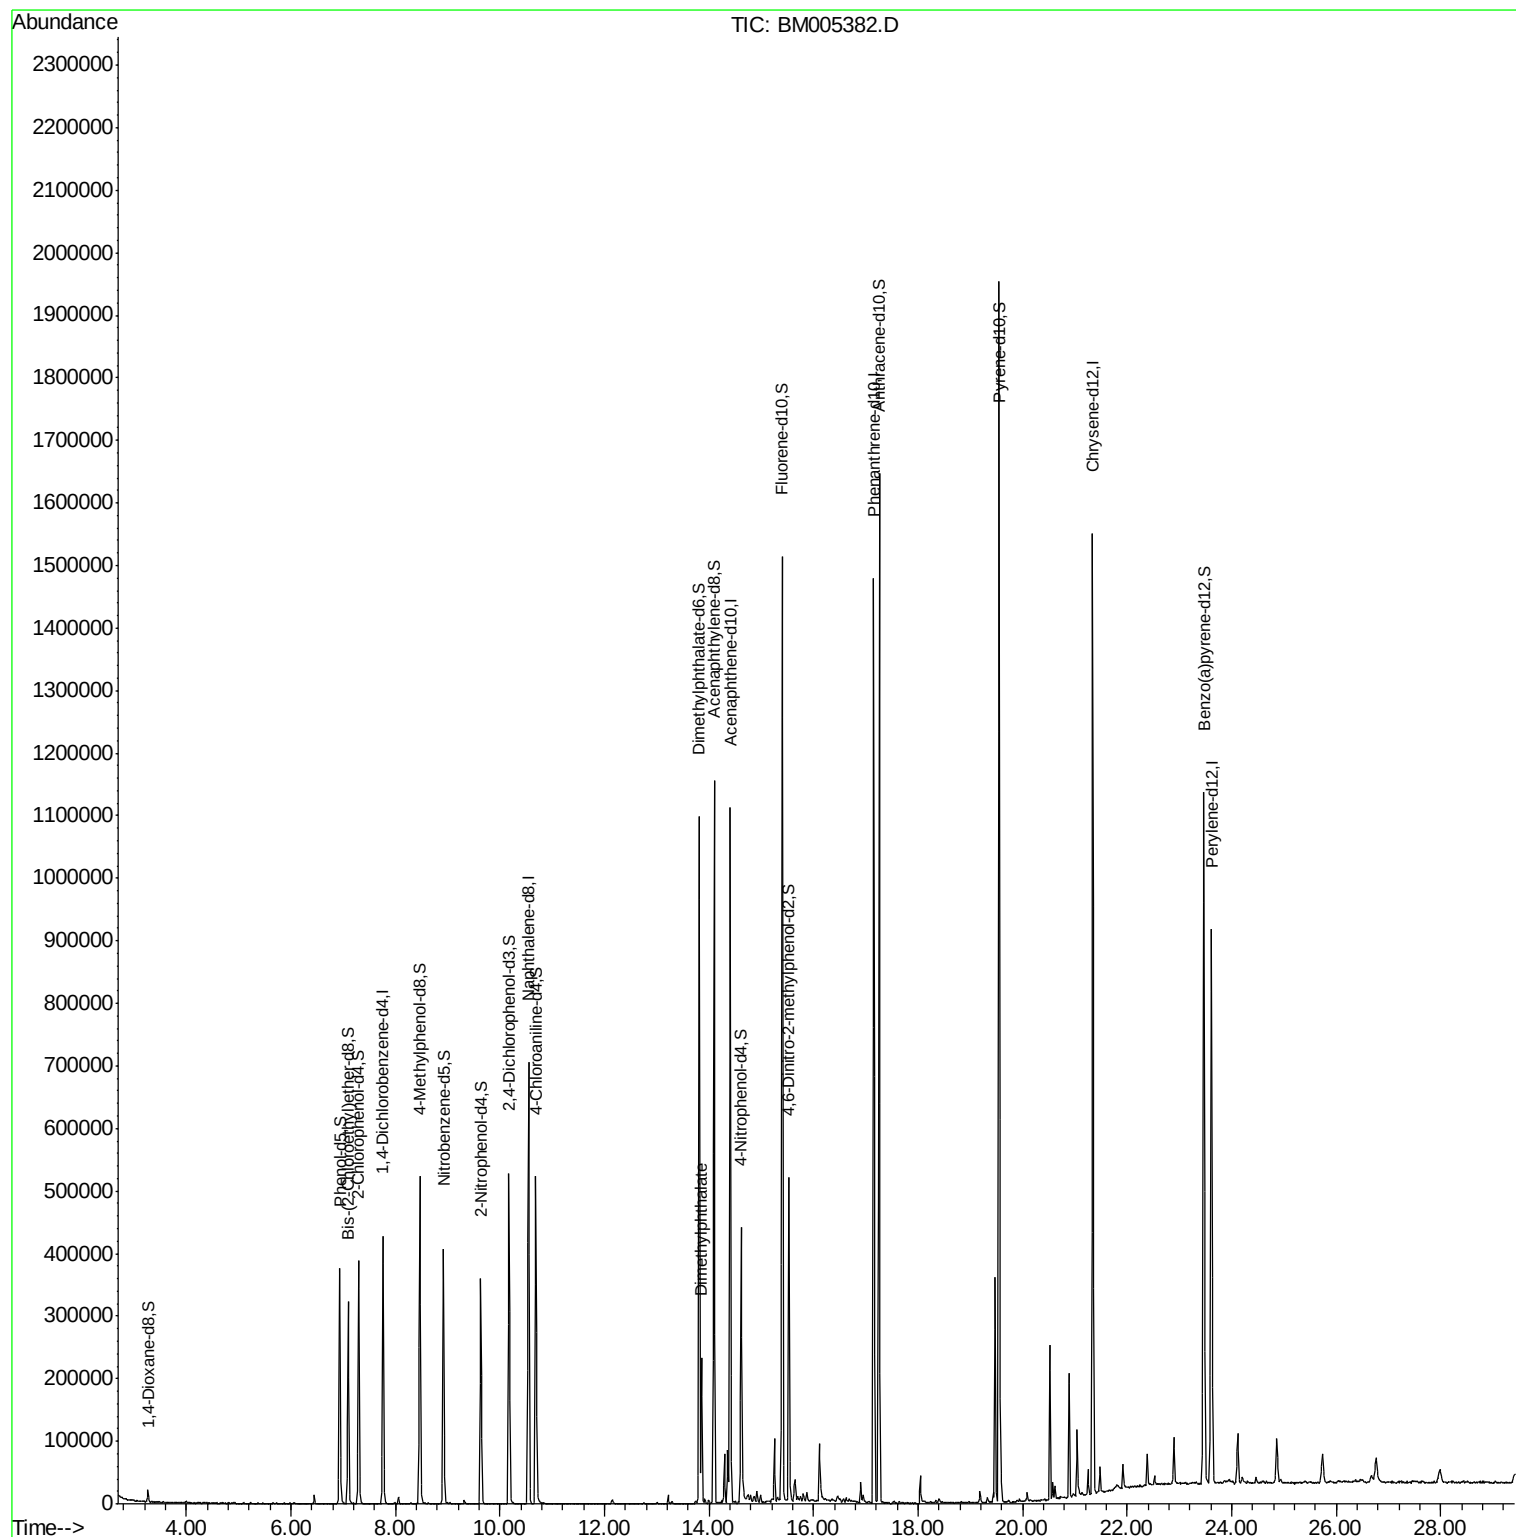

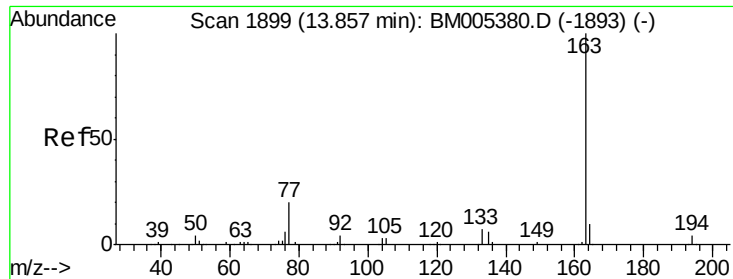

#44

Dimethylphthalate

Concen: 4.58 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. 0.00 min

Lab File: BM005382.D


Acq: 11 May 2016 10:13

Instrument :

BNA_M

ClientSampleId :

D9WX9

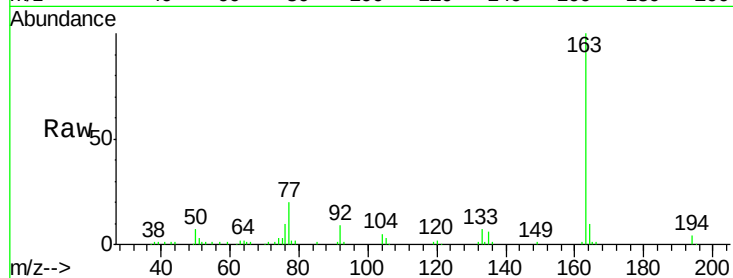

Tgt Ion:	163	Resp:	138620
Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.4	5.0
164	10.0	7.9	11.9

