

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005383.D
 Acq On : 11 May 2016 11:35
 Operator : UM/SJ
 Sample : H2888-18
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WY0

Quant Time: May 12 03:31:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 02:20:05 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	113000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	552707	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	368173	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	875077	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	958311	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	810996	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	8435	3.51	ng/uL	0.00
5) Phenol-d5	6.93	99	204562	19.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	125051	21.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	159538	20.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	178218	21.04	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	86227	21.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.63	143	102689	22.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	171509	20.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.69	131	254012	25.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.81	166	669348	22.68	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	762533	22.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	105248	19.54	ng/ul	0.00
57) Fluorene-d10	15.40	176	563792	22.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	103400	21.01	ng/ul	0.00
70) Anthracene-d10	17.25	188	889274	22.99	ng/ul	0.00
76) Pyrene-d10	19.55	212	1054754	23.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	852975	23.76	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.86	163	117154	3.97 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005383.D
Acq On : 11 May 2016 11:35
Operator : UM/SJ
Sample : H2888-18
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WY0

Quant Time: May 12 03:31:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 02:20:05 2016
Response via : Initial Calibration

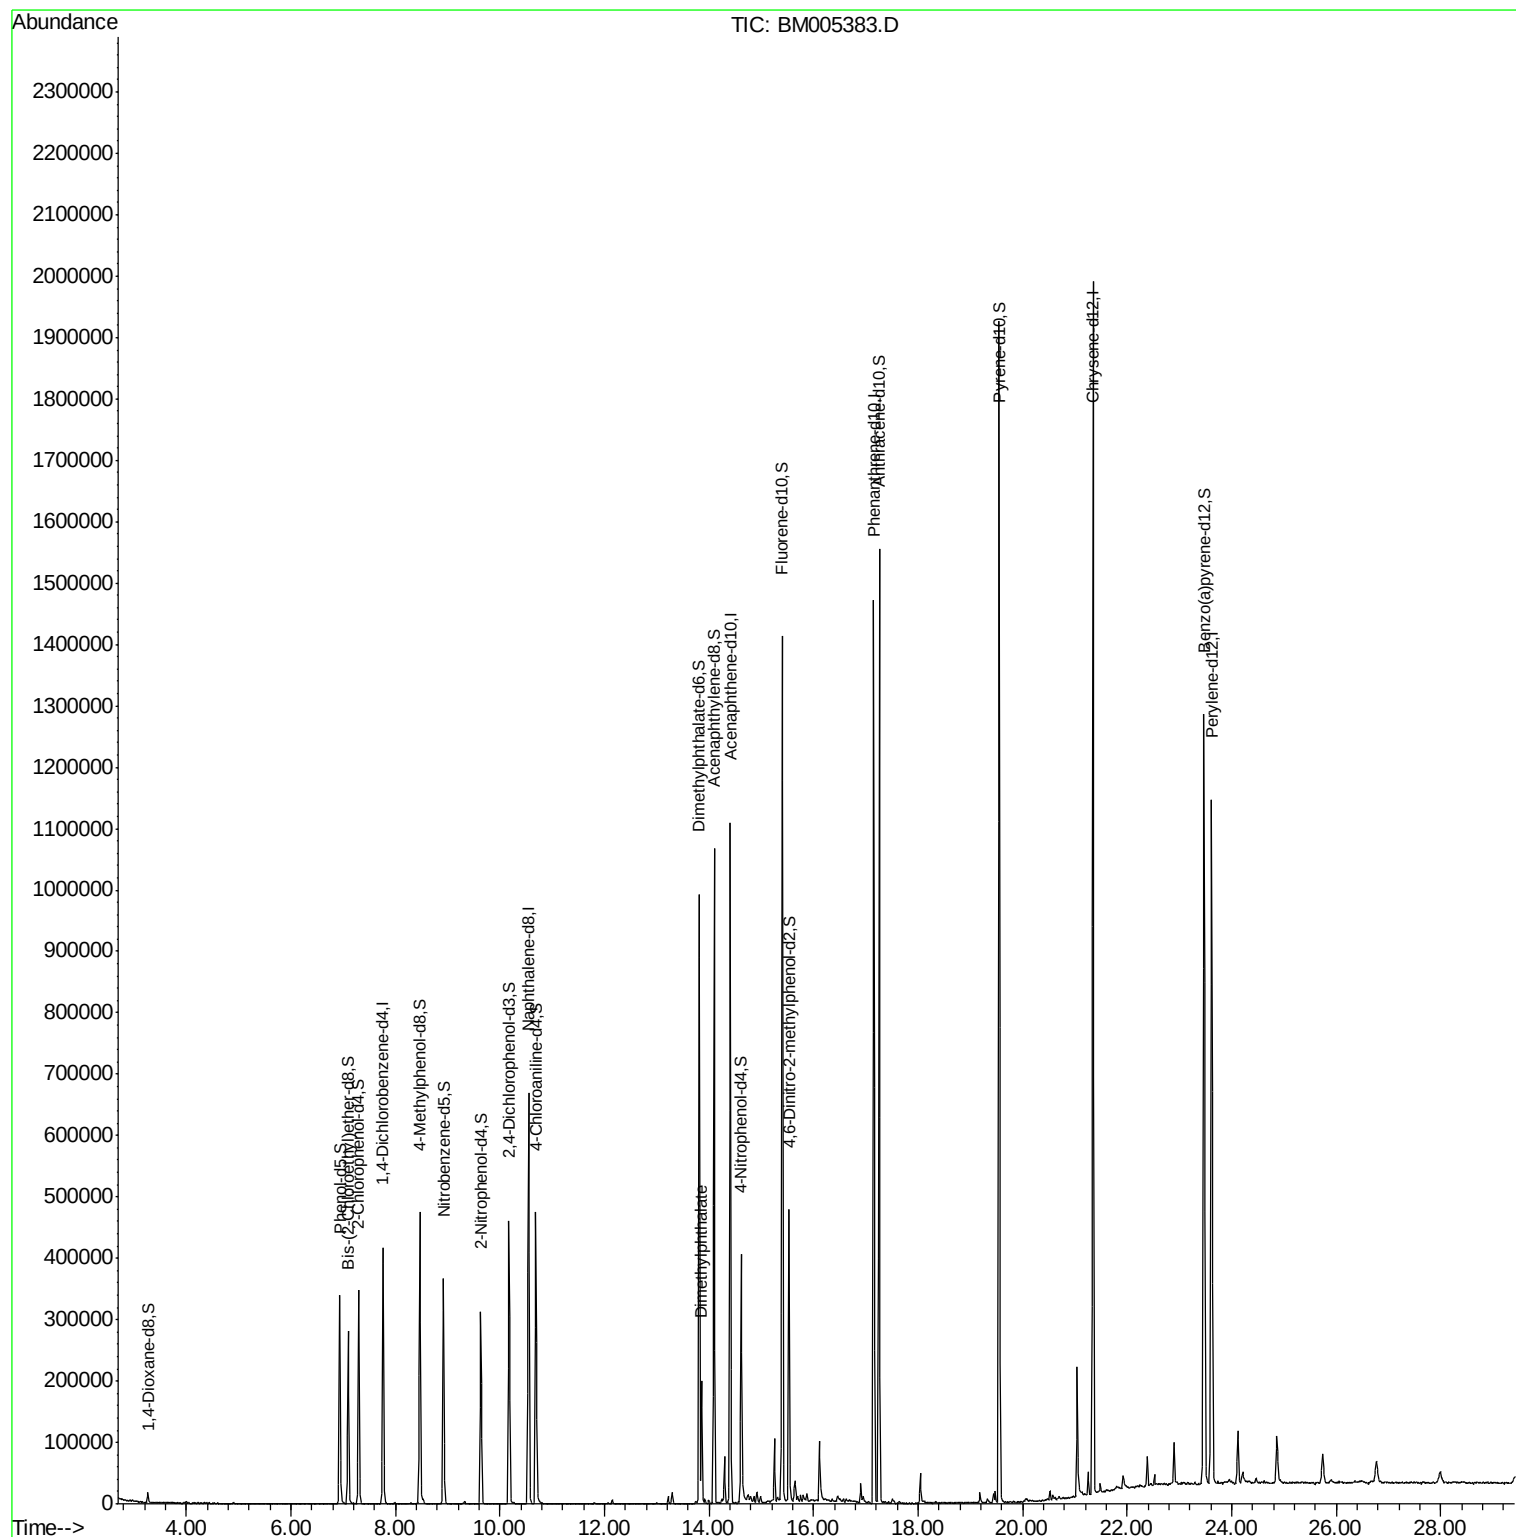

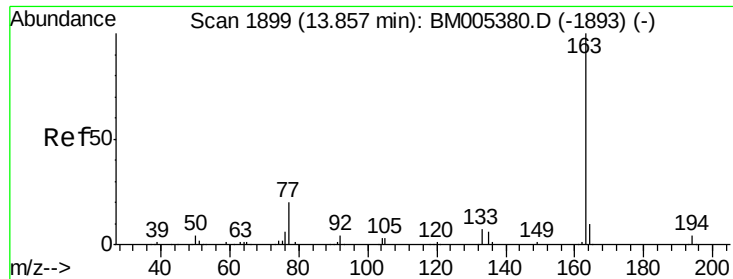

#44

Dimethylphthalate

Concen: 3.97 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. 0.00 min

Lab File: BM005383.D


Acq: 11 May 2016 11:35

Instrument :

BNA_M

ClientSampleId :

D9WY0

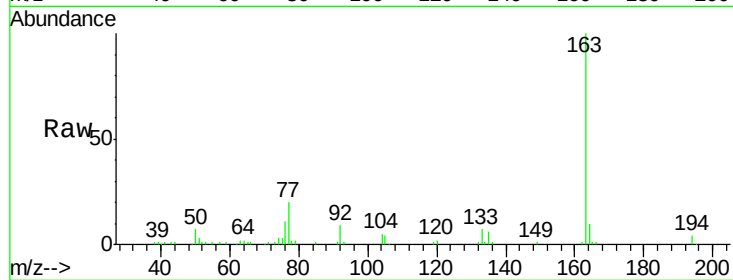

Tgt Ion:	163	Resp:	117154
Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.0
164	10.0	7.9	11.9

