

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005401.D
 Acq On : 11 May 2016 23:44
 Operator : UM/SJ
 Sample : H2890-22
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9X07

Quant Time: May 12 03:34:30 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 02:20:05 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	61022	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	288693	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	198534	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	478748	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	429450	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	338234	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.95	99	2073	0.37	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.10	67	3231	1.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	4482	1.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	3407	0.74	ng/ul	0.01
19) Nitrobenzene-d5	8.93	128	1234	0.60	ng/ul	0.01
22) 2-Nitrophenol-d4	9.65	143	1285	0.55	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.19	165	3735	0.86	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.81	166	16536	1.04	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	15808	0.85	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.40	176	14451	1.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	409	0.15	ng/ul	0.01
70) Anthracene-d10	17.25	188	21628	1.02	ng/ul	0.00
76) Pyrene-d10	19.54	212	22788	1.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	13774	0.92	ng/ul	-0.01


Target Compounds					Qvalue
44) Dimethylphthalate	13.86	163	20312	1.28 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005401.D
Acq On : 11 May 2016 23:44
Operator : UM/SJ
Sample : H2890-22
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X07

Quant Time: May 12 03:34:30 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 02:20:05 2016
Response via : Initial Calibration

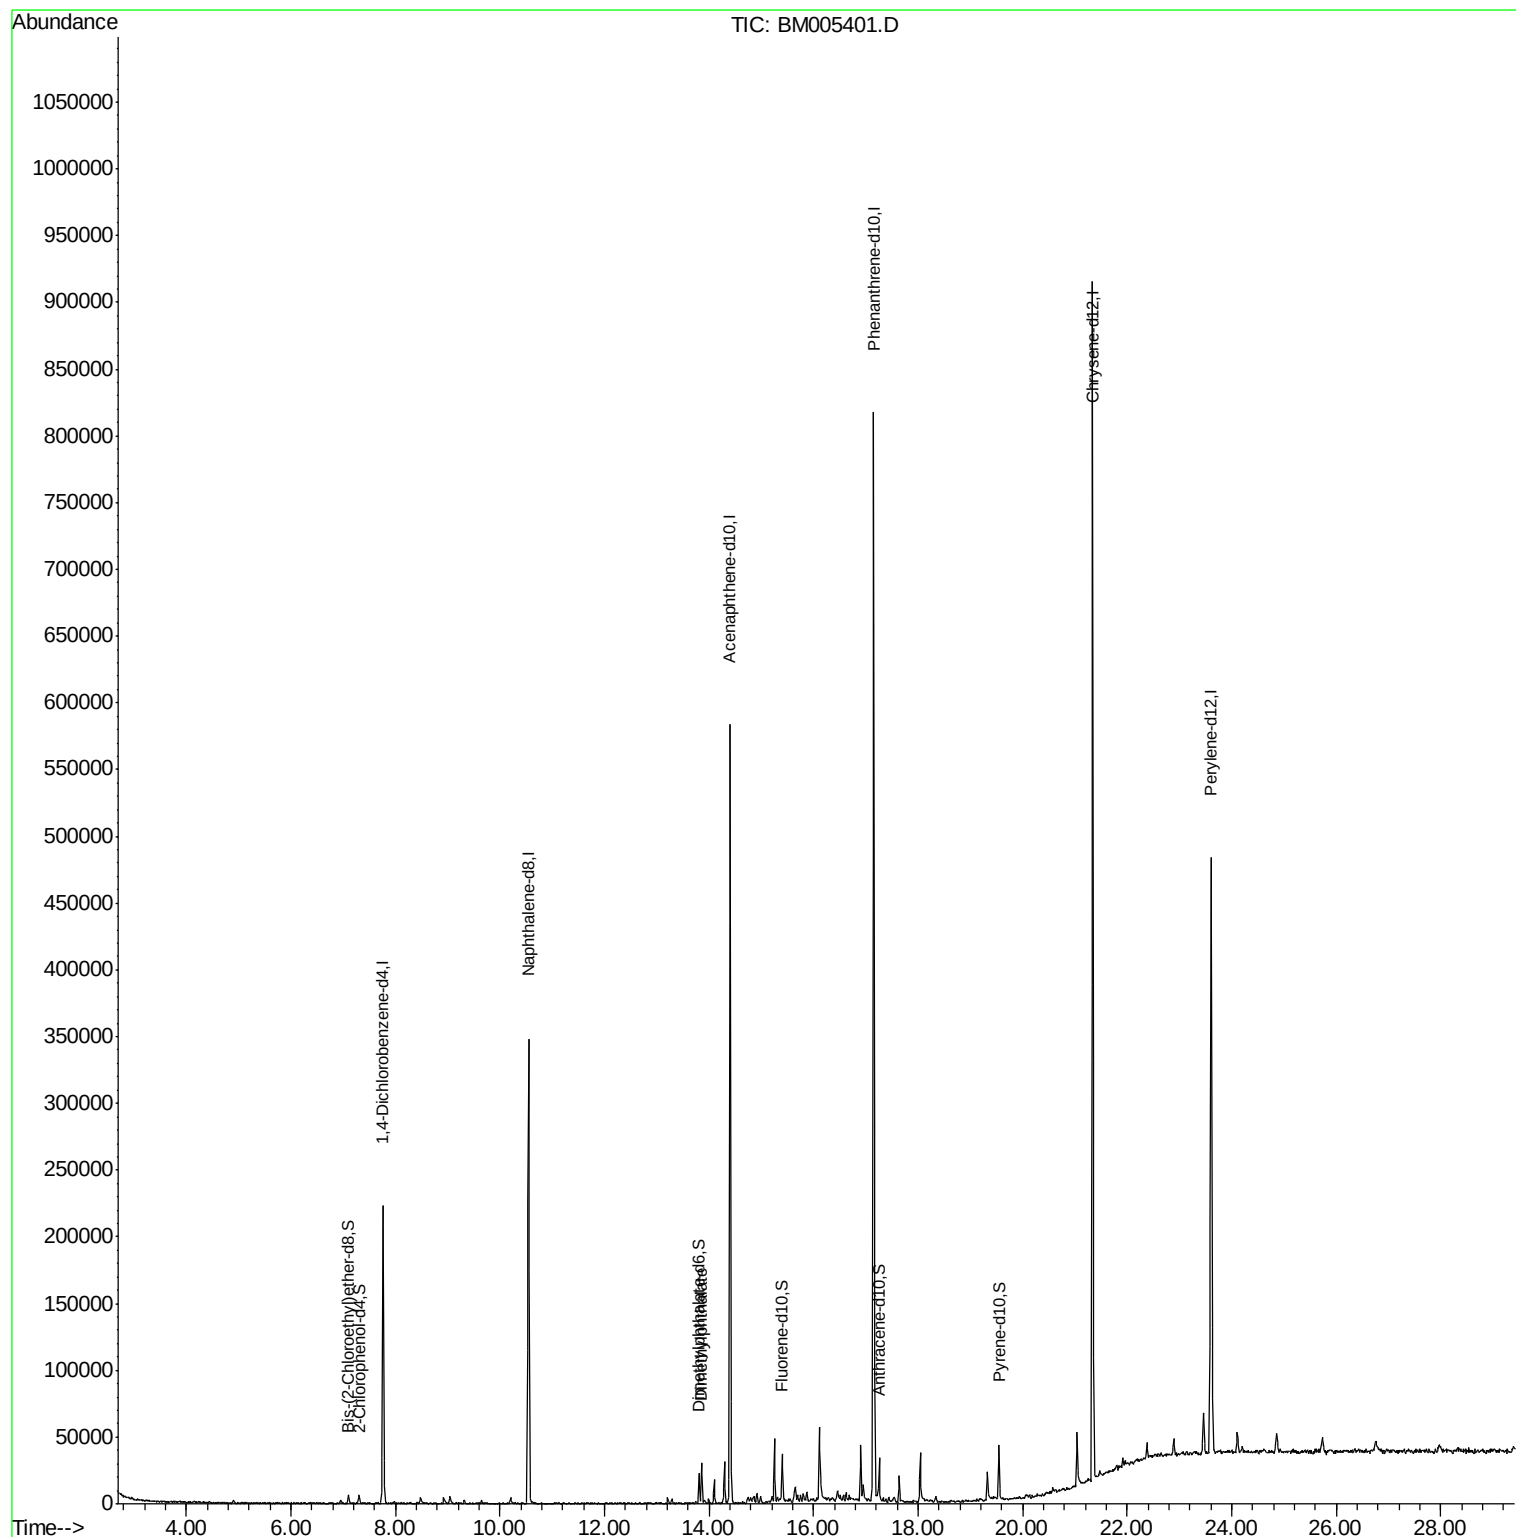

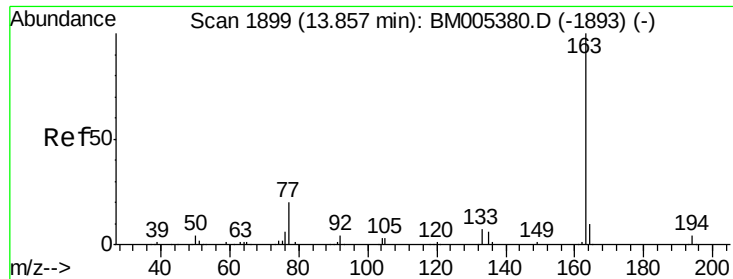

#44

Dimethylphthalate

Concen: 1.28 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. 0.00 min

Lab File: BM005401.D


Acq: 11 May 2016 23:44

Instrument :

BNA_M

ClientSampleId :

D9X07

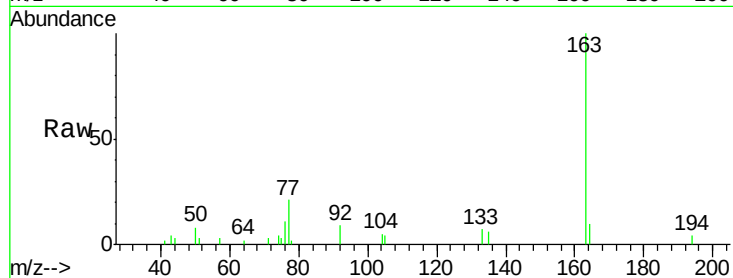


Tgt Ion:163 Resp: 20312

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.3 7.9 11.9

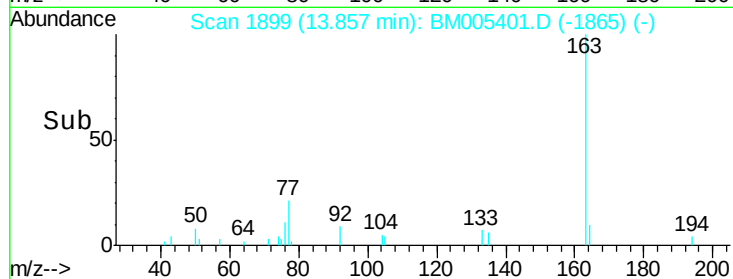

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

