

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005404.D
 Acq On : 12 May 2016 01:33
 Operator : UM/SJ
 Sample : H2846-01 25X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Quant Time: May 12 03:34:52 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 02:20:05 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	57795	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	268235	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	165365	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.14	188	366049	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	295769	20.00	ng/ul	0.00
83) Perylene-d12	23.60	264	251874	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.94	99	2570	0.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.09	67	5000	1.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	992	0.25	ng/ul	0.01
13) 4-Methylphenol-d8	8.47	113	1112	0.26	ng/ul	0.00
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	10.19	165	1077	0.27	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.81	166	4166	0.31	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	5092	0.33	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.40	176	4874	0.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.24	188	7557	0.47	ng/ul	0.00
76) Pyrene-d10	19.55	212	6427	0.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.46	264	4566	0.41	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
60) 4-Nitroaniline	15.49	138	233796	79.22	ng/ul#	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005404.D
Acq On : 12 May 2016 01:33
Operator : UM/SJ
Sample : H2846-01 25X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Quant Time: May 12 03:34:52 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 02:20:05 2016
Response via : Initial Calibration

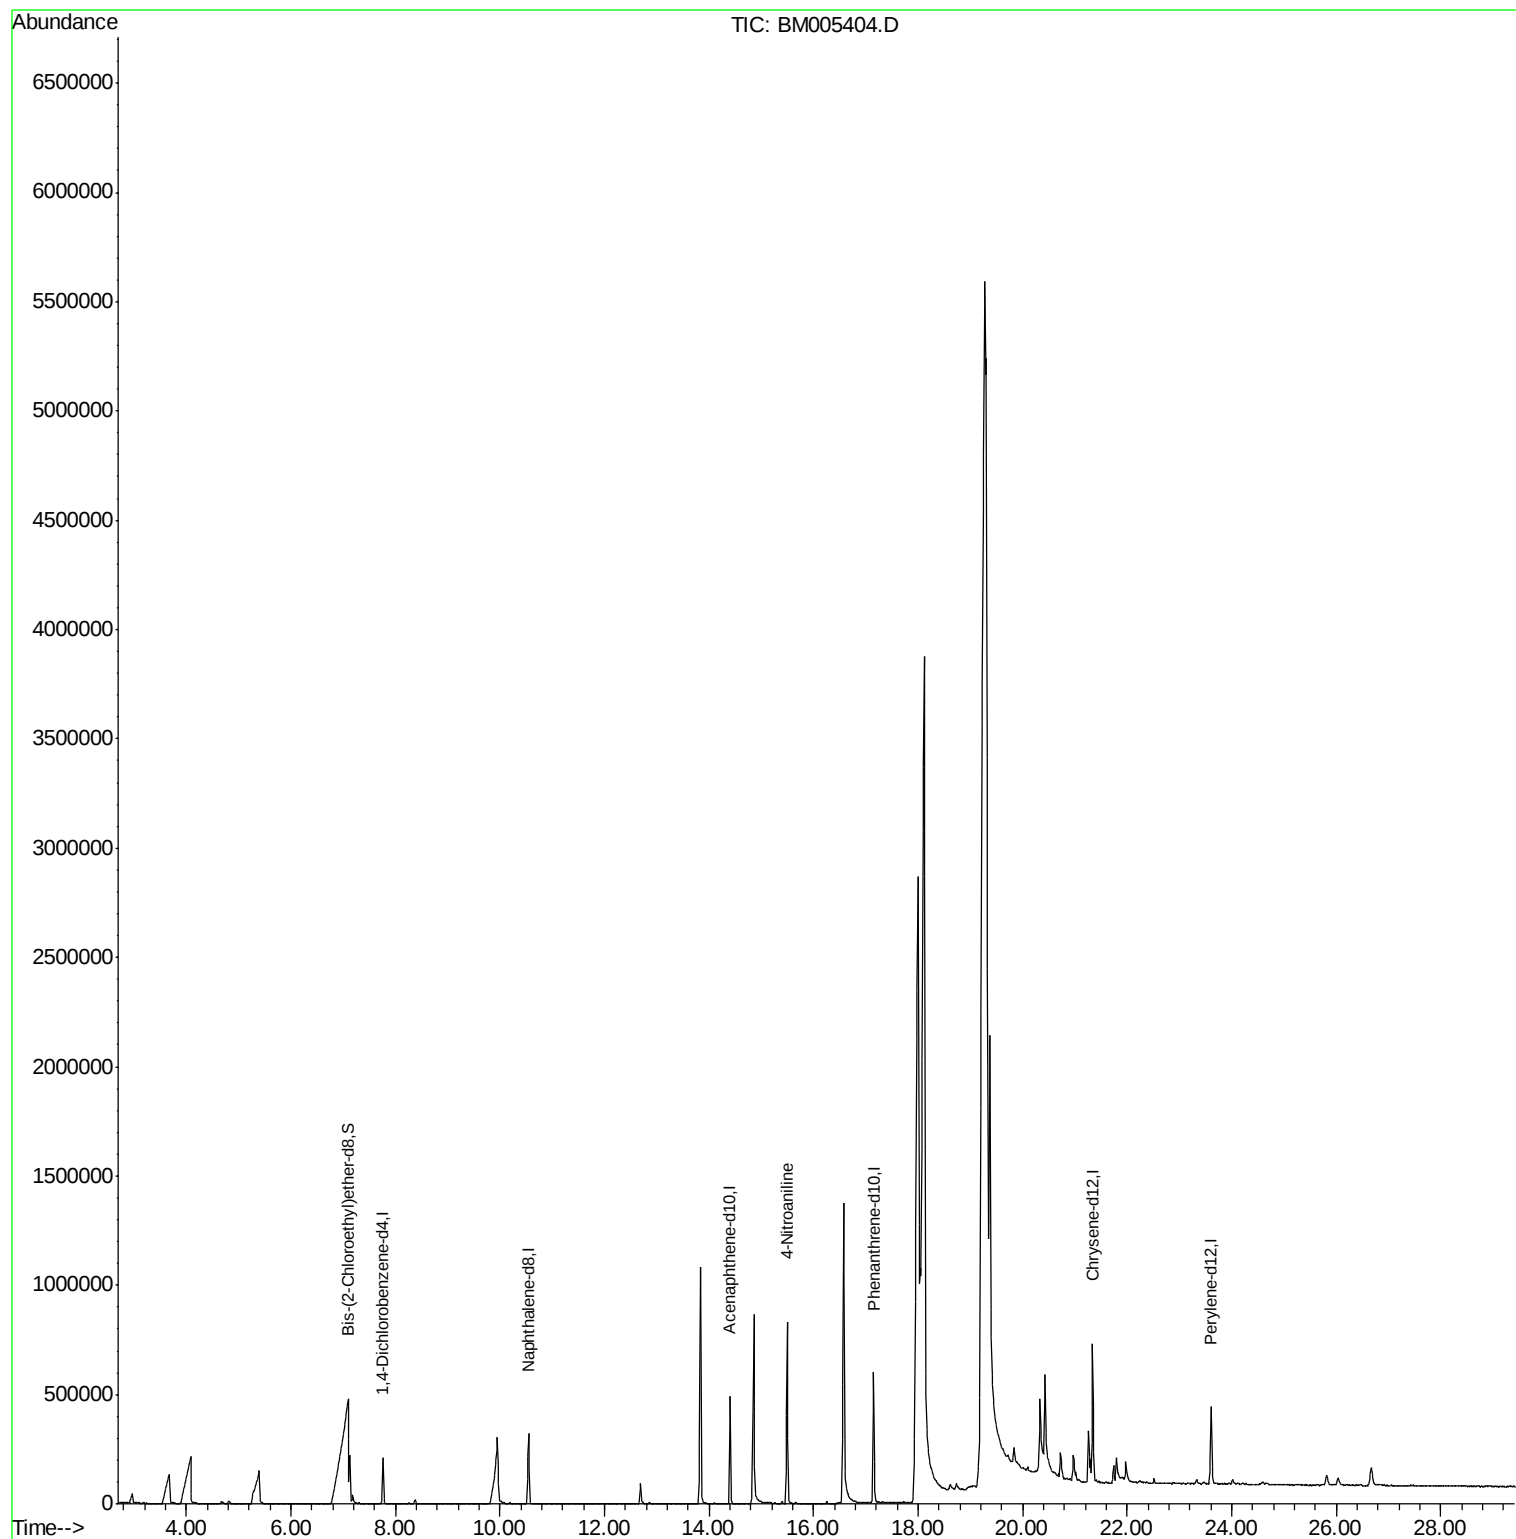

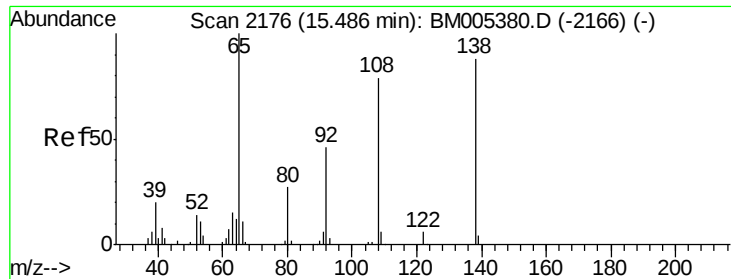

#60
 4-Nitroaniline
 Concen: 79.22 ng/ul
 RT: 15.49 min Scan# 2177
 Delta R.T. 0.01 min
 Lab File: BM005404.D
 Acq: 12 May 2016 01:33

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Tgt Ion	Ratio	Lower	Upper
138	100		
92	6.2	44.3	66.5#
108	0.0	66.3	99.5#

