

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005397.D
 Acq On : 11 May 2016 21:18
 Operator : UM/SJ
 Sample : H2847-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3J6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.934	717	722	736	rVB	52444	85578	3.71%	0.463%
2	7.092	744	749	760	rBV	182398	286371	12.40%	1.548%
3	7.292	777	783	796	rBB	196260	311377	13.49%	1.683%
4	7.757	856	862	871	rBV	187753	306692	13.28%	1.658%
5	8.463	977	982	999	rVB	167886	279934	12.12%	1.513%
6	8.916	1053	1059	1072	rBV	237690	393181	17.03%	2.125%
7	9.633	1175	1181	1193	rVB	204957	336871	14.59%	1.821%
8	10.169	1266	1272	1290	rBV	291064	518430	22.46%	2.802%
9	10.545	1329	1336	1350	rBV	314754	526384	22.80%	2.845%
10	13.810	1885	1891	1907	rBV	722603	1017144	44.06%	5.498%
11	14.092	1932	1939	1952	rBV	778728	1148271	49.74%	6.207%
12	14.404	1985	1992	2001	rVB2	520366	814609	35.28%	4.403%
13	14.621	2025	2029	2049	rBV	35751	78742	3.41%	0.426%
14	15.398	2154	2161	2169	rBV	1079184	1572130	68.09%	8.498%
15	15.521	2177	2182	2196	rVB	334843	484794	21.00%	2.621%
16	17.151	2453	2459	2466	rBV	755281	1094031	47.39%	5.914%
17	17.251	2469	2476	2491	rVV2	1235543	1844873	79.91%	9.973%
18	19.550	2860	2867	2877	rBV	1610163	2308739	100.00%	12.480%
19	21.344	3166	3172	3182	rBV	1110606	1488947	64.49%	8.049%
20	22.515	3367	3371	3375	rBV	46166	55445	2.40%	0.300%
21	23.468	3525	3533	3543	rBV2	1136330	2142973	92.82%	11.584%
22	23.609	3550	3557	3566	rVB	670544	1285606	55.68%	6.949%
23	24.109	3638	3642	3651	rVB	29788	55422	2.40%	0.300%
24	24.862	3765	3770	3779	rVB2	30257	62788	2.72%	0.339%


Sum of corrected areas: 18499332

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005397.D
Acq On : 11 May 2016 21:18
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

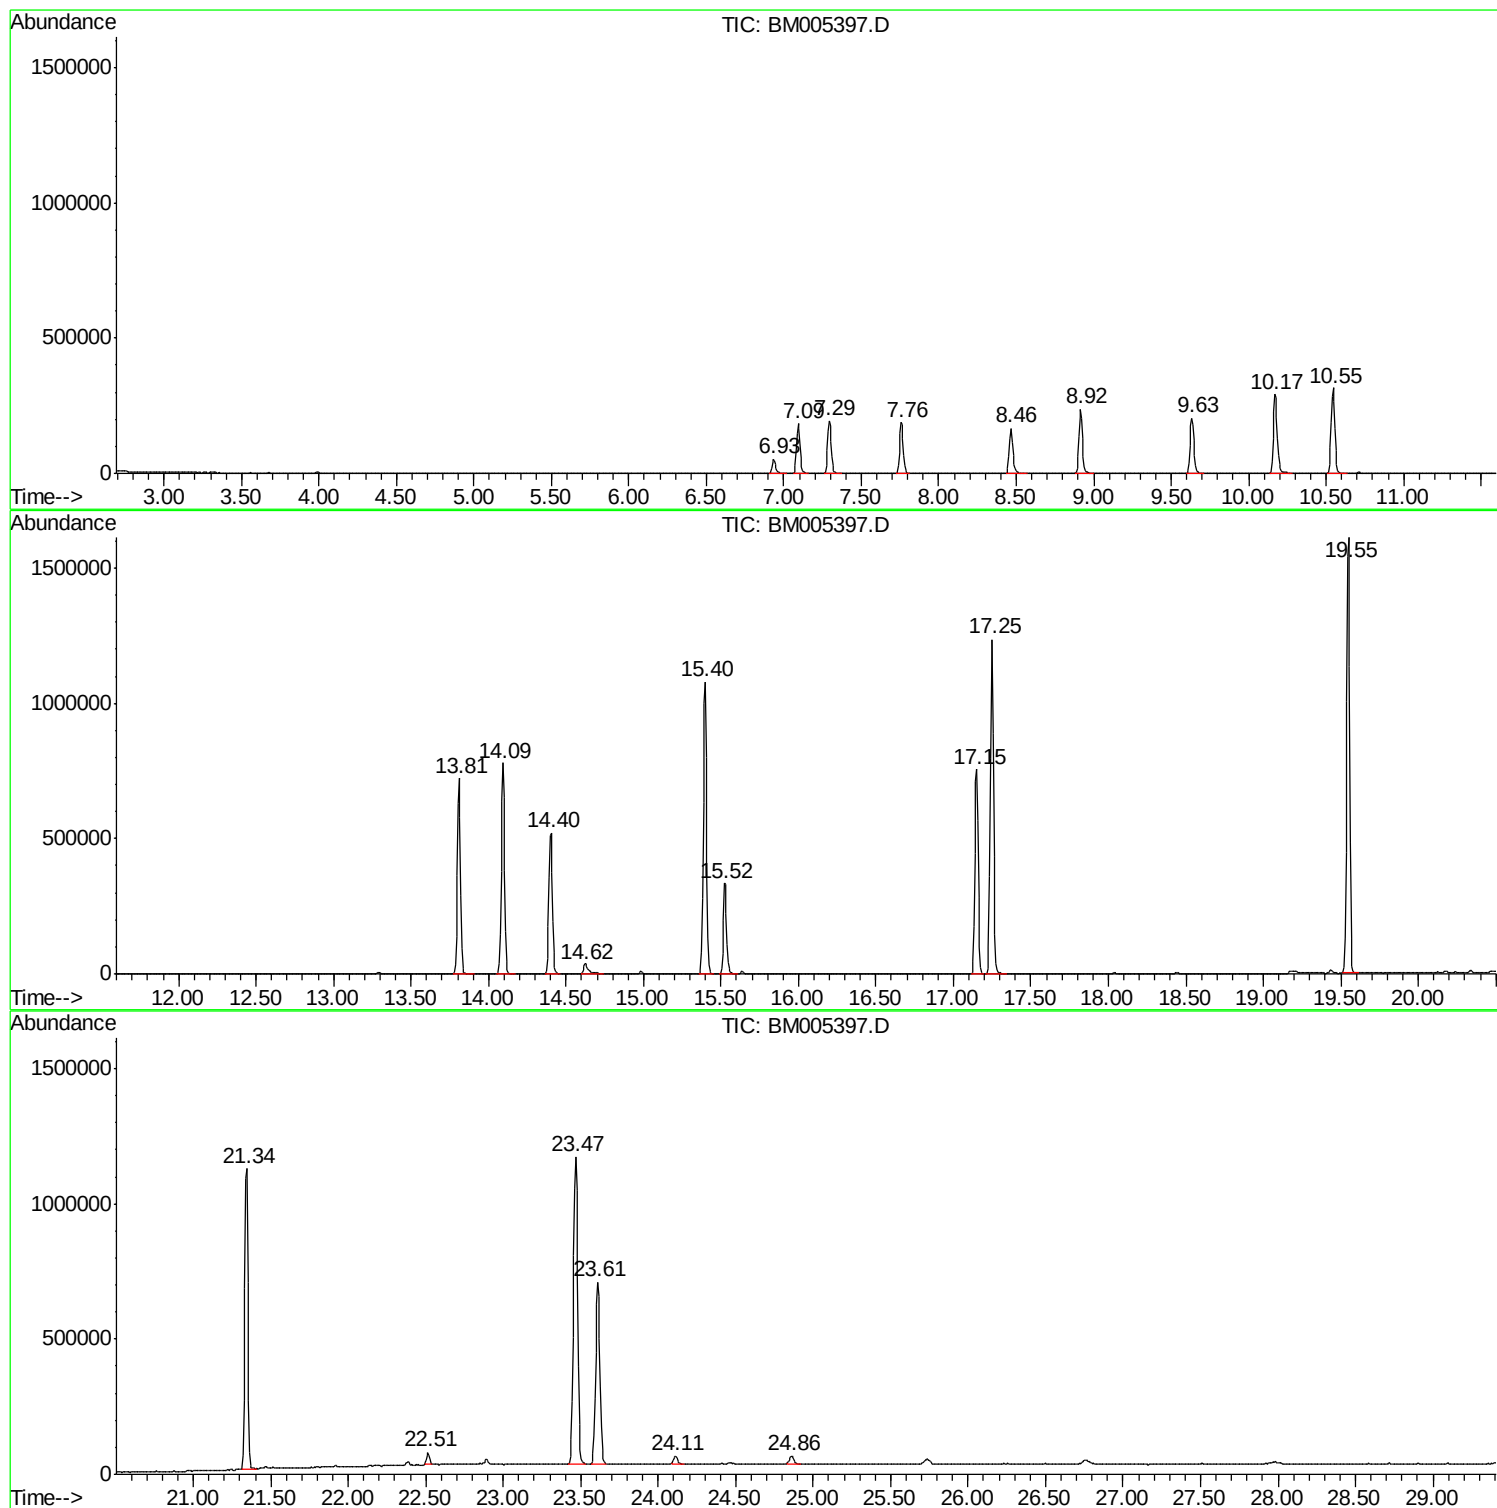

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005397.D
Acq On : 11 May 2016 21:18
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005397.D
Acq On : 11 May 2016 21:18
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc