

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
 Data File : BM005403.D
 Acq On : 12 May 2016 00:56
 Operator : UM/SJ
 Sample : PB90392BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.934	716	722	732	rBV	294577	470807	19.37%	2.209%
2	7.092	743	749	758	rBV	248959	378659	15.58%	1.777%
3	7.292	777	783	797	rVB	304075	488707	20.10%	2.293%
4	7.757	856	862	874	rVB	195901	318630	13.11%	1.495%
5	8.463	977	982	993	rBV	399808	643032	26.45%	3.018%
6	8.916	1052	1059	1069	rBV	315685	508708	20.93%	2.387%
7	9.633	1175	1181	1191	rBV	273811	444519	18.29%	2.086%
8	10.169	1266	1272	1290	rBV	388434	667424	27.45%	3.132%
9	10.545	1329	1336	1344	rBV	326026	538658	22.16%	2.528%
10	10.686	1353	1360	1377	rBV	418758	736685	30.30%	3.457%
11	13.810	1884	1891	1898	rBV	880053	1220527	50.21%	5.728%
12	14.092	1932	1939	1951	rBV	938959	1392078	57.26%	6.533%
13	14.398	1985	1991	1999	rBV2	547326	840029	34.56%	3.942%
14	14.615	2022	2028	2047	rBV	296404	517070	21.27%	2.427%
15	15.398	2154	2161	2175	rBV	1200830	1794547	73.82%	8.422%
16	15.527	2177	2183	2193	rBV	352242	513738	21.13%	2.411%
17	17.151	2452	2459	2469	rBV	751118	1090911	44.88%	5.120%
18	17.250	2469	2476	2495	rVB	1347187	2017513	82.99%	9.468%
19	19.544	2860	2866	2875	rBV2	1698781	2430991	100.00%	11.408%
20	21.338	3165	3171	3185	rBV	1041910	1336901	54.99%	6.274%
21	23.462	3524	3532	3543	rBV	997621	1876803	77.20%	8.808%
22	23.603	3549	3556	3568	rVB2	529395	1002763	41.25%	4.706%
23	24.103	3638	3641	3649	rVB2	19436	34426	1.42%	0.162%
24	24.850	3764	3768	3778	rVB3	20397	44743	1.84%	0.210%


Sum of corrected areas: 21308869

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005403.D
Acq On : 12 May 2016 00:56
Operator : UM/SJ
Sample : PB90392BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

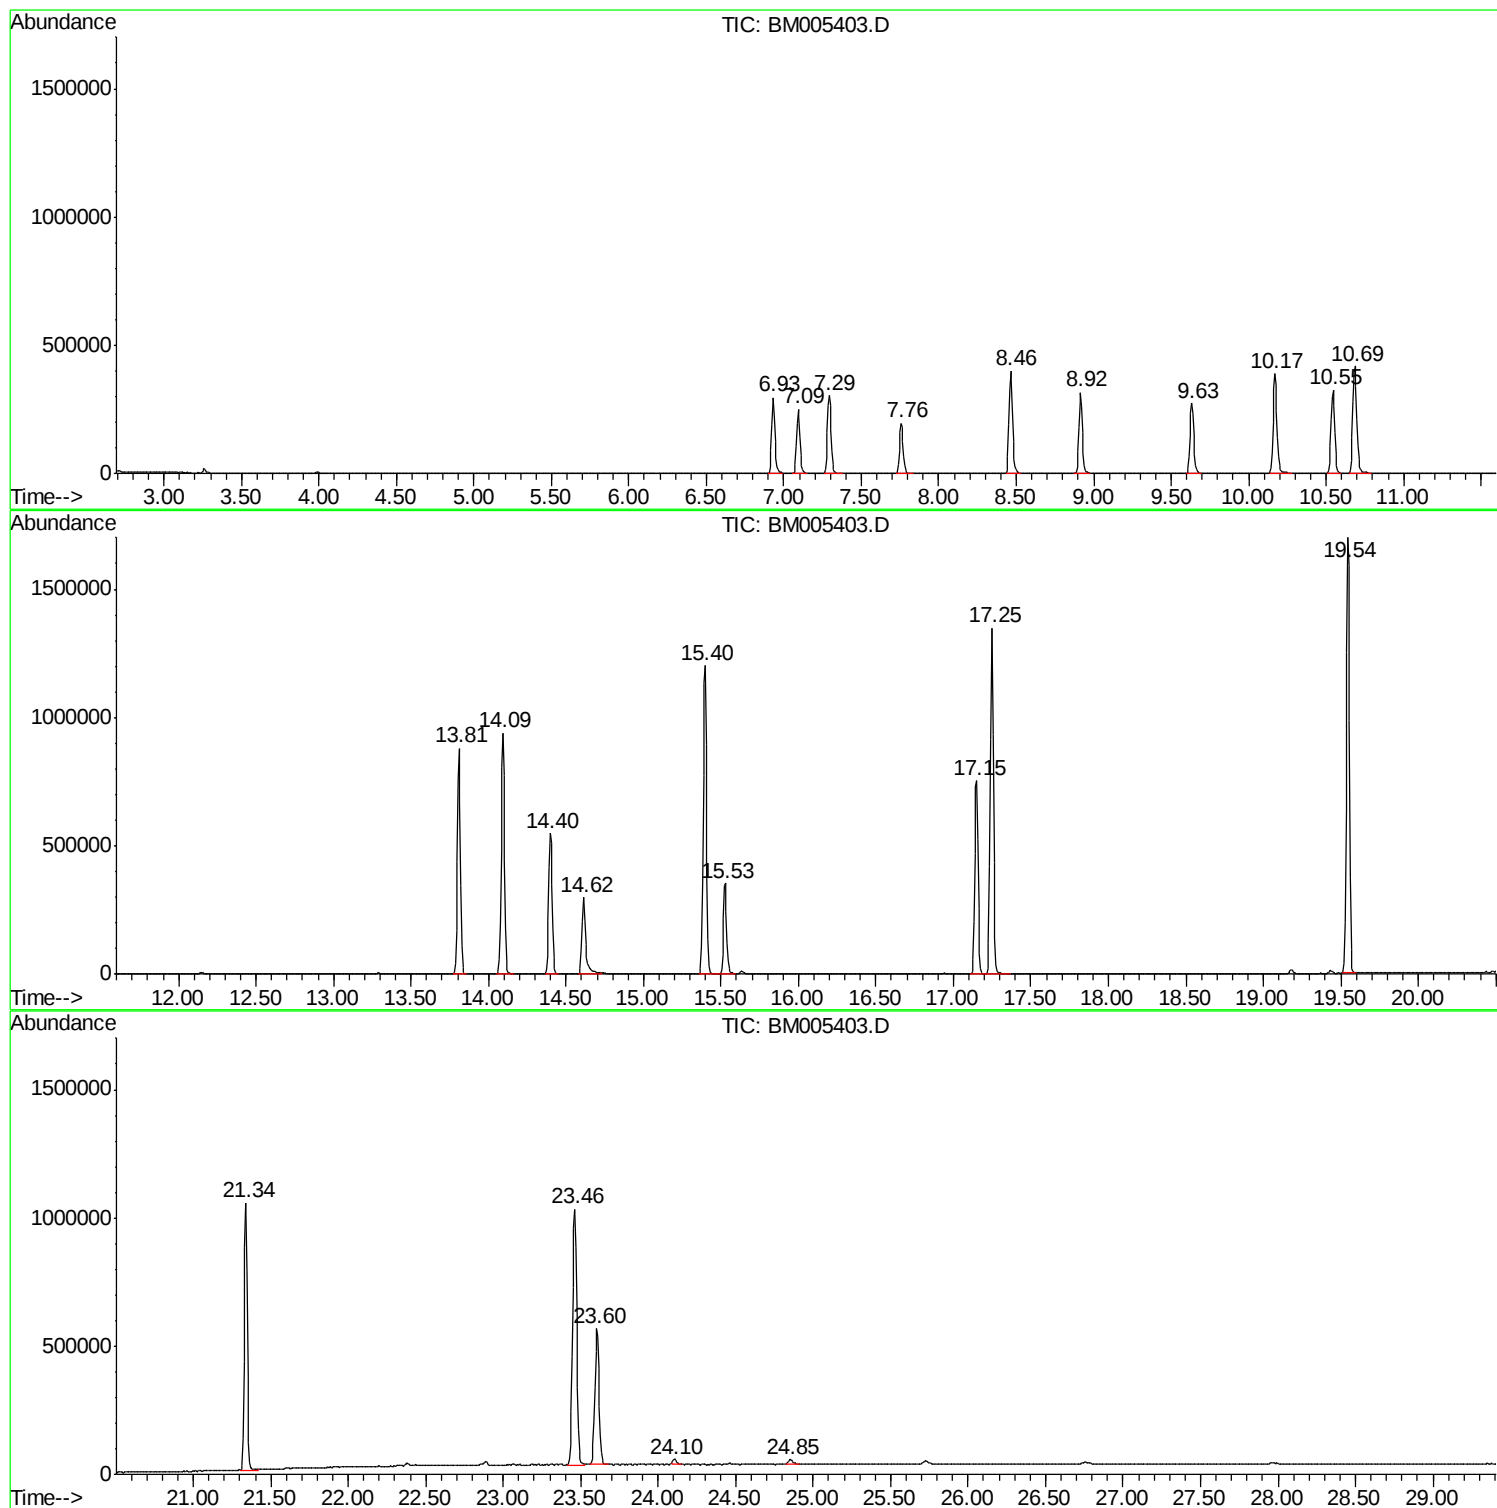

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005403.D
Acq On : 12 May 2016 00:56
Operator : UM/SJ
Sample : PB90392BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051116\
Data File : BM005403.D
Acq On : 12 May 2016 00:56
Operator : UM/SJ
Sample : PB90392BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc