


2,4-Dinitrophenol


Response Ratio

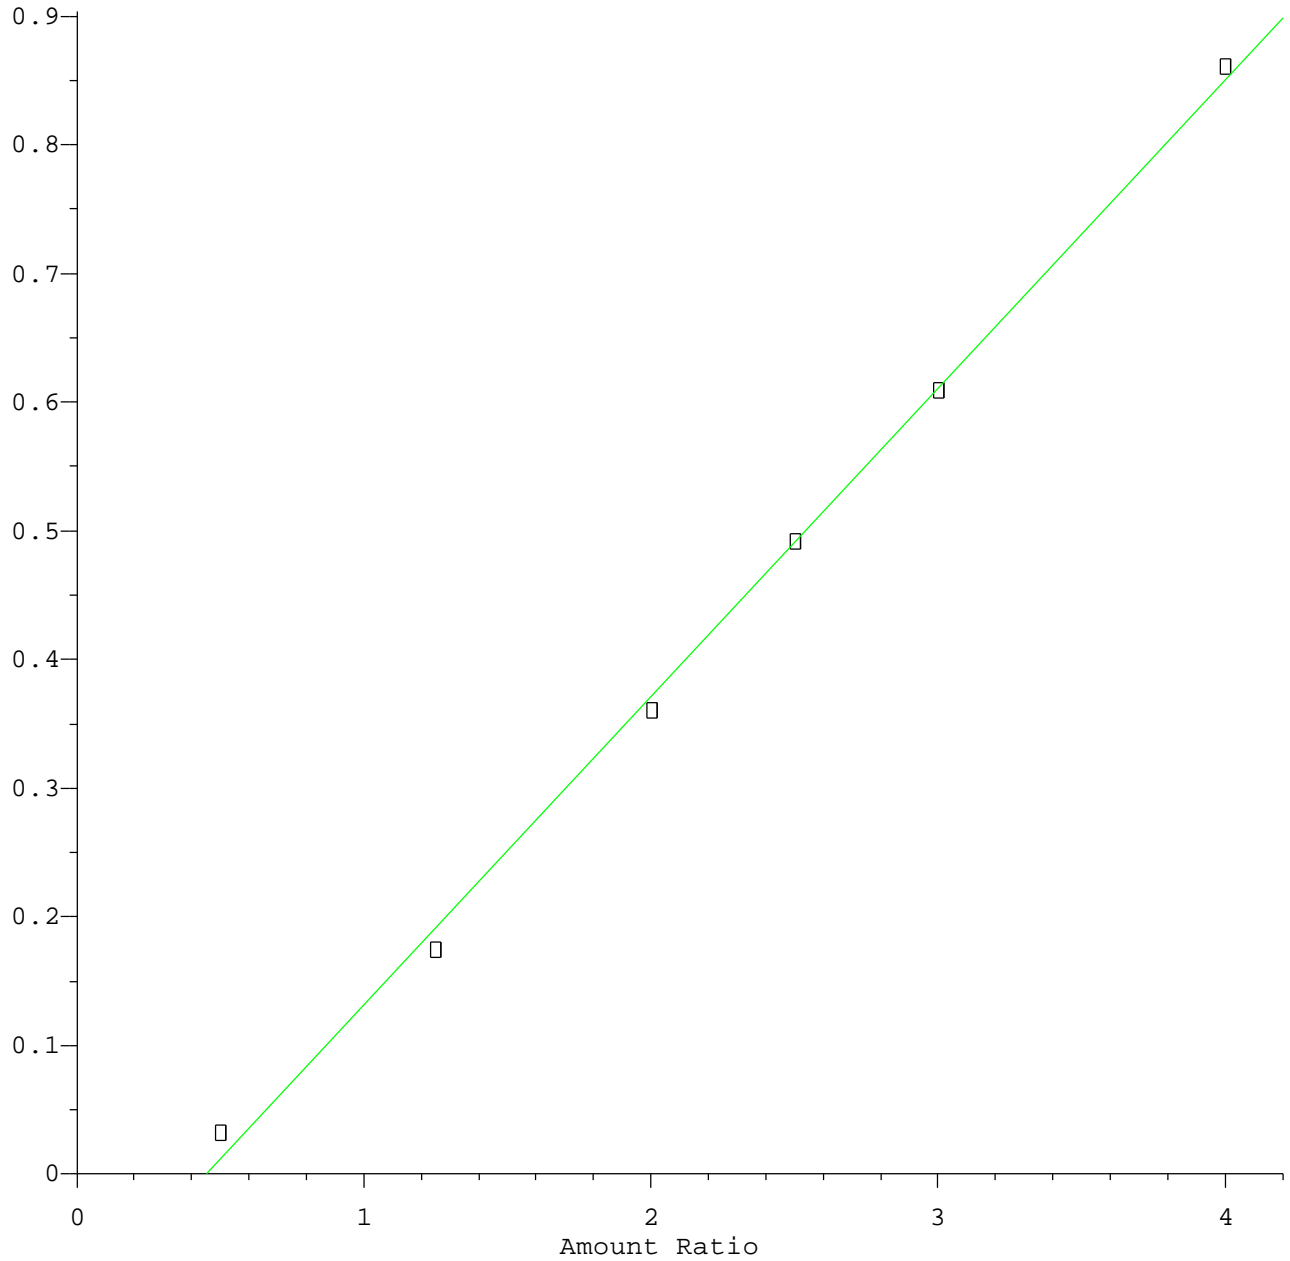

Resp Ratio = 2.40e-001 * Amt - 1.08e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
Calibration Table Last Updated: Thu May 11 19:50:16 2017


4,6-Dinitro-2-methylphenol

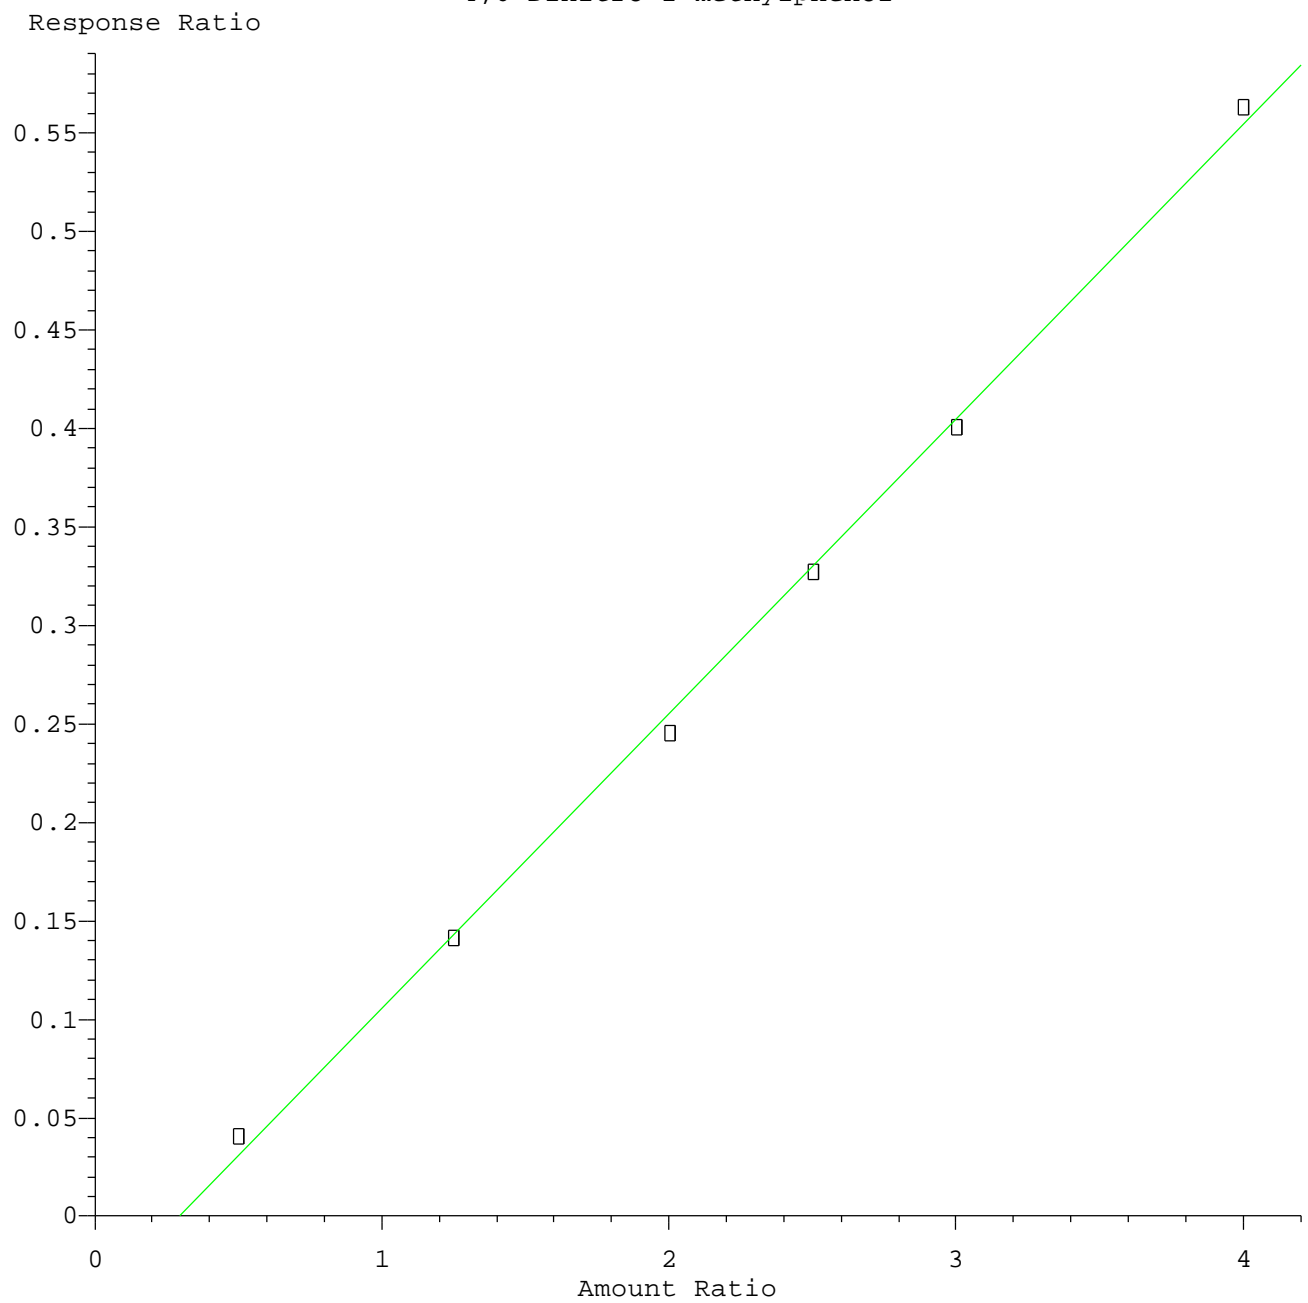

Resp Ratio = 1.49e-001 * Amt - 4.37e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
Calibration Table Last Updated: Thu May 11 19:50:16 2017

Pentachlorophenol

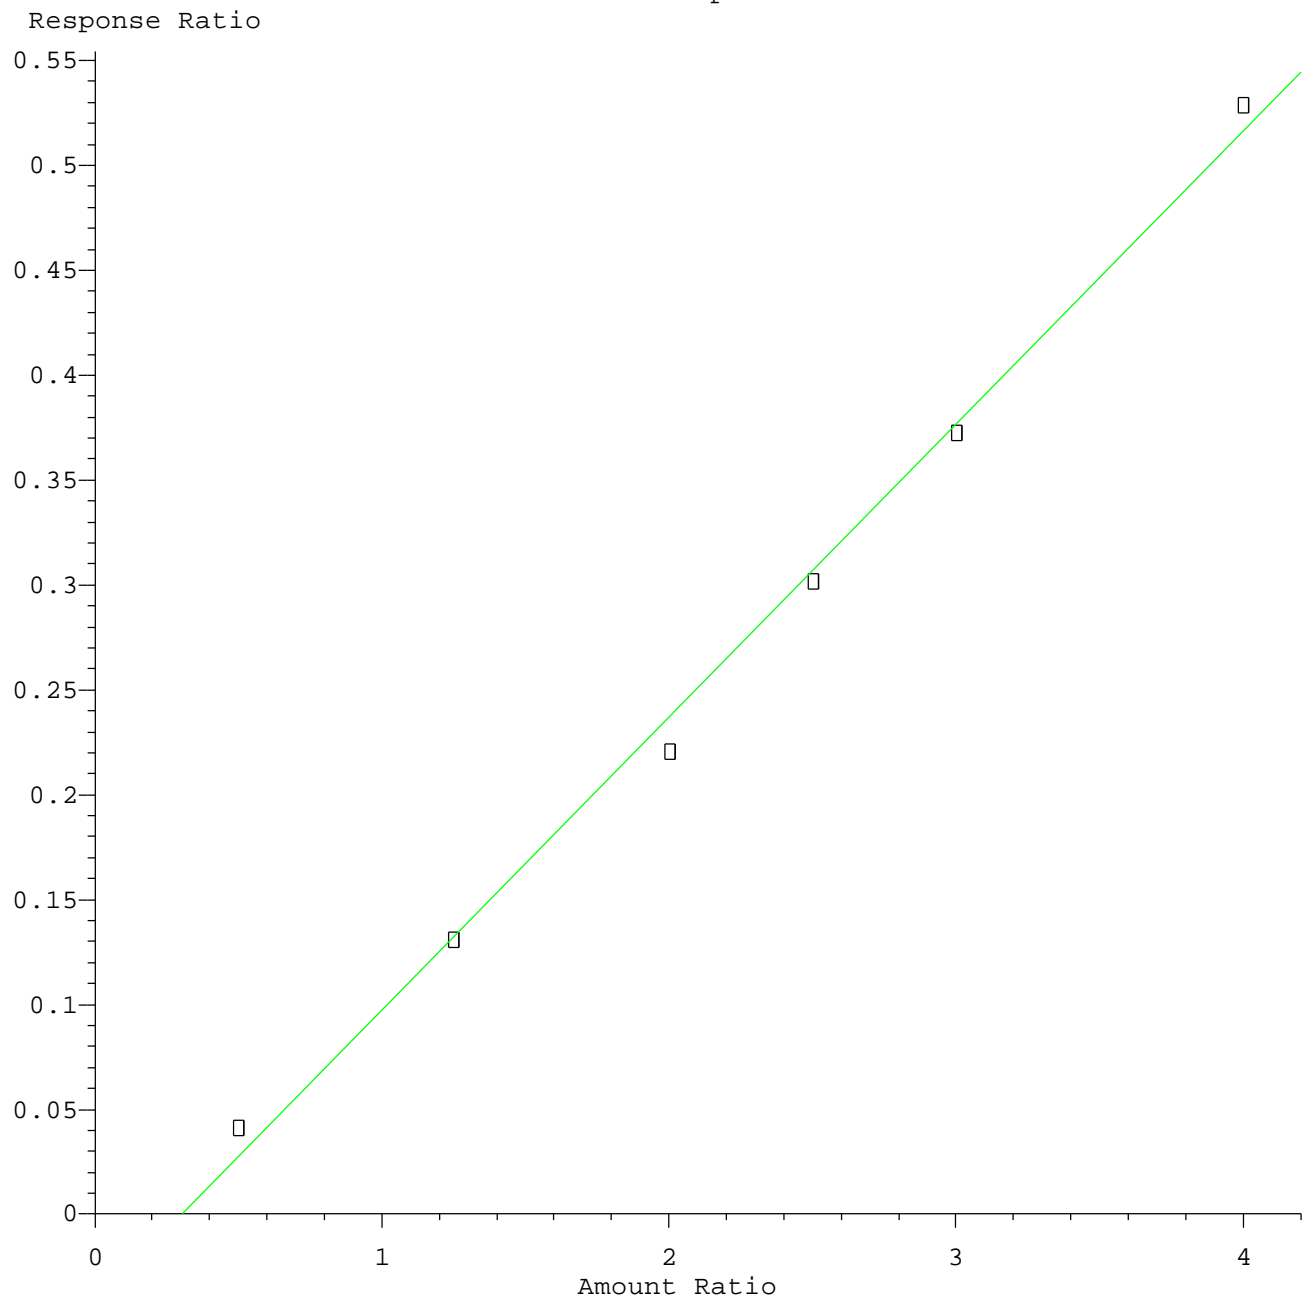


Resp Ratio = 1.40e-001 * Amt - 4.25e-002
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
Calibration Table Last Updated: Thu May 11 19:50:16 2017

Hexachlorocyclopentadiene

Response Ratio

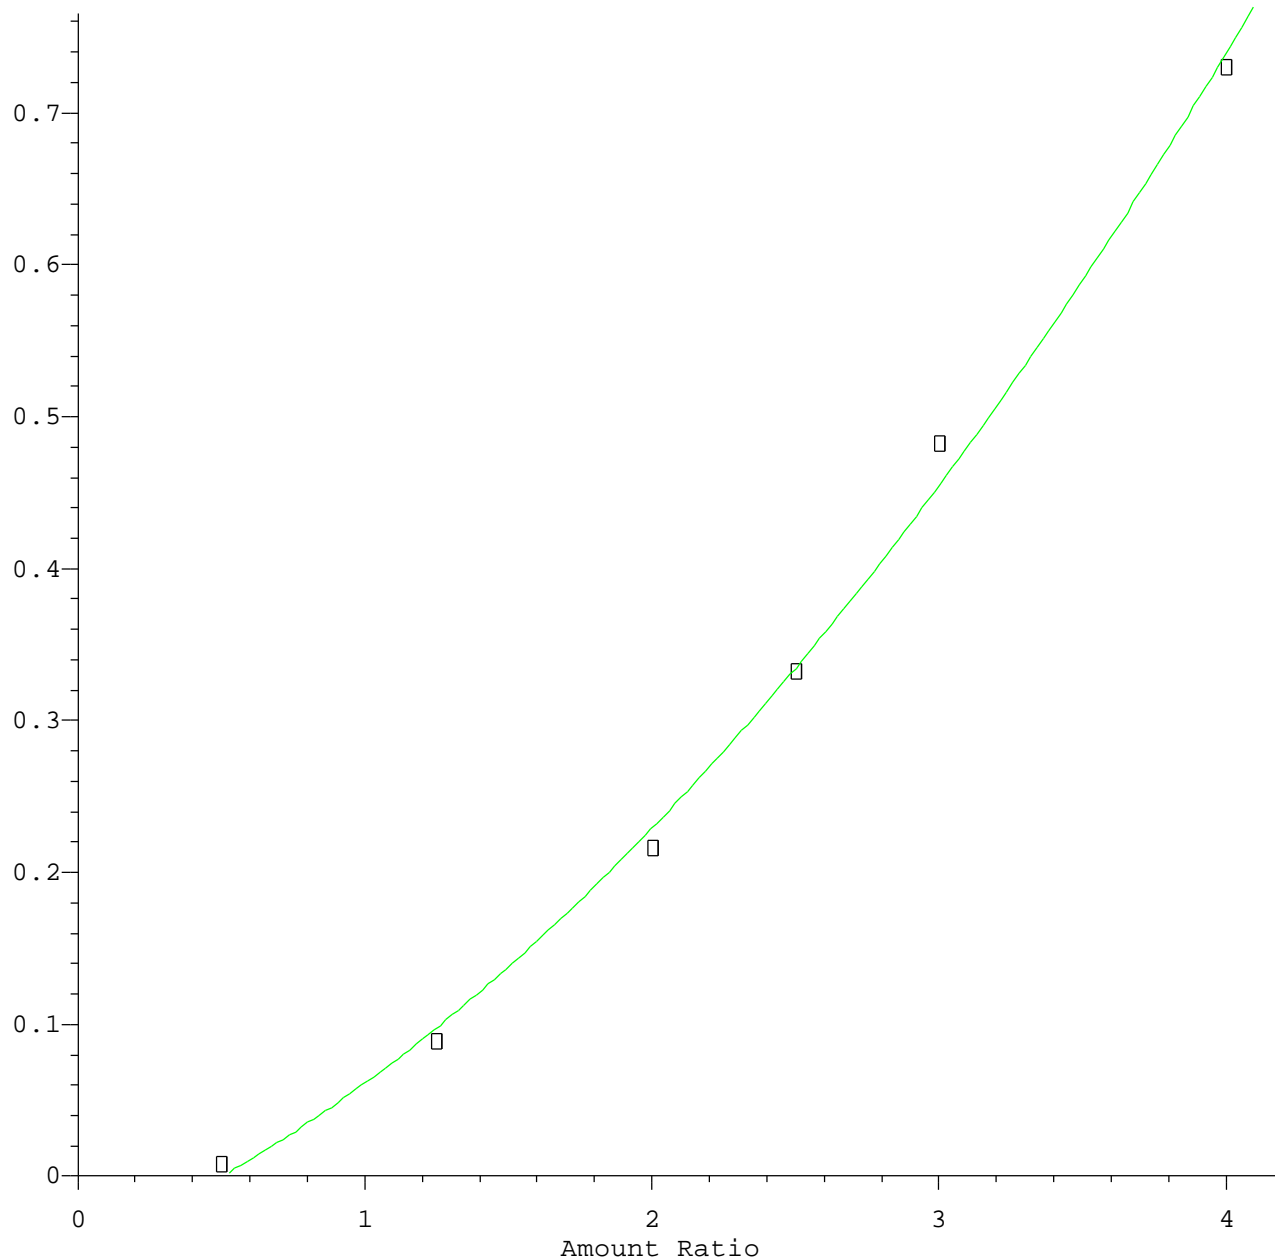

$R = 2.92e-002 A^2 + 8.00e-002 A - 4.79e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
Calibration Table Last Updated: Thu May 11 19:50:16 2017