
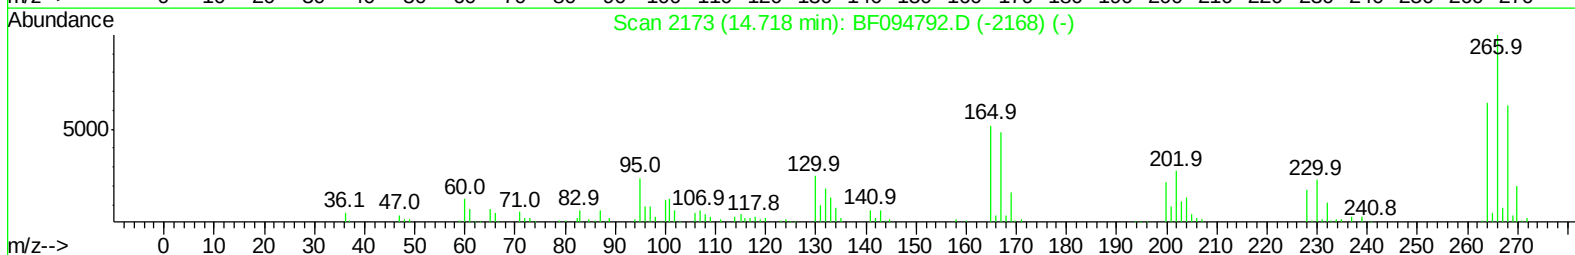
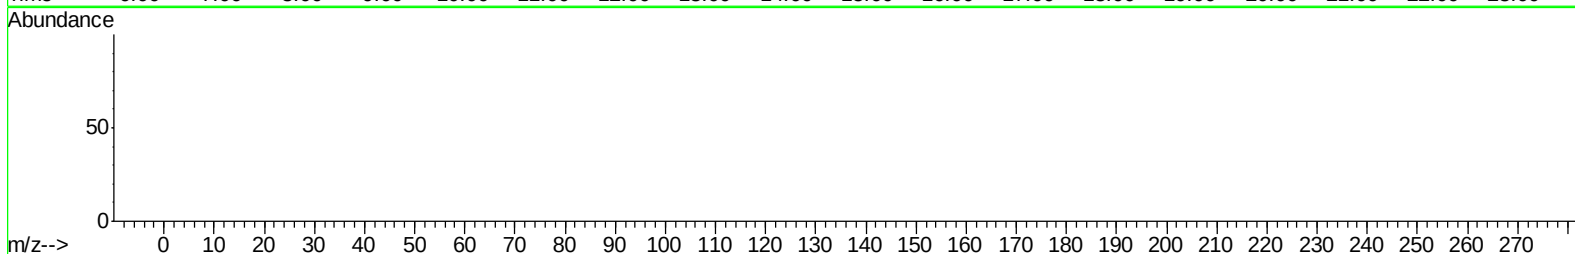


Data Path : Z:\HPCHEM1\BNA M\DATA\BM051117\
Data File : BM009983.D
Acq On : 11 May 2017 14:16
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 18:25:38 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

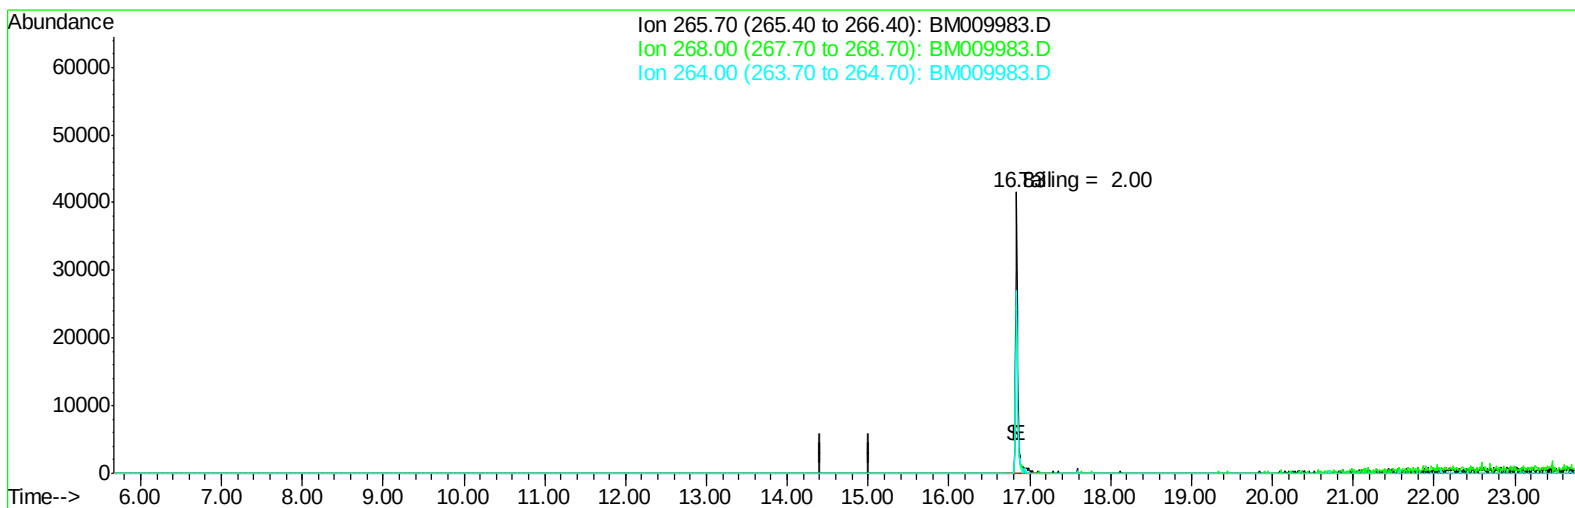

TIC: BM009983.D

(69) Pentachlorophenol (C)




14.718min (-14.718) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.90	0.00#
264.00	64.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051117\
 Data File : BM009983.D
 Acq On : 11 May 2017 14:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 18:25:38 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 03 17:24:51 2017
 Response via : Initial Calibration

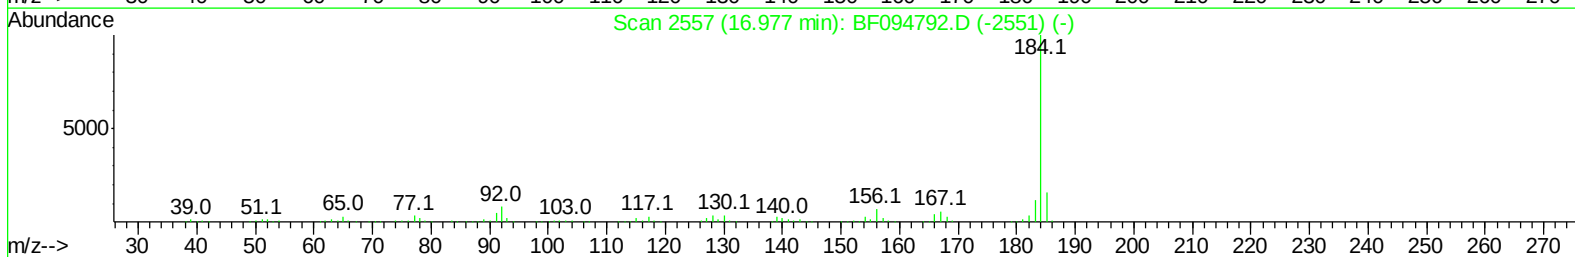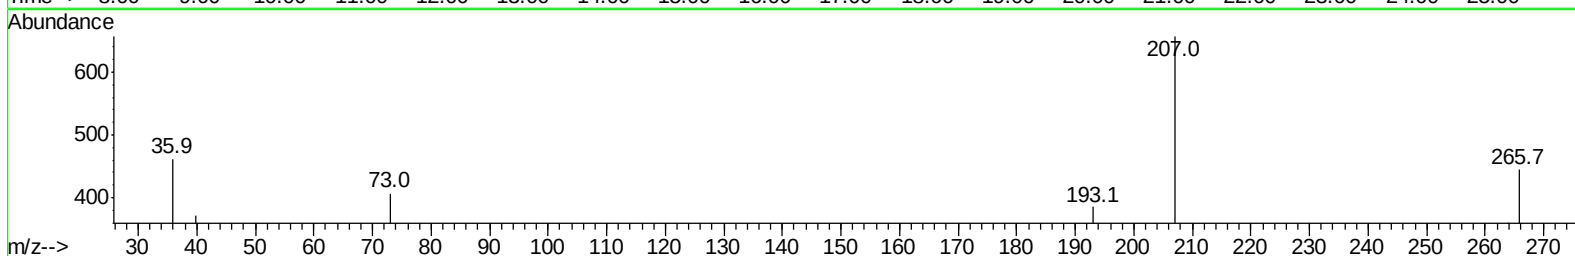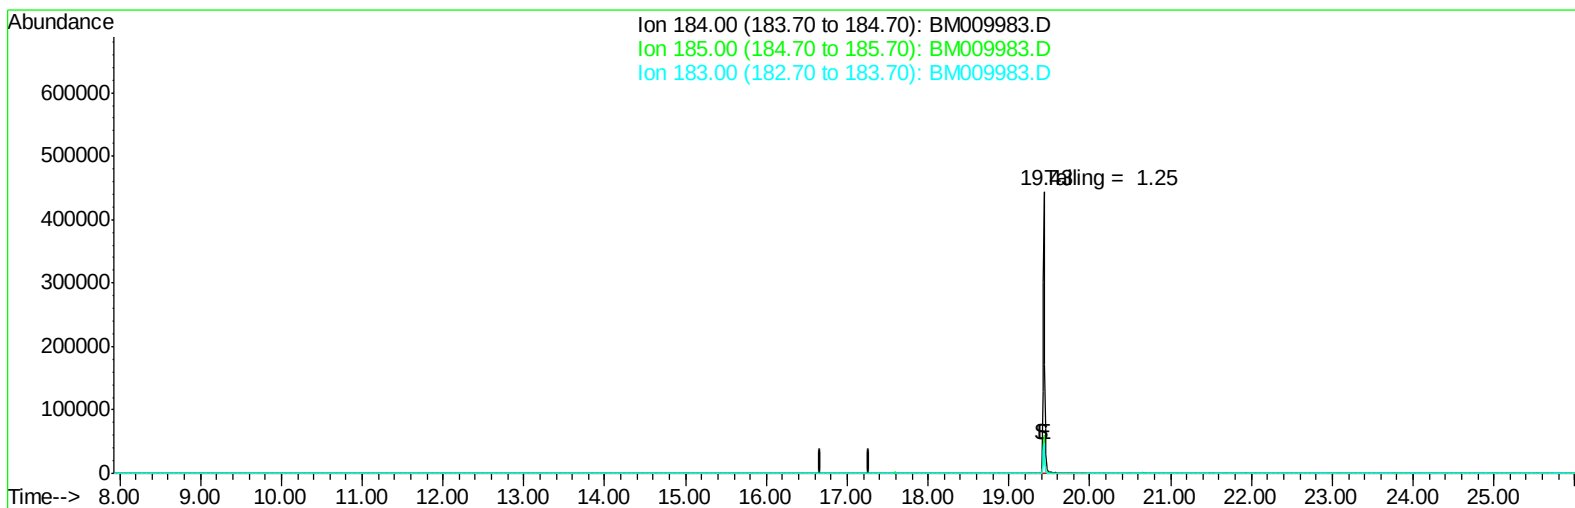

TIC: BM009983.D

(76) Benzidine

16.977min (-16.977) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	19.40	0.00#
183.00	12.20	0.00#
0.00	0.00	0.00