
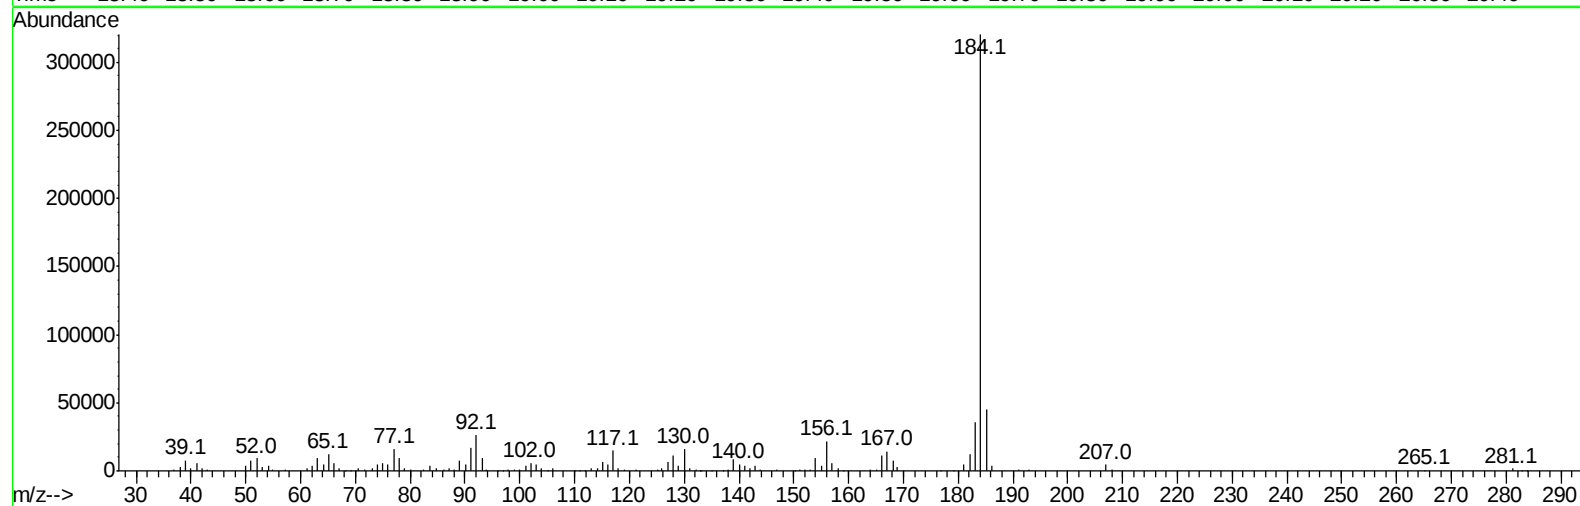


Data Path : Z:\HPCHEM1\BNA M\DATA\BM051117\
Data File : BM010001.D
Acq On : 12 May 2017 01:06
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:15:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

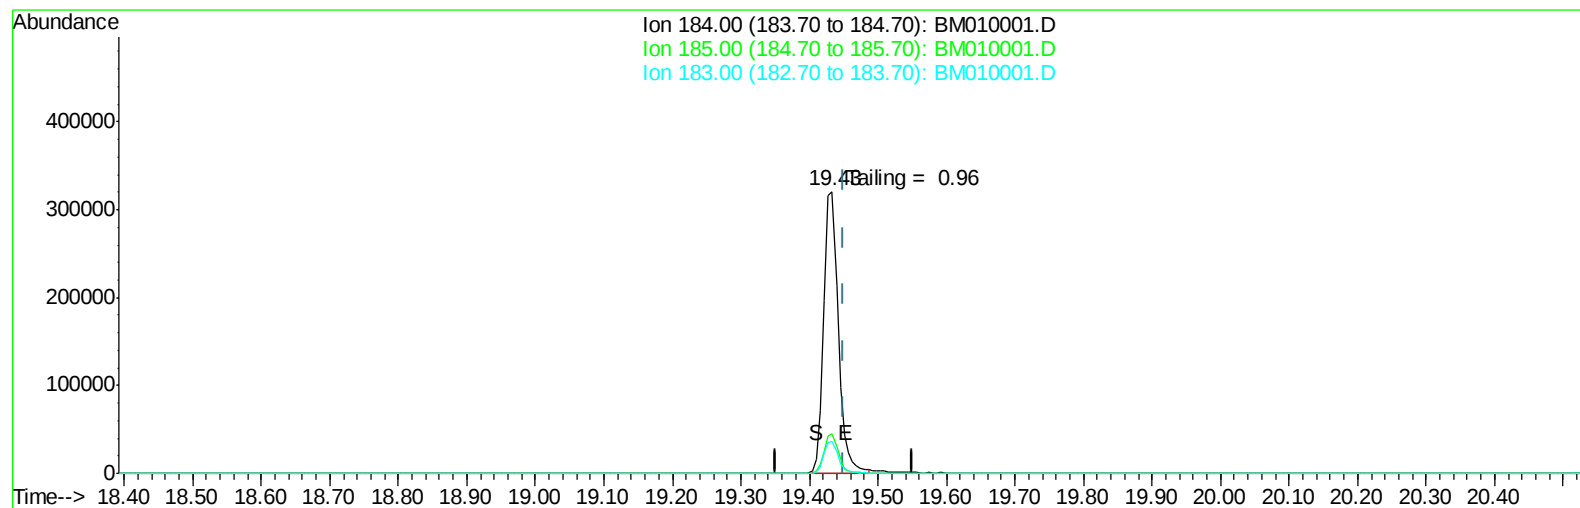

TIC: BM010001.D

(76) Benzidine



19.433min (-0.017) 0.00ng

response 477924

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.95
183.00	11.10	11.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051117\
Data File : BM010001.D
Acq On : 12 May 2017 01:06
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:15:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

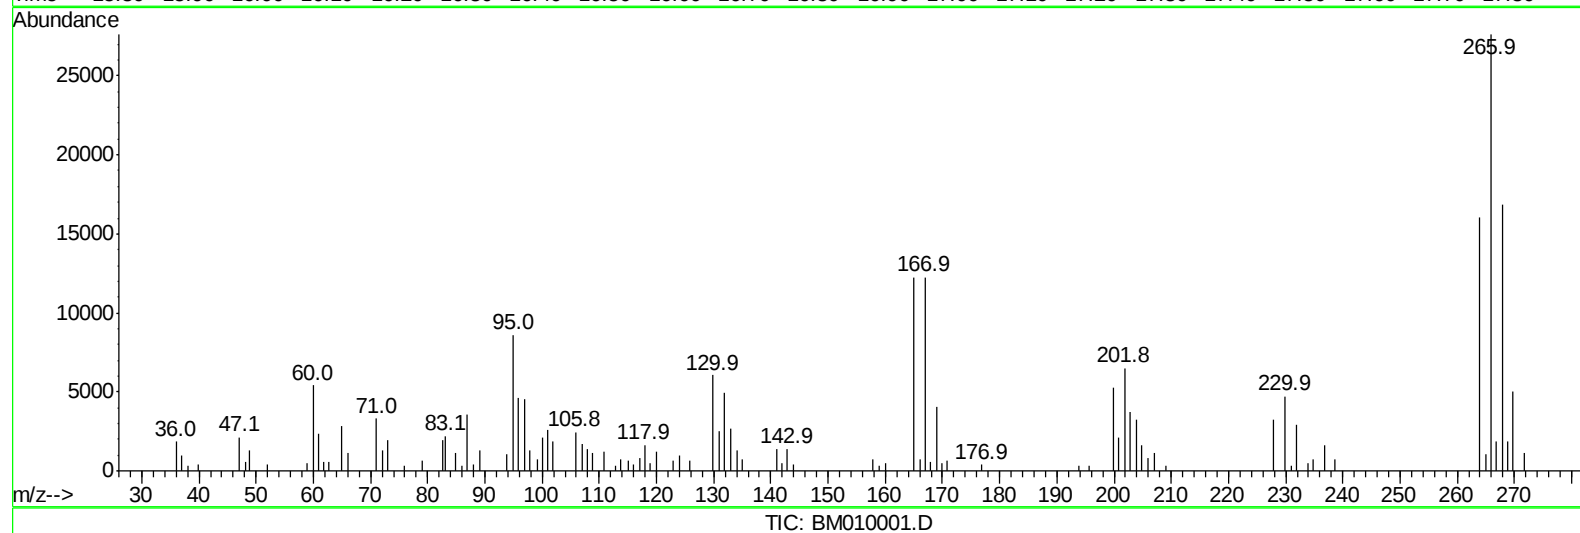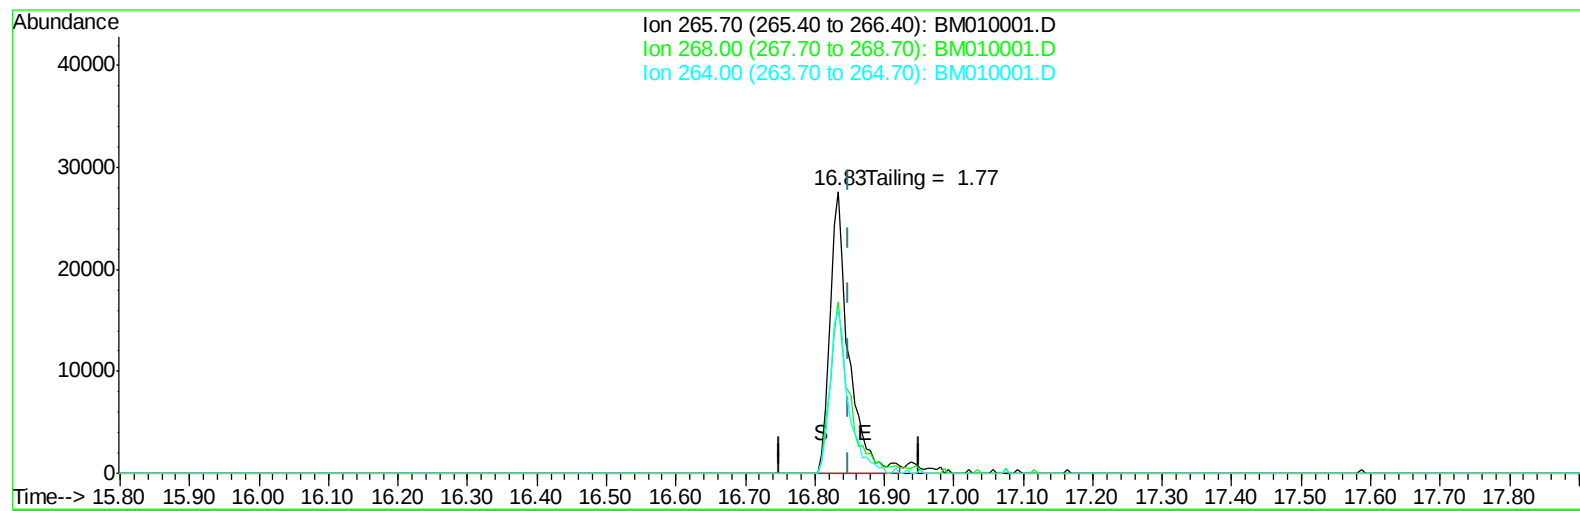

(69) Pentachlorophenol (C)

16.833min (-0.017) 0.00ng

response 51141

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.14
264.00	61.20	57.94
0.00	0.00	0.00