


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051117\
 Data File : BM009983.D
 Acq On : 11 May 2017 14:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 19:50:16 2017

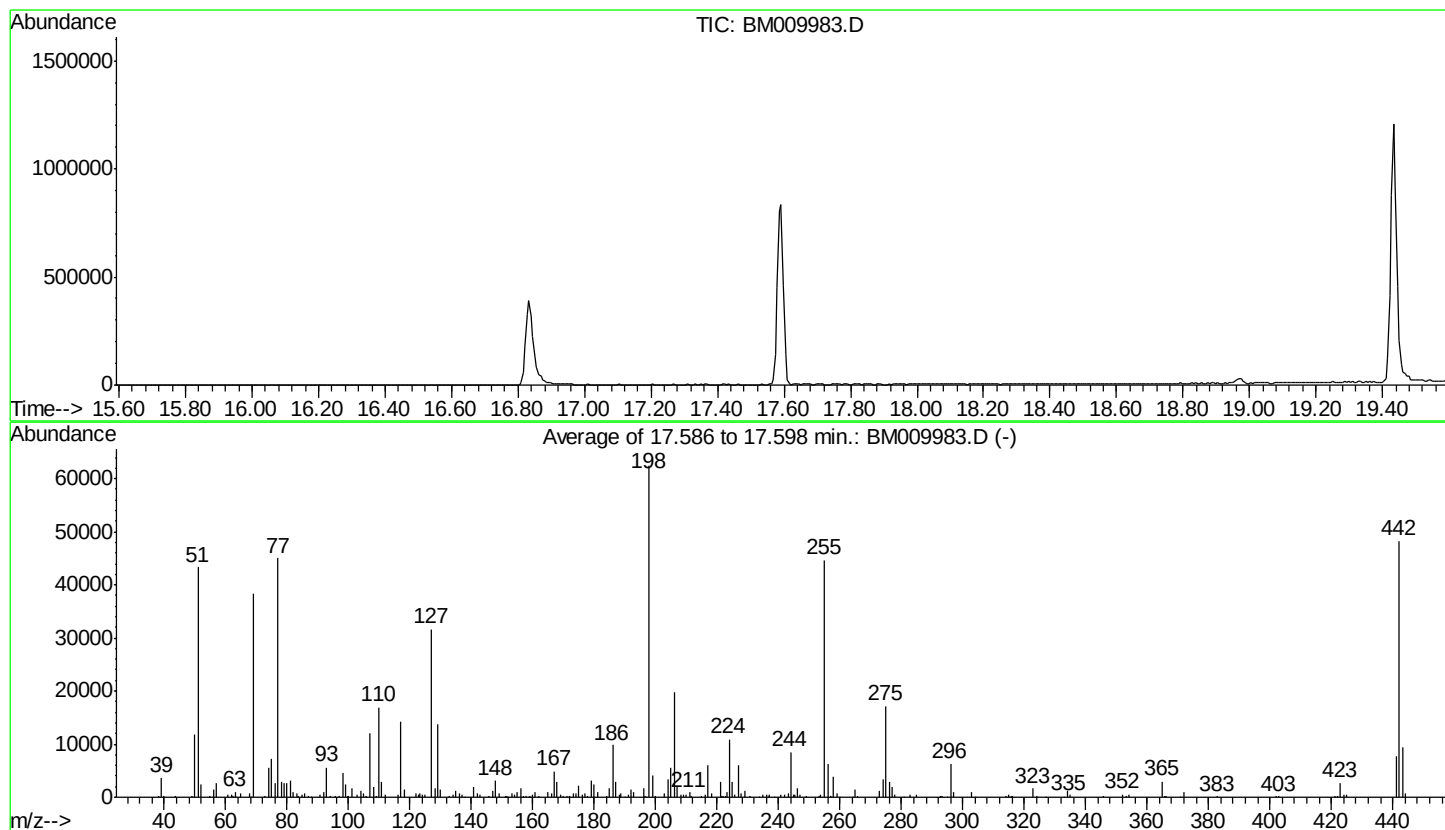

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.3	43317	PASS
68	69	0.00	2	1.7	641	PASS
69	198	0.00	100	61.3	38277	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	31706	PASS
197	198	0.00	2	0.4	222	PASS
198	198	100	100	100.0	62464	PASS
199	198	5	9	6.6	4119	PASS
275	198	10	60	27.5	17149	PASS
365	198	1	100	4.7	2921	PASS
441	442	0.01	24	15.8	7638	PASS
442	198	50	100	77.3	48261	PASS
443	442	15	24	19.7	9529	PASS