


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051117\
 Data File : BM010001.D
 Acq On : 12 May 2017 01:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 19:50:16 2017

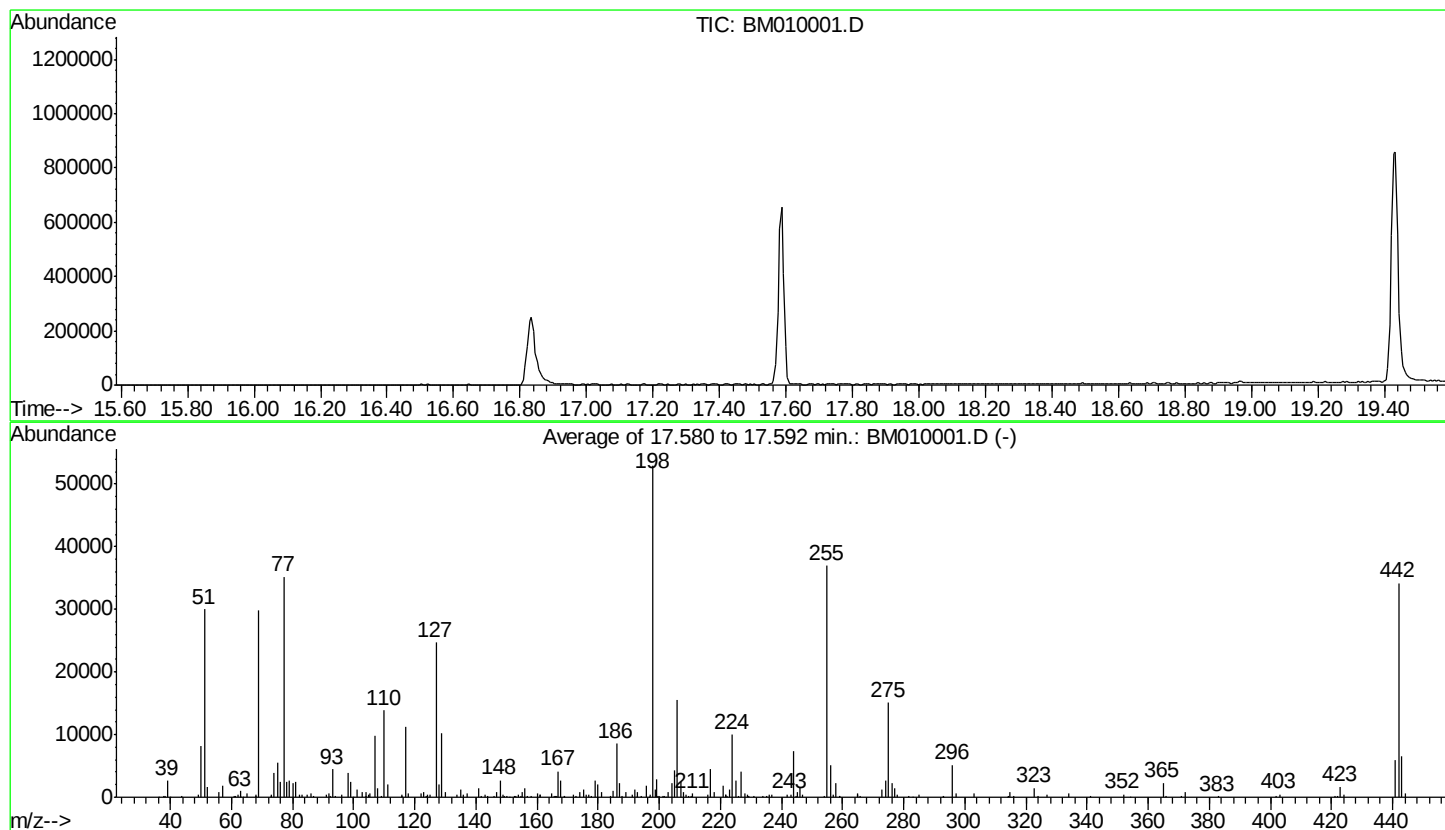

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	29960	PASS
68	69	0.00	2	1.6	489	PASS
69	198	0.00	100	56.6	29944	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	24648	PASS
197	198	0.00	2	0.6	323	PASS
198	198	100	100	100.0	52938	PASS
199	198	5	9	5.6	2940	PASS
275	198	10	60	28.6	15116	PASS
365	198	1	100	4.4	2324	PASS
441	442	0.01	24	17.2	5892	PASS
442	198	50	100	64.6	34221	PASS
443	442	15	24	19.0	6500	PASS