




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM034998.D
 Acq On : 11 May 2022 22:58
 Operator : CG/JU
 Sample : N2707-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA4

Manual IntegrationsAPPROVED

Quant Time: May 12 03:31:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 16:40:09 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

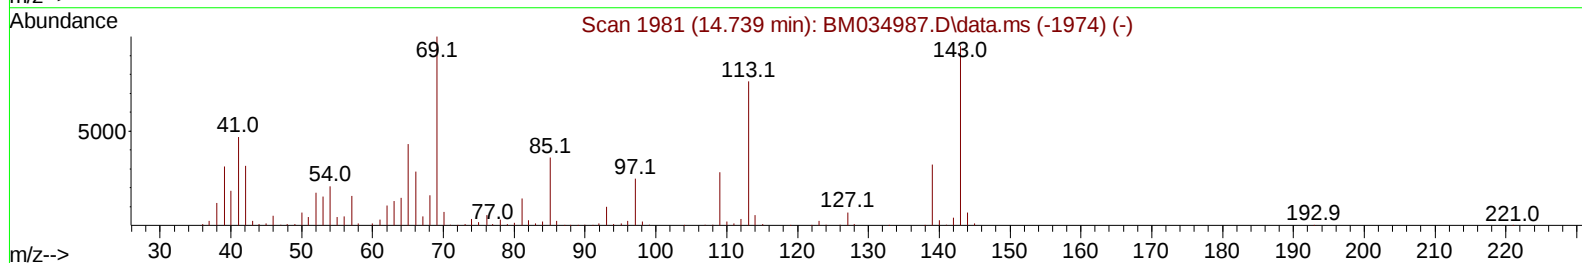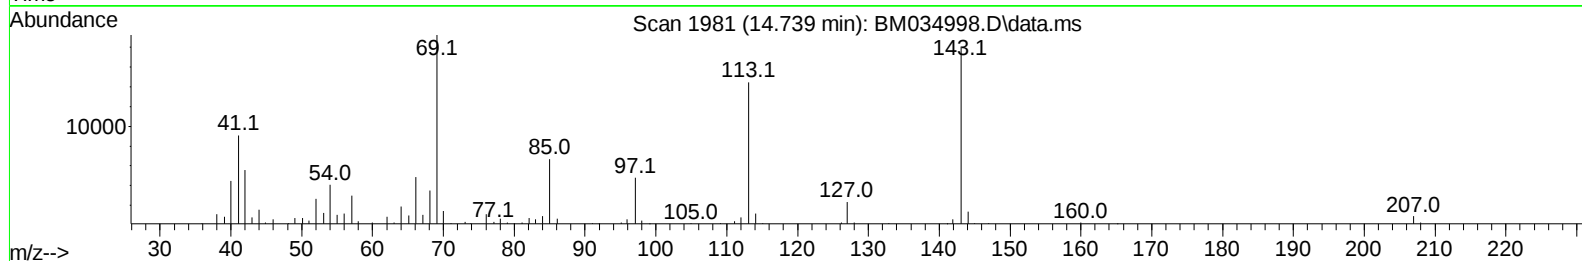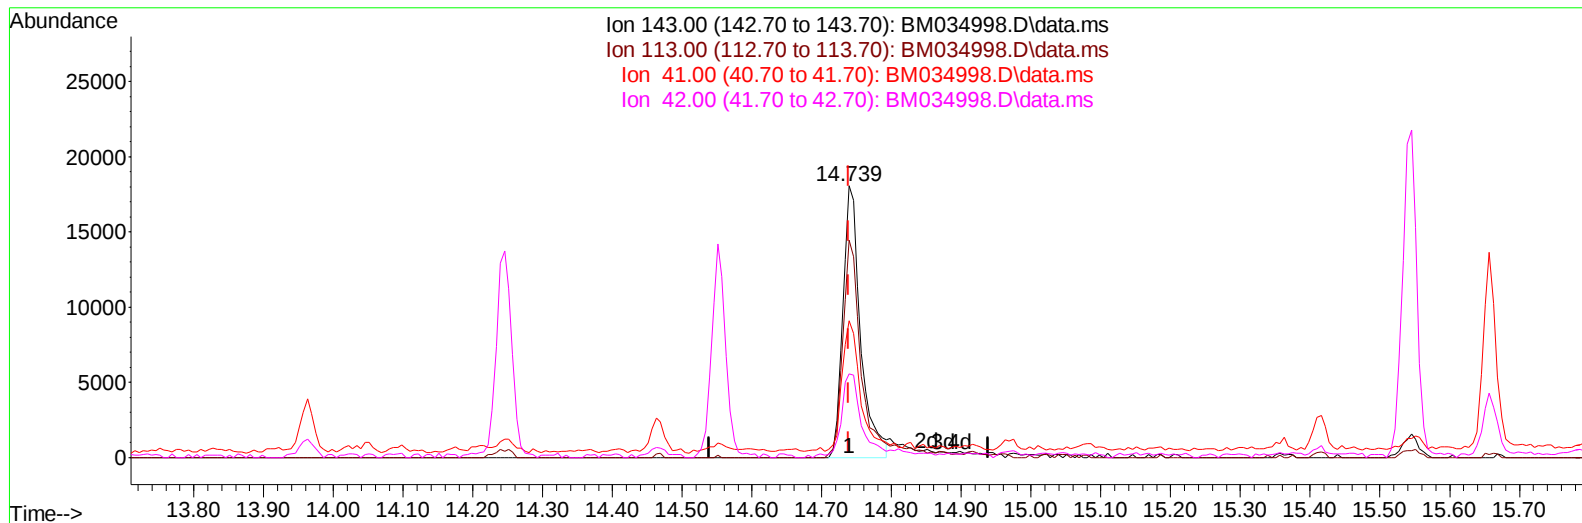

TIC: BM034998.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.000) 4.73 ng/u1

response 31758

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	80.00
41.00	42.20	50.29
42.00	28.30	30.87




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM034998.D
 Acq On : 11 May 2022 22:58
 Operator : CG/JU
 Sample : N2707-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA4

Manual IntegrationsAPPROVED

Quant Time: May 12 03:31:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 16:40:09 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

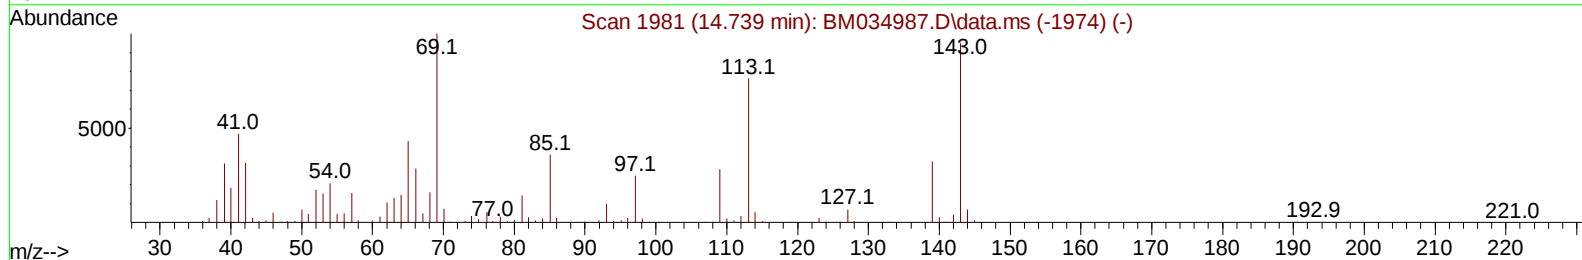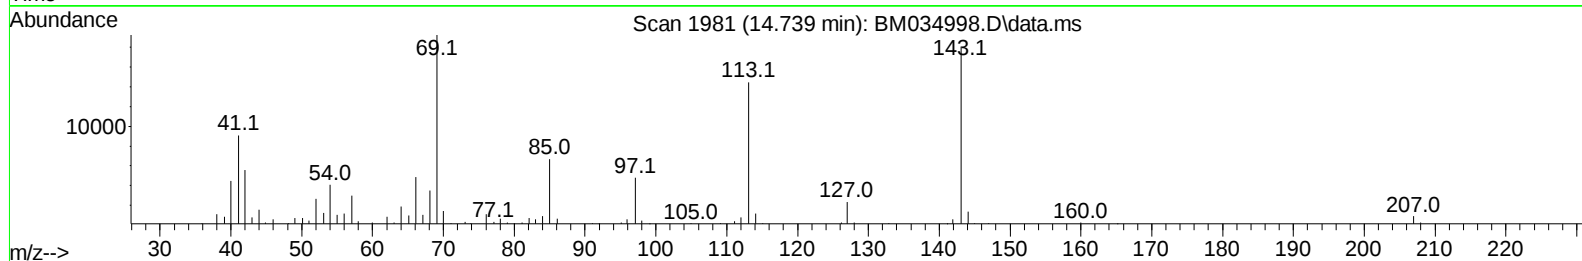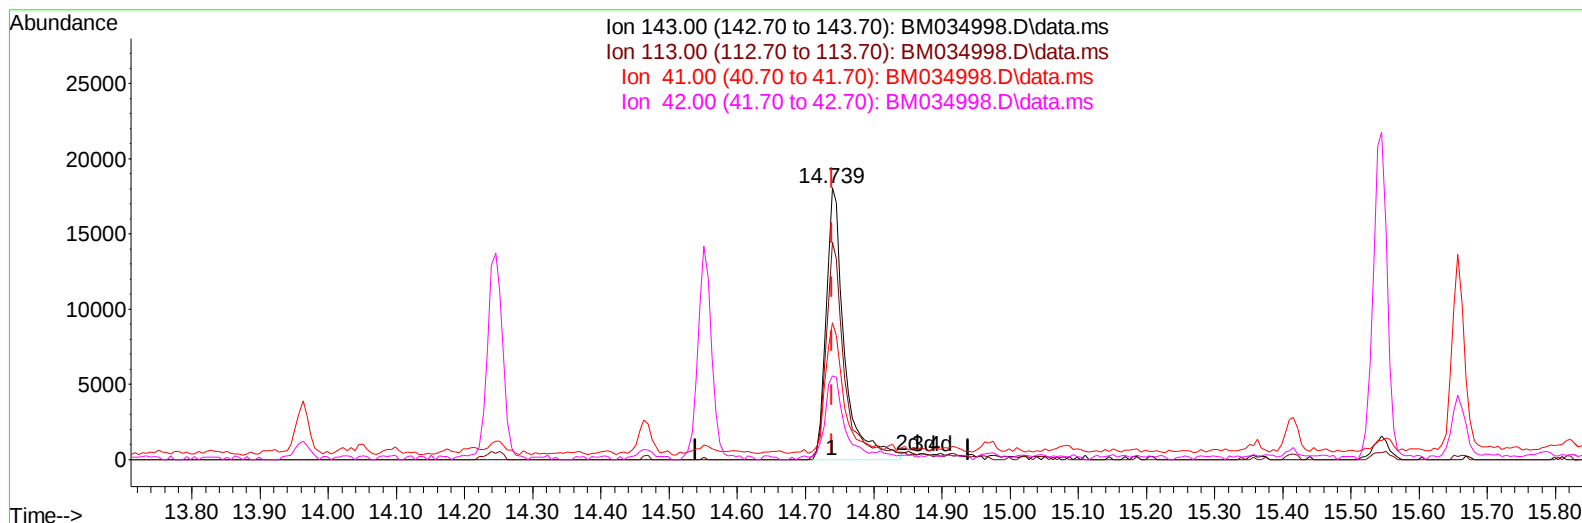

TIC: BM034998.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.000) 5.06 ng/ul m

response 33919

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	80.00
41.00	42.20	50.29
42.00	28.30	30.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM034998.D
 Acq On : 11 May 2022 22:58
 Operator : CG/JU
 Sample : N2707-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 03:31:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 16:40:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	250595	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	987682	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	520666	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	919609	20.000	ng/ul	0.00
79) Chrysene-d12	21.468	240	802745	20.000	ng/ul	0.00
88) Perylene-d12	23.856	264	902038	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	26693	4.456	ng/uL	0.00
4) Pyridine-d5	3.787	84	87107	5.276	ng/ul	0.01
7) Phenol-d5	7.087	99	120187	5.544	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.252	67	374220	27.502	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	393246	23.083	ng/ul	0.00
15) 4-Methylphenol-d8	8.628	113	232501	13.154	ng/ul	0.00
21) Nitrobenzene-d5	9.081	128	240698	31.796	ng/ul	0.00
24) 2-Nitrophenol-d4	9.804	143	251226	30.769	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	386931	25.322	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	467820	21.502	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	1210033	30.815	ng/ul	0.00
49) Acenaphthylene-d8	14.245	160	1467858	29.460	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	33919m	5.056	ng/ul	0.00
60) Fluorene-d10	15.545	176	1008303	30.437	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	154130	26.597	ng/ul	0.00
73) Anthracene-d10	17.392	188	1541720	34.458	ng/ul	0.00
81) Pyrene-d10	19.680	212	1605444	32.028	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.703	264	1747084	37.059	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034998.D
Acq On : 11 May 2022 22:58
Operator : CG/JU
Sample : N2707-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 03:31:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 16:40:09 2022
Response via : Initial Calibration

