

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM034981.D
 Acq On : 11 May 2022 12:41
 Operator : CG/JU
 Sample : N2603-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW489

Quant Time: May 12 03:27:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 16:40:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	209930	20.000	ng/u1	0.00
20) Naphthalene-d8	10.722	136	953820	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.551	164	631228	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.292	188	1275020	20.000	ng/u1	0.00
79) Chrysene-d12	21.468	240	939497	20.000	ng/u1	0.00
88) Perylene-d12	23.850	264	795946	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	20744	4.134	ng/uL	0.00
4) Pyridine-d5	3.781	84	101708	7.354	ng/u1	0.00
7) Phenol-d5	7.081	99	401310	22.097	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.245	67	281257	24.674	ng/u1	0.00
11) 2-Chlorophenol-d4	7.451	132	353409	24.764	ng/u1	0.00
15) 4-Methylphenol-d8	8.622	113	347692	23.482	ng/u1	0.00
21) Nitrobenzene-d5	9.075	128	179020	24.488	ng/u1	0.00
24) 2-Nitrophenol-d4	9.798	143	194896	24.717	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.339	165	338827	22.961	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	321959	15.324	ng/u1	0.00
46) Dimethylphthalate-d6	13.963	166	1283164	26.954	ng/u1	0.00
49) Acenaphthylene-d8	14.245	160	1427785	23.637	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	173333	21.310	ng/u1	0.00
60) Fluorene-d10	15.545	176	1066924	26.565	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	172402	21.458	ng/u1	0.00
73) Anthracene-d10	17.392	188	1681456	27.106	ng/u1	0.00
81) Pyrene-d10	19.680	212	1767641	30.131	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.697	264	1172577	28.188	ng/u1	0.00


Target Compounds					Qvalue
16) Acetophenone	8.739	105	45332	1.972 ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034981.D
Acq On : 11 May 2022 12:41
Operator : CG/JU
Sample : N2603-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW489


Quant Time: May 12 03:27:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 16:40:09 2022
Response via : Initial Calibration

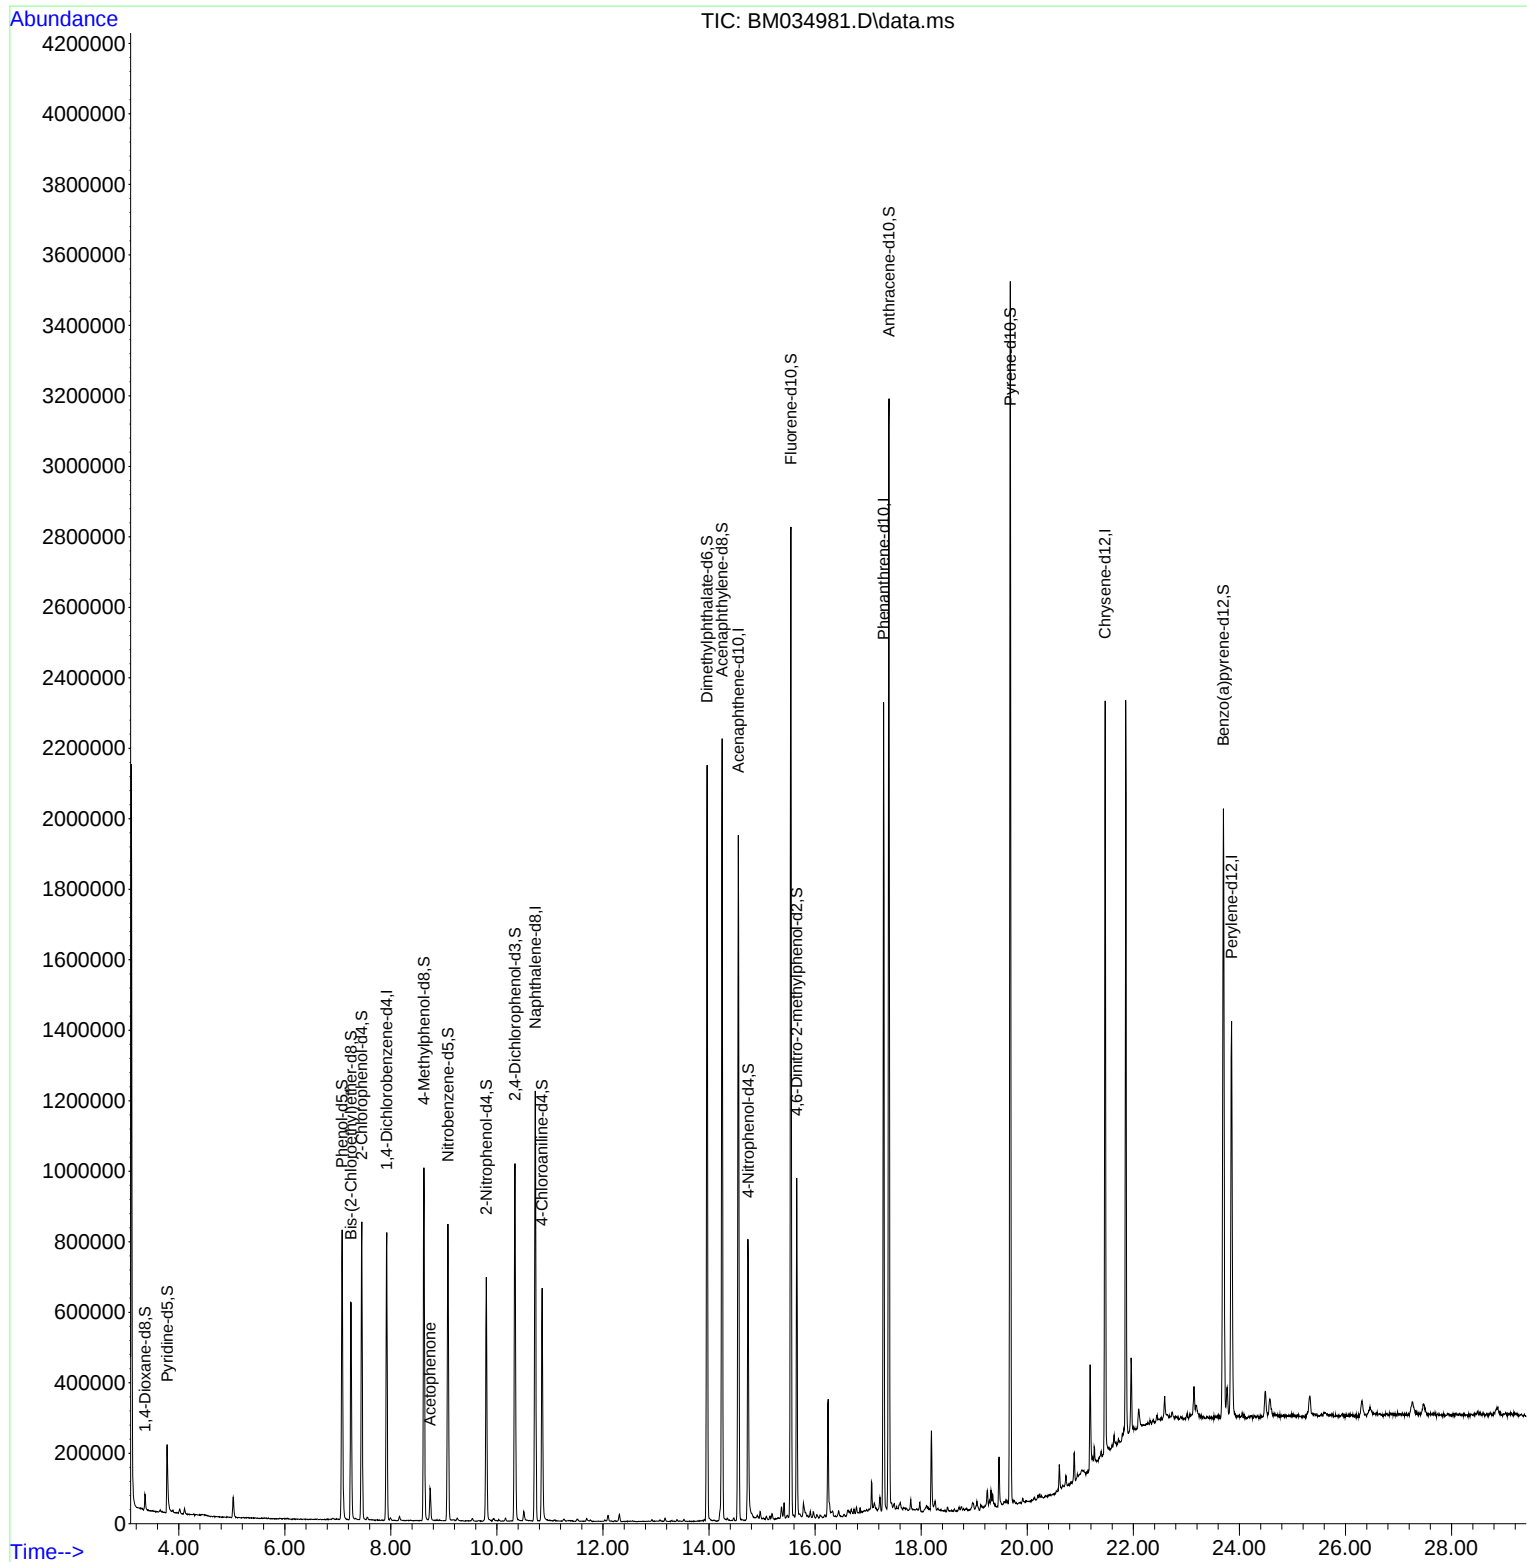

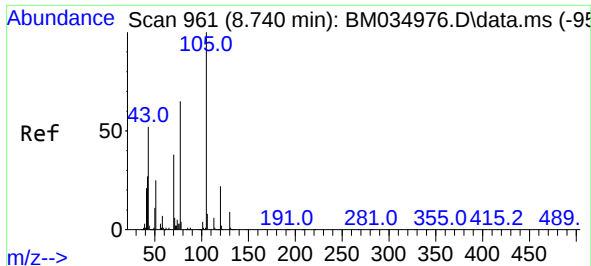

#16
 Acetophenone
 Concen: 1.972 ng/ul
 RT: 8.739 min Scan# 961
 Delta R.T. -0.006 min
 Lab File: BM034981.D
 Acq: 11 May 2022 12:41

Instrument :
 BNA_M
 ClientSampleId :
 EW489

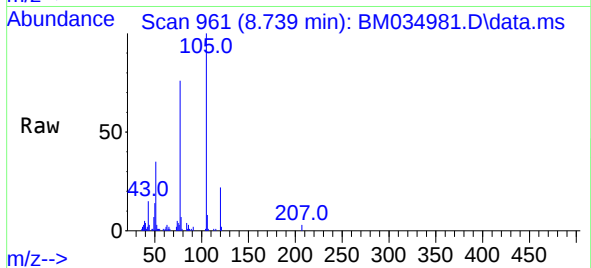

Tgt Ion:105 Resp: 45332

Ion	Ratio	Lower	Upper
105	100		
77	76.0	62.4	93.6
51	34.7	23.8	35.6

