

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM034977.D
 Acq On : 11 May 2022 10:17
 Operator : CG/JU
 Sample : PB144571BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	54	rVB	50372	65461	1.39%	0.125%
2	3.775	114	117	134	rBV	657937	1035376	22.06%	1.975%
3	4.110	170	174	178	rVB	16259	22426	0.48%	0.043%
4	7.081	672	679	690	rBV	804235	1261691	26.88%	2.407%
5	7.245	701	707	722	rVB	637036	1000082	21.31%	1.908%
6	7.451	735	742	751	rBV	862595	1348892	28.74%	2.573%
7	7.916	813	821	831	rBV	830851	1366363	29.11%	2.606%
8	8.622	934	941	955	rBV	1042005	1627306	34.67%	3.104%
9	9.075	1010	1018	1028	rBV	849651	1354315	28.86%	2.584%
10	9.798	1132	1141	1152	rBV	692445	1128463	24.04%	2.153%
11	10.339	1226	1233	1244	rBV	991016	1640814	34.96%	3.130%
12	10.722	1290	1298	1309	rVB	1253377	2095110	44.64%	3.997%
13	10.851	1313	1320	1332	rBV	1039064	1764579	37.60%	3.366%
14	12.310	1562	1568	1573	rBV2	16598	29287	0.62%	0.056%
15	13.963	1842	1849	1861	rBV	2058927	2773479	59.09%	5.291%
16	14.245	1889	1897	1914	rBV	2136339	3120279	66.48%	5.952%
17	14.551	1942	1949	1957	rBV	2076541	2963573	63.14%	5.653%
18	14.733	1973	1980	1993	rBV	800904	1231714	26.24%	2.350%
19	15.539	2111	2117	2130	rBV	2758927	3978415	84.77%	7.589%
20	15.651	2130	2136	2149	rVV	848347	1200366	25.58%	2.290%
21	15.780	2153	2158	2163	rVB	34214	48427	1.03%	0.092%
22	16.321	2246	2250	2255	rBV3	9756	13389	0.29%	0.026%
23	16.974	2358	2361	2366	rVB5	4775	5303	0.11%	0.010%
24	17.080	2375	2379	2383	rVB4	3915	6846	0.15%	0.013%
25	17.292	2408	2415	2425	rBV	2532011	3423157	72.94%	6.530%
26	17.392	2425	2432	2444	rVV	3084660	4351399	92.71%	8.301%
27	17.474	2444	2446	2452	rVB5	3985	4848	0.10%	0.009%
28	17.668	2475	2479	2483	rVB4	3450	6170	0.13%	0.012%
29	19.245	2743	2747	2752	rBV	33027	44049	0.94%	0.084%
30	19.315	2754	2759	2763	rBV	30637	41706	0.89%	0.080%
31	19.621	2809	2811	2814	rVB4	6189	5078	0.11%	0.010%
32	19.680	2815	2821	2828	rBV	3614661	4693320	100.00%	8.953%
33	21.468	3120	3125	3133	rBV	2516358	3037511	64.72%	5.794%
34	23.697	3497	3504	3512	rBV2	1665899	3278024	69.84%	6.253%
35	23.850	3523	3530	3539	rVB2	1222842	2454157	52.29%	4.682%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034977.D
Acq On : 11 May 2022 10:17
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52421375

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034977.D
Acq On : 11 May 2022 10:17
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

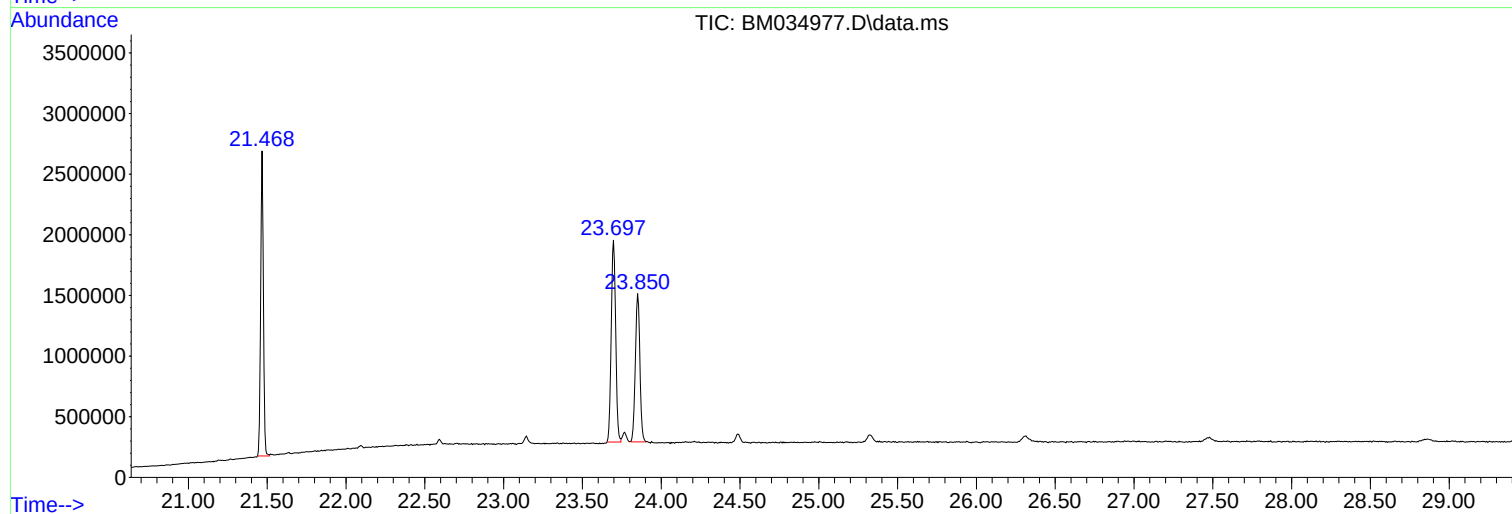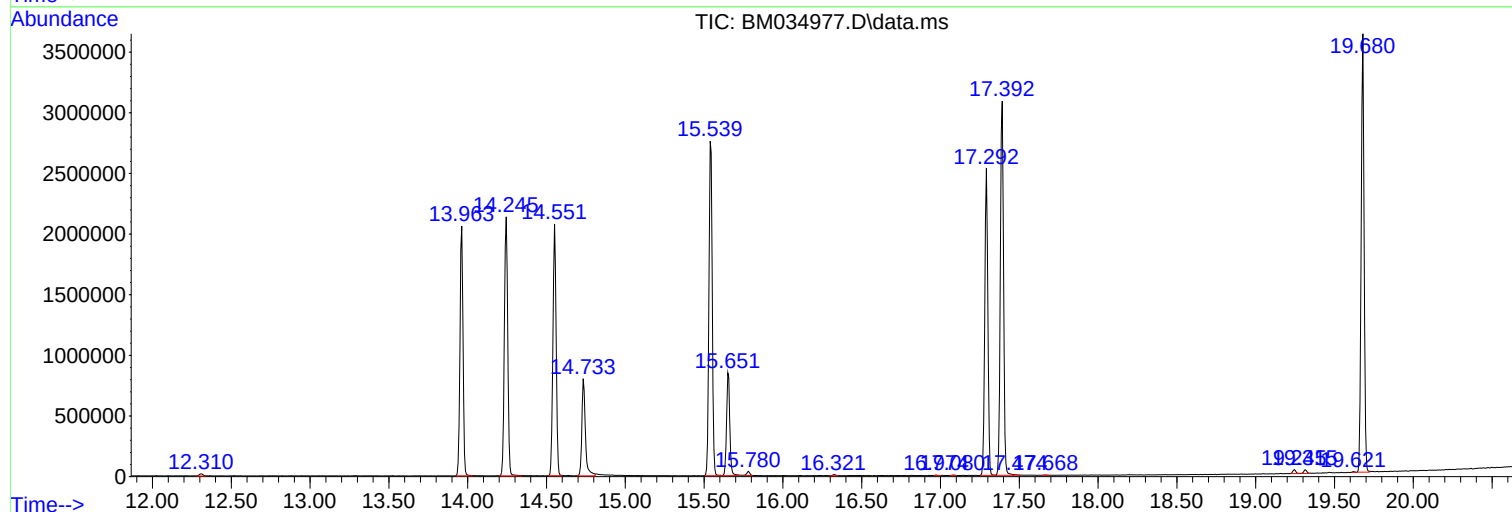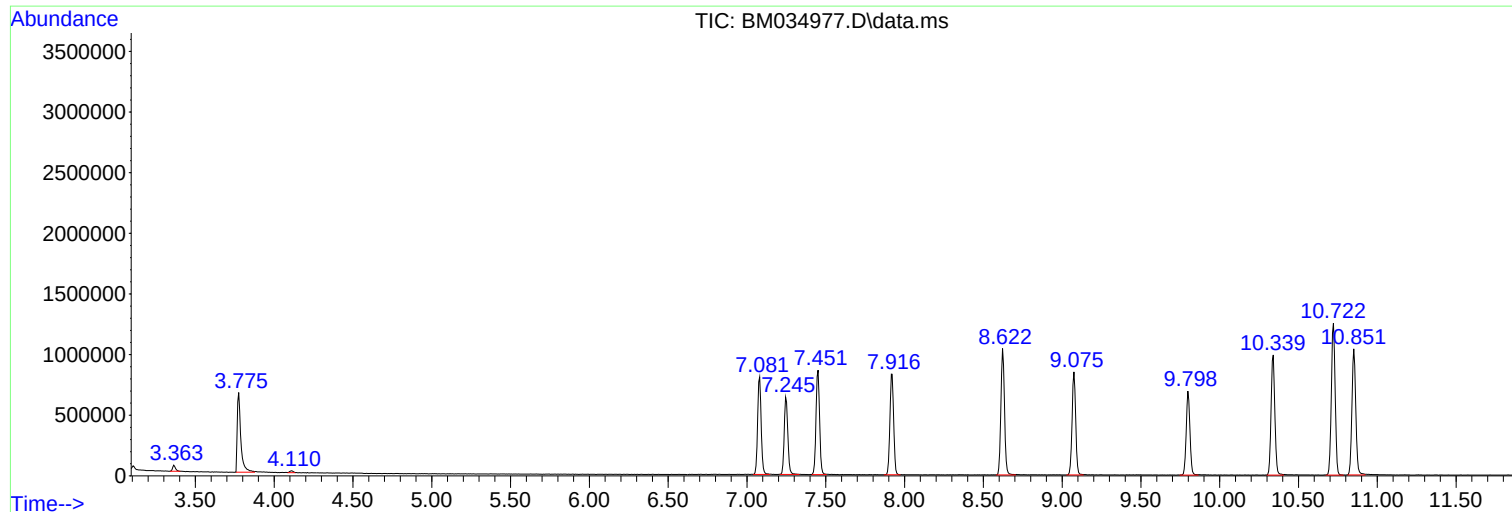

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034977.D
Acq On : 11 May 2022 10:17
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM034977.D
Acq On : 11 May 2022 10:17
Operator : CG/JU
Sample : PB144571BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc