

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM035006.D
 Acq On : 12 May 2022 04:21
 Operator : CG/JU
 Sample : PB144632BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	53	rBV	57038	75964	2.25%	0.184%
2	3.775	114	117	135	rBV	683090	1021618	30.26%	2.481%
3	4.110	171	174	182	rVB3	15806	22948	0.68%	0.056%
4	7.081	673	679	692	rBV	818749	1259984	37.32%	3.060%
5	7.245	701	707	721	rVV	594301	944503	27.98%	2.294%
6	7.451	735	742	751	rBV	859674	1350601	40.00%	3.280%
7	7.922	814	822	831	rBV	729803	1167101	34.57%	2.834%
8	8.622	934	941	953	rBV	963252	1548105	45.85%	3.760%
9	9.075	1010	1018	1030	rBV	777675	1265540	37.48%	3.073%
10	9.186	1034	1037	1040	rBV5	2370	3608	0.11%	0.009%
11	9.798	1134	1141	1155	rBV	631869	1058365	31.35%	2.570%
12	10.339	1225	1233	1249	rBV	901060	1502279	44.50%	3.648%
13	10.722	1290	1298	1306	rBV	968205	1595413	47.26%	3.875%
14	10.851	1311	1320	1341	rBV	885370	1527428	45.24%	3.709%
15	12.310	1564	1568	1573	rVB2	15709	23232	0.69%	0.056%
16	13.963	1842	1849	1859	rBV	1428353	1945284	57.62%	4.724%
17	14.245	1890	1897	1904	rBV	1688385	2406457	71.28%	5.844%
18	14.551	1941	1949	1958	rBV	1378628	1919311	56.85%	4.661%
19	14.739	1975	1981	1999	rBV	538579	946458	28.03%	2.298%
20	14.963	2017	2019	2023	rVB5	2746	3382	0.10%	0.008%
21	15.539	2111	2117	2128	rBV	1990964	2846567	84.31%	6.913%
22	15.657	2131	2137	2146	rBV	625346	841359	24.92%	2.043%
23	15.780	2154	2158	2165	rVB2	27136	38586	1.14%	0.094%
24	16.321	2247	2250	2255	rVB4	6192	8613	0.26%	0.021%
25	16.968	2358	2360	2365	rBV4	3582	4257	0.13%	0.010%
26	17.080	2376	2379	2383	rVB5	2967	3857	0.11%	0.009%
27	17.292	2408	2415	2423	rBV	1464679	2019320	59.81%	4.904%
28	17.392	2425	2432	2446	rVV	1996086	2908351	86.14%	7.063%
29	17.786	2496	2499	2503	rBV6	2500	3580	0.11%	0.009%
30	18.192	2565	2568	2569	rBV3	4771	4051	0.12%	0.010%
31	19.245	2743	2747	2753	rVB3	23748	32180	0.95%	0.078%
32	19.315	2755	2759	2764	rVV	20647	27009	0.80%	0.066%
33	19.680	2815	2821	2828	rBV	2344316	3181298	94.23%	7.726%
34	21.462	3119	3124	3130	rBV	1617160	2075423	61.47%	5.040%
35	23.697	3497	3504	3511	rBV2	1743830	3376146	100.00%	8.199%
36	23.850	3523	3530	3541	rVB	1088127	2219053	65.73%	5.389%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035006.D
Acq On : 12 May 2022 04:21
Operator : CG/JU
Sample : PB144632BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK632

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Title : SVOA CALIBRATION


Sum of corrected areas: 41177231

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035006.D
Acq On : 12 May 2022 04:21
Operator : CG/JU
Sample : PB144632BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

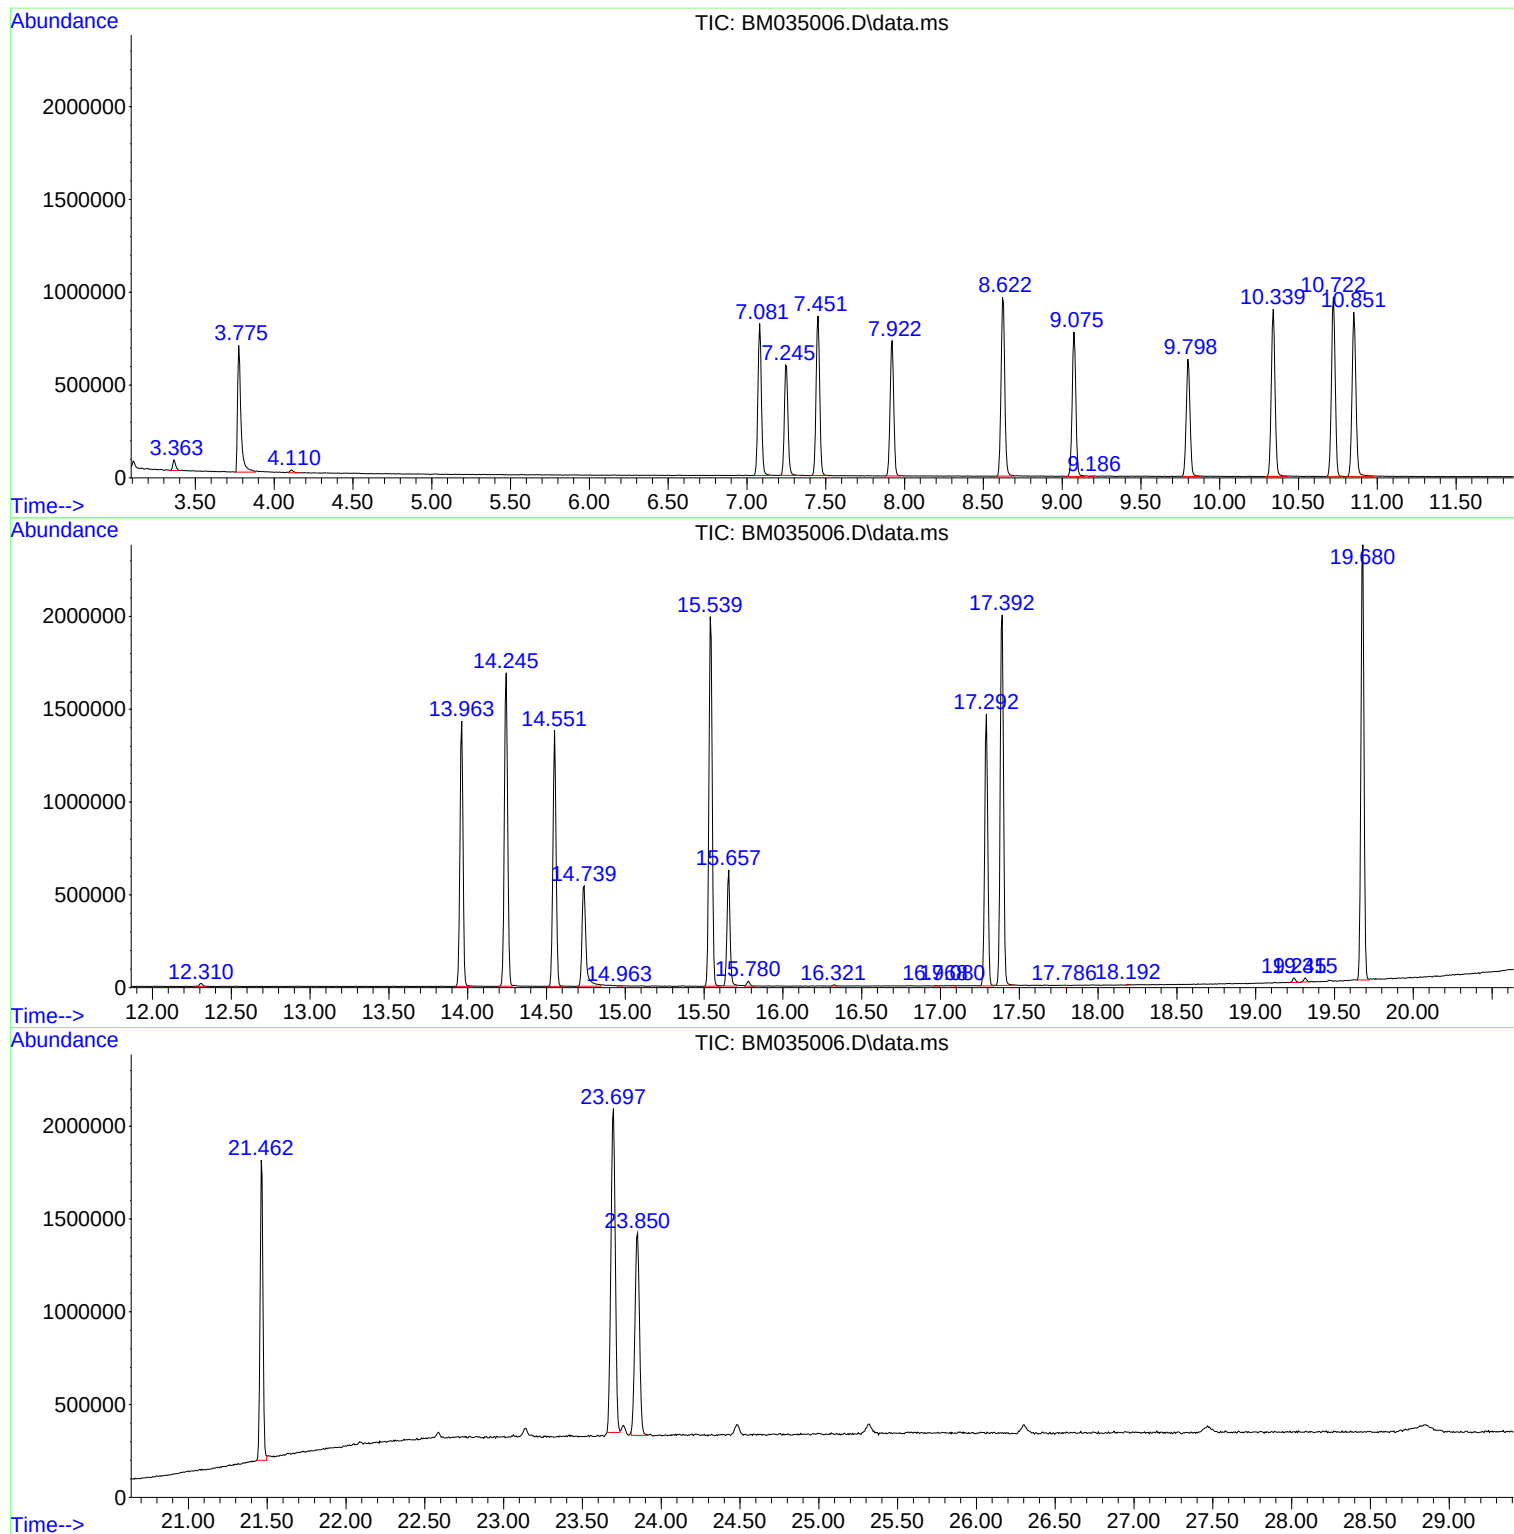

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035006.D
Acq On : 12 May 2022 04:21
Operator : CG/JU
Sample : PB144632BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035006.D
Acq On : 12 May 2022 04:21
Operator : CG/JU
Sample : PB144632BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc