

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM035009.D
 Acq On : 12 May 2022 06:09
 Operator : CG/JU
 Sample : N2707-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	53	rVB	45138	59669	1.25%	0.126%
2	3.781	114	118	133	rBV	226607	368188	7.70%	0.775%
3	4.110	169	174	179	rBV	14739	21179	0.44%	0.045%
4	4.640	260	264	269	rBV2	23392	30926	0.65%	0.065%
5	5.022	326	329	334	rBV2	6940	10016	0.21%	0.021%
6	7.081	671	679	694	rVB	223826	362702	7.59%	0.763%
7	7.246	700	707	717	rBV	813599	1280518	26.80%	2.694%
8	7.451	734	742	750	rBV	885758	1388991	29.07%	2.922%
9	7.551	756	759	765	rVB6	3784	6016	0.13%	0.013%
10	7.922	815	822	830	rBV	696004	1119452	23.43%	2.355%
11	7.993	830	834	841	rVB3	9525	14987	0.31%	0.032%
12	8.622	935	941	953	rBV	632339	1017034	21.28%	2.140%
13	9.075	1011	1018	1028	rBV	1057205	1716329	35.92%	3.611%
14	9.257	1046	1049	1053	rVB4	4863	5637	0.12%	0.012%
15	9.534	1091	1096	1103	rVB2	27204	44159	0.92%	0.093%
16	9.798	1133	1141	1150	rBV	837042	1385320	28.99%	2.914%
17	10.339	1226	1233	1246	rBV	1095715	1835000	38.40%	3.860%
18	10.522	1259	1264	1266	rBV5	3432	5598	0.12%	0.012%
19	10.722	1289	1298	1310	rBV	943464	1602685	33.54%	3.372%
20	10.851	1312	1320	1333	rBV	954668	1646121	34.45%	3.463%
21	11.522	1428	1434	1437	rBV6	2790	5924	0.12%	0.012%
22	11.769	1472	1476	1482	rVB7	3247	5036	0.11%	0.011%
23	12.157	1536	1542	1549	rBV2	12572	18903	0.40%	0.040%
24	12.304	1562	1567	1574	rVB3	21869	37486	0.78%	0.079%
25	12.963	1675	1679	1684	rVB5	4546	8879	0.19%	0.019%
26	13.051	1690	1694	1700	rBV7	2736	5782	0.12%	0.012%
27	13.110	1700	1704	1708	rVB5	3600	5206	0.11%	0.011%
28	13.392	1748	1752	1760	rBV	22891	30747	0.64%	0.065%
29	13.522	1770	1774	1781	rBV6	5176	8631	0.18%	0.018%
30	13.963	1842	1849	1855	rBV	2051010	2777459	58.12%	5.843%
31	14.245	1885	1897	1907	rBV	2229112	3286339	68.77%	6.913%
32	14.463	1931	1934	1938	rBV4	4196	4802	0.10%	0.010%
33	14.551	1938	1949	1961	rBV	1324807	1959568	41.01%	4.122%
34	14.639	1961	1964	1972	rVB5	3704	5294	0.11%	0.011%
35	14.739	1972	1981	1999	rBV	120948	241127	5.05%	0.507%
36	14.963	2016	2019	2023	rBV3	9757	11666	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
 Data File : BM035009.D
 Acq On : 12 May 2022 06:09
 Operator : CG/JU
 Sample : N2707-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
 Title : SVOA CALIBRATION

37	15.363	2082	2087	2092	rVV2	10714	16782	0.35%	0.035%
38	15.539	2111	2117	2128	rBV	2808320	3977860	83.24%	8.368%
39	15.657	2131	2137	2144	rBV	883346	1207771	25.27%	2.541%
40	15.780	2154	2158	2164	rVB	32458	46667	0.98%	0.098%
41	16.110	2208	2214	2218	rBV7	2850	4988	0.10%	0.010%
42	16.321	2246	2250	2256	rBV3	12522	19030	0.40%	0.040%
43	17.080	2373	2379	2383	rBV6	2501	5184	0.11%	0.011%
44	17.292	2408	2415	2422	rBV	1359259	1937267	40.54%	4.075%
45	17.386	2425	2431	2442	rBV	2797139	4093170	85.65%	8.611%
46	17.521	2450	2454	2458	rVB2	11443	14092	0.29%	0.030%
47	17.968	2527	2530	2535	rVB7	4645	6367	0.13%	0.013%
48	18.192	2562	2568	2577	rBV	124993	183380	3.84%	0.386%
49	18.257	2577	2579	2586	rVB5	8418	13166	0.28%	0.028%
50	19.245	2742	2747	2752	rBV2	36977	50726	1.06%	0.107%
51	19.315	2755	2759	2762	rBV	43061	57974	1.21%	0.122%
52	19.462	2781	2784	2793	rVV	94061	125377	2.62%	0.264%
53	19.621	2808	2811	2814	rBV5	10219	12276	0.26%	0.026%
54	19.680	2814	2821	2828	rBV	3296323	4412061	92.33%	9.282%
55	21.186	3073	3077	3084	rBV3	112218	178940	3.74%	0.376%
56	21.462	3119	3124	3133	rBV	1494632	1973391	41.30%	4.151%
57	23.697	3496	3504	3512	rBV2	2429558	4778755	100.00%	10.053%
58	23.850	3523	3530	3539	rVB2	1033259	2087180	43.68%	4.391%




Sum of corrected areas: 47535780

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035009.D
Acq On : 12 May 2022 06:09
Operator : CG/JU
Sample : N2707-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

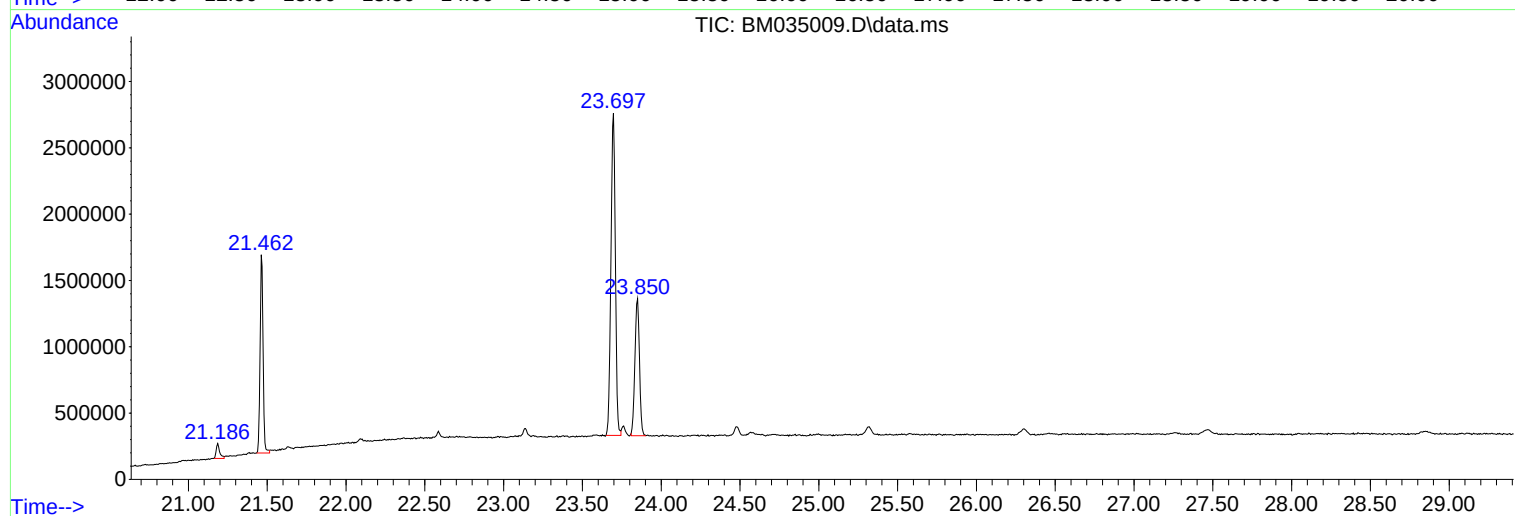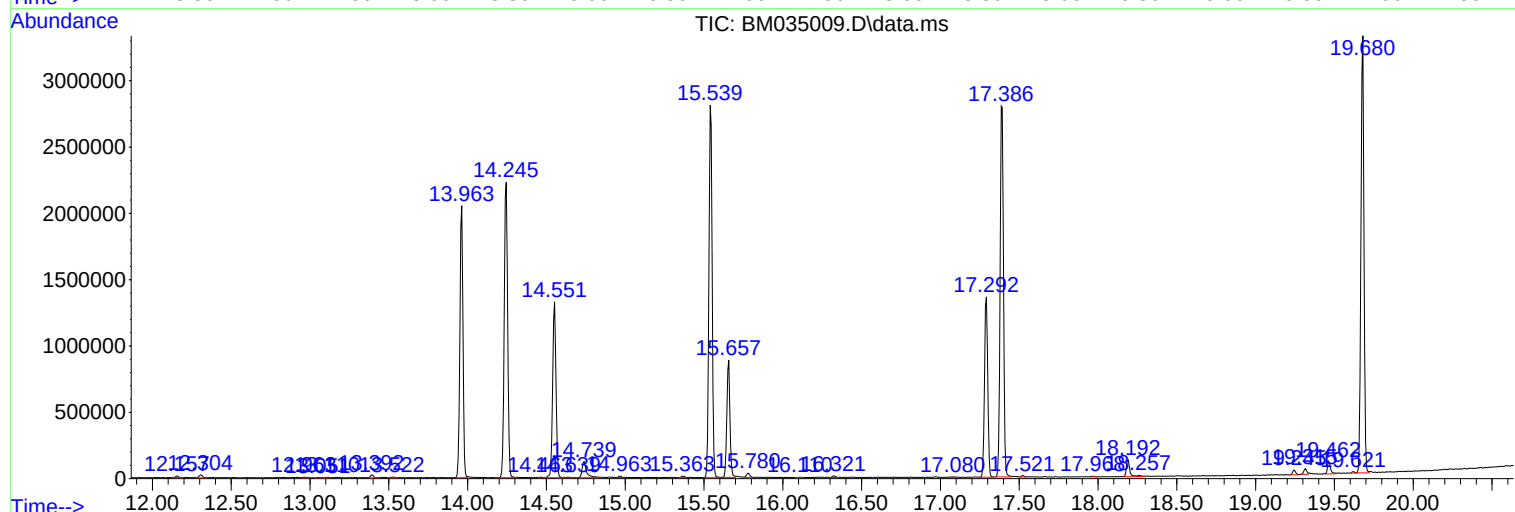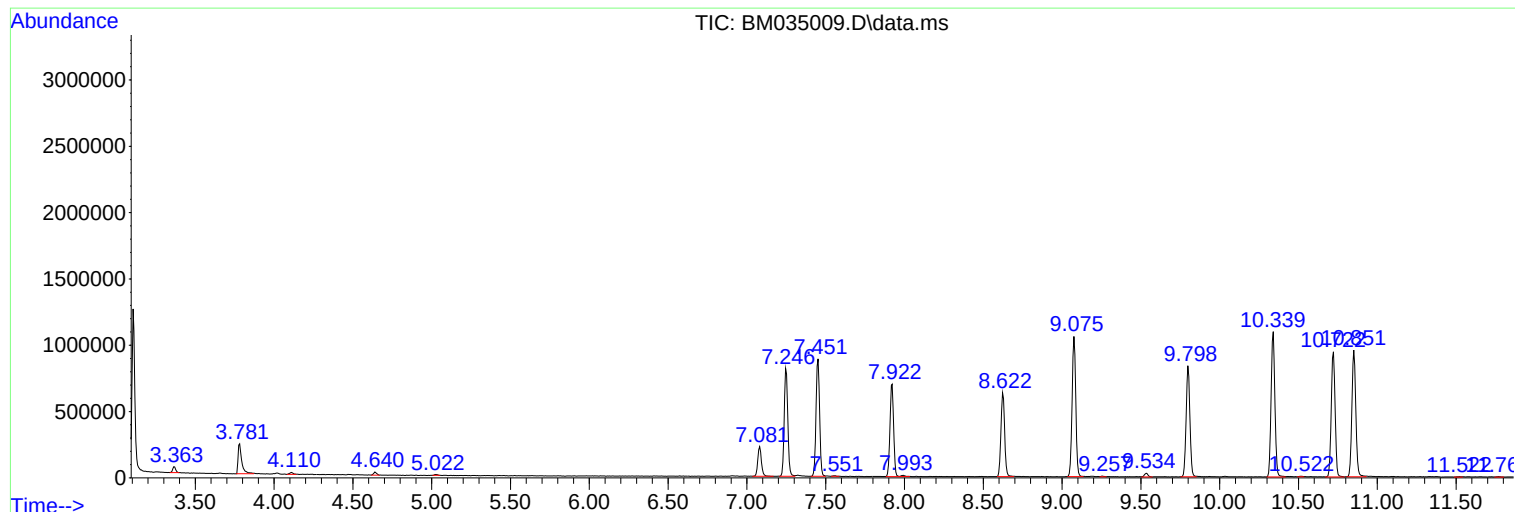

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035009.D
Acq On : 12 May 2022 06:09
Operator : CG/JU
Sample : N2707-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051122\
Data File : BM035009.D
Acq On : 12 May 2022 06:09
Operator : CG/JU
Sample : N2707-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------