

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051215\
 Data File : BM001254.D
 Acq On : 12 May 2015 11:40
 Operator : TP/IZ
 Sample : PB83268BL
 Misc : SBLK57
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051215.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.875	28	32	40	rVB2	56108	71864	1.41%	0.138%
2	3.440	124	128	134	rBV4	24149	31024	0.61%	0.059%
3	5.663	501	506	509	rBV5	6411	10431	0.20%	0.020%
4	6.634	664	671	684	rBV	969674	1446119	28.28%	2.768%
5	6.787	690	697	706	rBV	758243	1107534	21.66%	2.120%
6	6.881	710	713	717	rVB4	4953	7588	0.15%	0.015%
7	6.975	723	729	740	rBV	980085	1473803	28.83%	2.821%
8	7.075	742	746	754	rVB2	24830	39653	0.78%	0.076%
9	7.440	802	808	817	rVB	663485	1035717	20.26%	1.983%
10	7.669	844	847	851	rBV5	8232	11378	0.22%	0.022%
11	7.981	895	900	903	rBV3	7044	9252	0.18%	0.018%
12	8.116	917	923	926	rBV4	7841	13505	0.26%	0.026%
13	8.169	926	932	946	rVB	1222718	1876679	36.71%	3.592%
14	8.598	999	1005	1014	rBV	931267	1461652	28.59%	2.798%
15	8.675	1014	1018	1025	rVB	16724	24950	0.49%	0.048%
16	9.322	1120	1128	1138	rBV	802217	1254418	24.53%	2.401%
17	9.857	1213	1219	1230	rBV	1199311	1883137	36.83%	3.605%
18	10.228	1275	1282	1289	rBV	919388	1476346	28.88%	2.826%
19	10.375	1300	1307	1321	rBV	1263678	2071905	40.52%	3.966%
20	12.457	1657	1661	1666	rVB3	8221	11495	0.22%	0.022%
21	12.716	1701	1705	1711	rBV3	12393	18376	0.36%	0.035%
22	13.539	1839	1845	1852	rBV	2155835	2838307	55.51%	5.433%
23	13.810	1884	1891	1901	rBV	2529981	3535721	69.15%	6.768%
24	14.121	1935	1944	1955	rVB2	1290742	1910181	37.36%	3.656%
25	14.345	1977	1982	2002	rBV	937456	1373866	26.87%	2.630%
26	15.121	2107	2114	2120	rBV	3298487	4377314	85.61%	8.379%
27	15.257	2131	2137	2150	rBV	1110253	1486146	29.07%	2.845%
28	15.357	2150	2154	2159	rVB	26234	37474	0.73%	0.072%
29	16.868	2405	2411	2421	rBV2	1498953	2113079	41.33%	4.045%
30	16.968	2421	2428	2439	rBV2	3443294	4661436	91.17%	8.923%
31	19.162	2797	2801	2807	rBV2	23423	32109	0.63%	0.061%
32	19.274	2814	2820	2830	rBV	3801534	5112849	100.00%	9.787%
33	20.874	3089	3092	3100	rBV8	17799	22332	0.44%	0.043%
34	21.074	3121	3126	3135	rBV	1758478	2275460	44.50%	4.356%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051215\
Data File : BM001254.D
Acq On : 12 May 2015 11:40
Operator : TP/IZ
Sample : PB83268BL
Misc : SBLK57
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051215.M
Title : SVOA CALIBRATION

35	22.509	3366	3370	3376	rbV9	18155	32449	0.63%	0.062%
36	23.062	3456	3464	3478	rbV2	2862403	4916770	96.16%	9.412%
37	23.192	3479	3486	3494	rbV	1294044	2178478	42.61%	4.170%


Sum of corrected areas: 52240797

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051215\
Data File : BM001254.D
Acq On : 12 May 2015 11:40
Operator : TP/IZ
Sample : PB83268BL
Misc : SBLK57
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051215.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

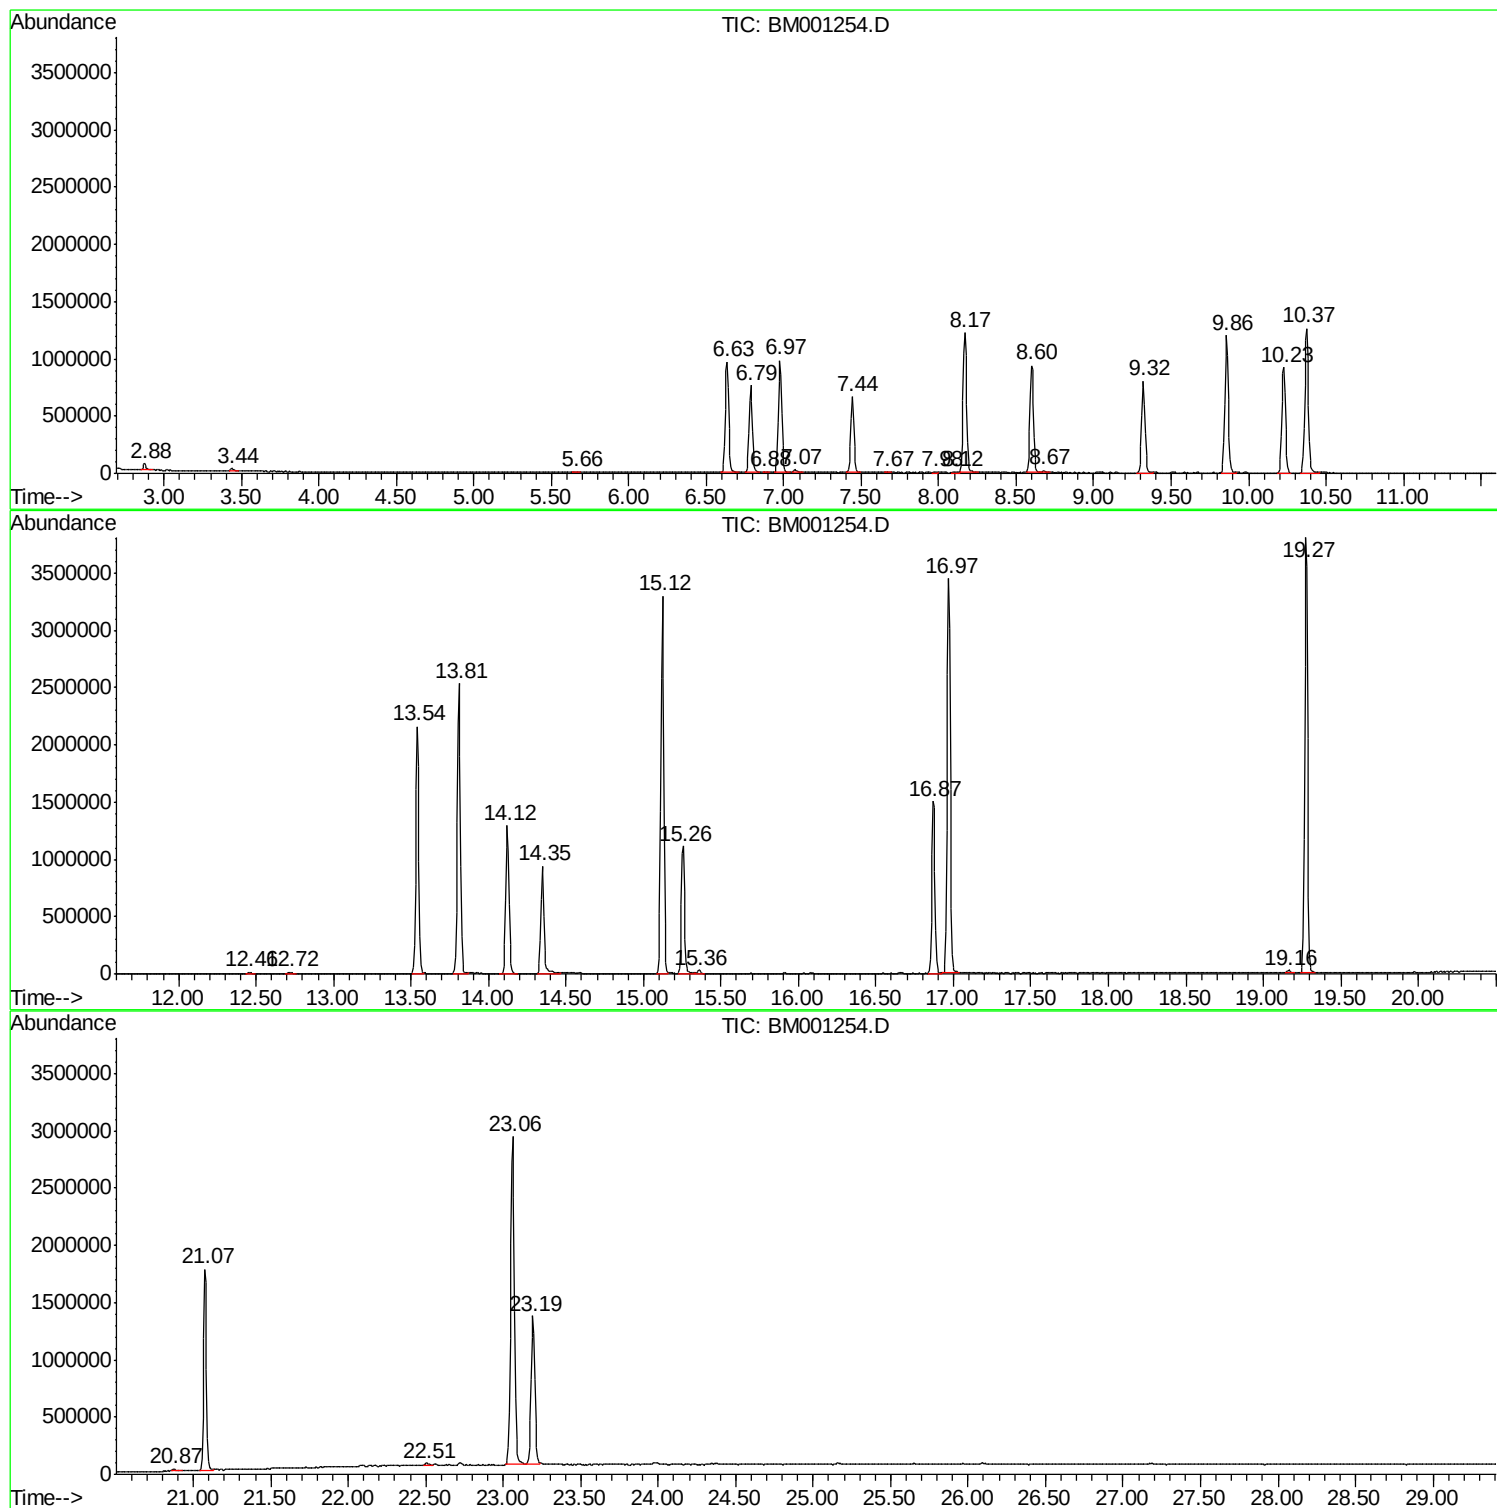

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051215\
Data File : BM001254.D
Acq On : 12 May 2015 11:40
Operator : TP/IZ
Sample : PB83268BL
Misc : SBLK57
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051215.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051215\
Data File : BM001254.D
Acq On : 12 May 2015 11:40
Operator : TP/IZ
Sample : PB83268BL
Misc : SBLK57
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK57

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051215.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc