

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
 Data File : BM005413.D
 Acq On : 12 May 2016 10:48
 Operator : UM/SJ
 Sample : H2847-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3J6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.934	717	722	733	rBV	71273	114861	4.11%	0.518%
2	7.093	743	749	760	rBV	249387	382301	13.69%	1.725%
3	7.293	777	783	794	rVB	262857	419207	15.01%	1.892%
4	7.757	855	862	870	rBV	255177	411038	14.72%	1.855%
5	8.463	977	982	1001	rBV	225763	374158	13.40%	1.688%
6	8.916	1052	1059	1073	rBV	306823	519431	18.60%	2.344%
7	9.634	1174	1181	1192	rBV	272158	443189	15.87%	2.000%
8	10.169	1266	1272	1288	rBV	393234	699606	25.05%	3.157%
9	10.545	1329	1336	1348	rVB	397953	688284	24.65%	3.106%
10	13.810	1885	1891	1902	rBV	947058	1291029	46.23%	5.826%
11	14.092	1932	1939	1950	rBV	990610	1492738	53.45%	6.736%
12	14.398	1985	1991	2001	rBV2	671159	1054483	37.76%	4.758%
13	14.627	2025	2030	2052	rVB	45032	97486	3.49%	0.440%
14	15.398	2154	2161	2169	rBV	1342894	1999449	71.60%	9.022%
15	15.527	2177	2183	2194	rBV	342960	503952	18.05%	2.274%
16	17.151	2452	2459	2469	rBV2	944414	1380556	49.44%	6.230%
17	17.251	2469	2476	2489	rBV2	1516213	2276573	81.52%	10.273%
18	19.204	2806	2808	2821	rVB5	13998	30468	1.09%	0.137%
19	19.551	2860	2867	2878	rBV	1912348	2792589	100.00%	12.602%
20	21.345	3166	3172	3178	rBV	1199628	1663579	59.57%	7.507%
21	22.515	3366	3371	3376	rBV	60651	87484	3.13%	0.395%
22	23.468	3525	3533	3541	rVB2	1069275	2040791	73.08%	9.209%
23	23.609	3550	3557	3567	rVB	642384	1233785	44.18%	5.567%
24	24.109	3637	3642	3650	rVB	39662	78007	2.79%	0.352%
25	24.856	3765	3769	3781	rVB	35519	85667	3.07%	0.387%


Sum of corrected areas: 22160711

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005413.D
Acq On : 12 May 2016 10:48
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

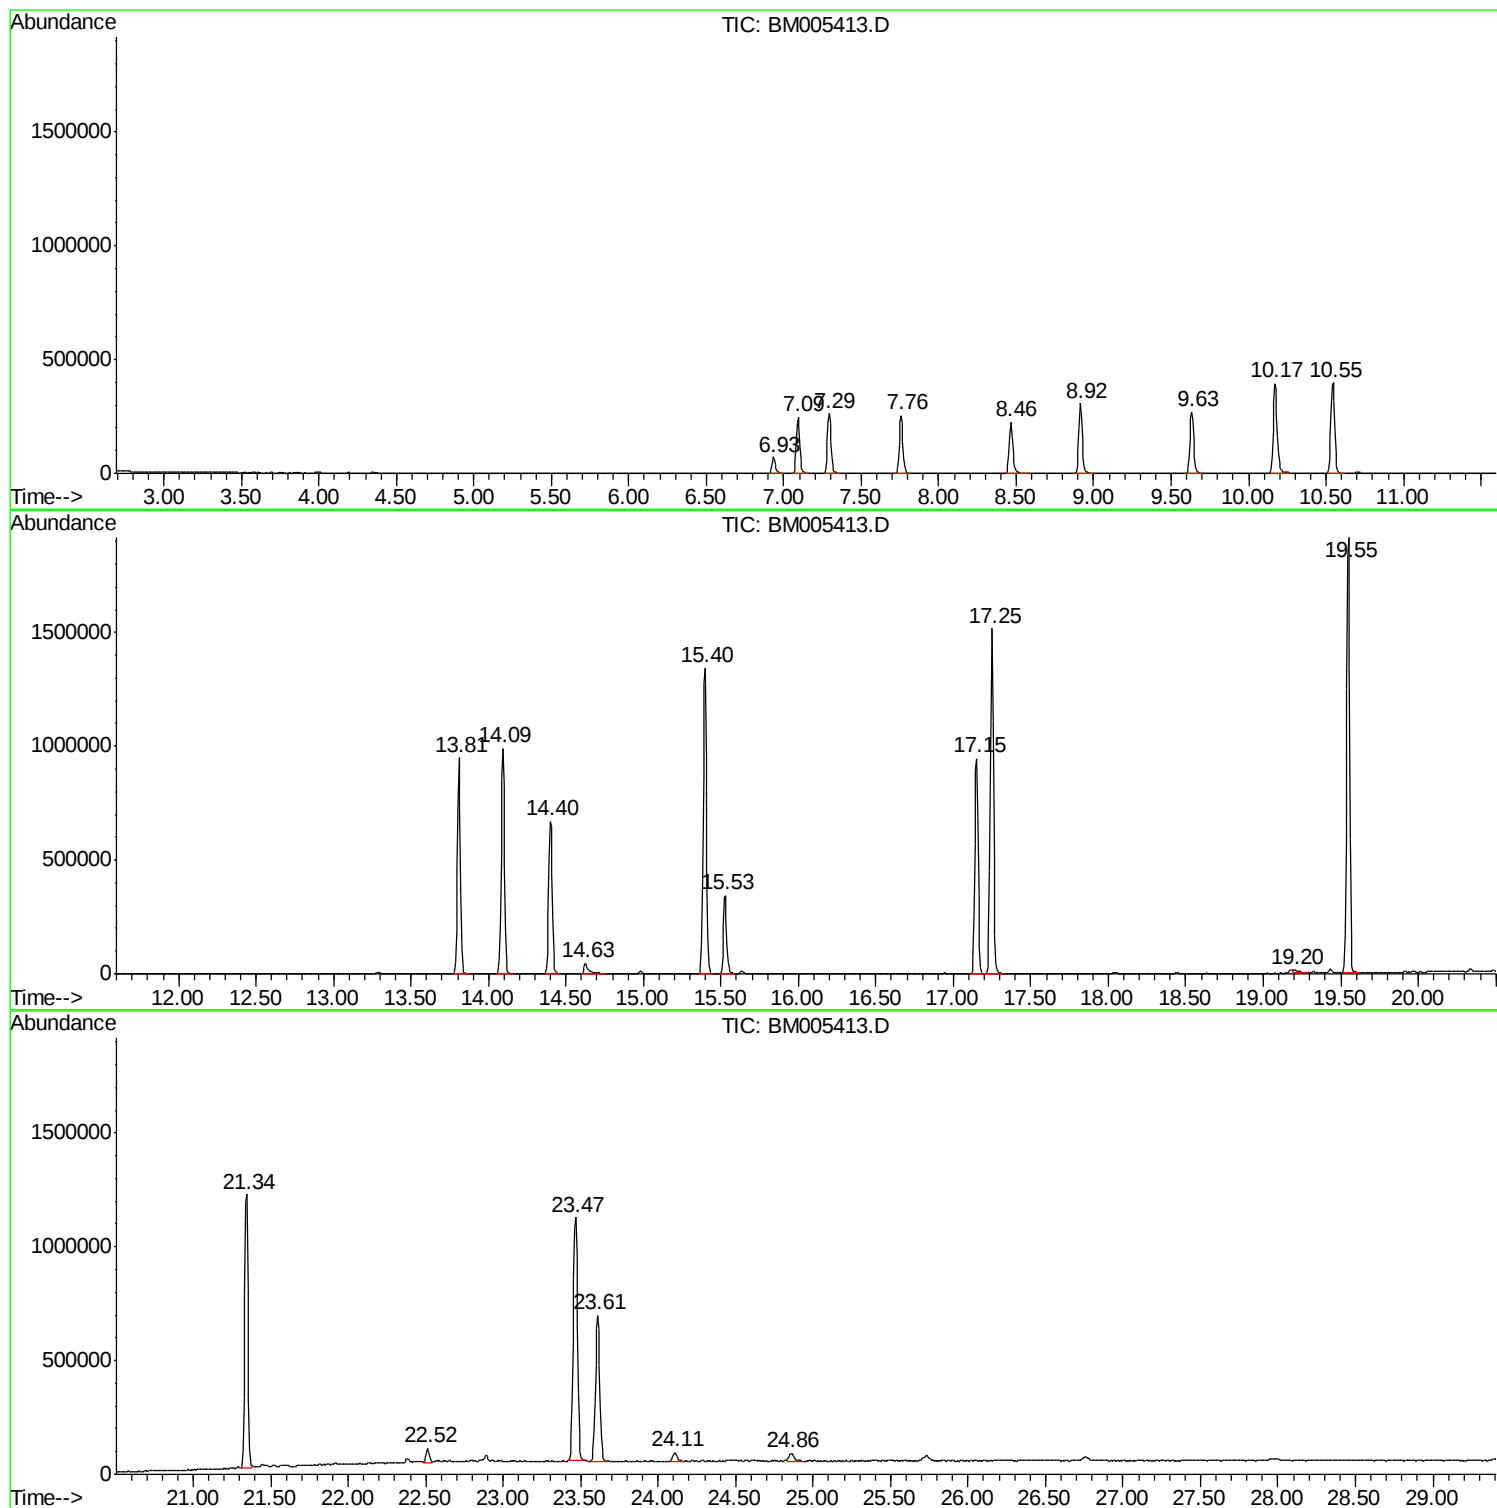

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005413.D
Acq On : 12 May 2016 10:48
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005413.D
Acq On : 12 May 2016 10:48
Operator : UM/SJ
Sample : H2847-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3J6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc