

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
 Data File : BM005422.D
 Acq On : 12 May 2016 16:23
 Operator : UM/SJ
 Sample : H2853-19
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9X11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.092	745	749	759	rVB	20283	36114	2.49%	0.456%
2	7.298	779	784	791	rBV	22567	34855	2.40%	0.440%
3	7.757	855	862	873	rBV	257126	408635	28.18%	5.163%
4	8.475	979	984	994	rVB	17209	30311	2.09%	0.383%
5	8.922	1054	1060	1068	rBV	19289	34464	2.38%	0.435%
6	9.051	1077	1082	1089	rBV3	9699	19862	1.37%	0.251%
7	9.639	1177	1182	1190	rVB	14834	24646	1.70%	0.311%
8	10.186	1270	1275	1282	rBV	21676	40394	2.79%	0.510%
9	10.545	1327	1336	1347	rBV	402325	680656	46.94%	8.600%
10	13.810	1885	1891	1895	rBV	76451	106036	7.31%	1.340%
11	13.857	1895	1899	1906	rVB	51979	77568	5.35%	0.980%
12	14.092	1933	1939	1945	rBV	68828	102678	7.08%	1.297%
13	14.292	1966	1973	1980	rBV	32251	40708	2.81%	0.514%
14	14.404	1980	1992	2002	rVB2	684733	1089604	75.14%	13.767%
15	14.910	2071	2078	2085	rVB2	8007	15573	1.07%	0.197%
16	15.245	2130	2135	2141	rVB	43128	53422	3.68%	0.675%
17	15.398	2155	2161	2171	rVB	111046	164729	11.36%	2.081%
18	15.651	2192	2204	2208	rBV2	12208	27140	1.87%	0.343%
19	16.109	2277	2282	2294	rBV	71125	113880	7.85%	1.439%
20	16.451	2335	2340	2344	rBV3	8273	14957	1.03%	0.189%
21	16.898	2411	2416	2420	rBV	43823	53460	3.69%	0.675%
22	16.951	2420	2425	2430	rVB2	11430	18986	1.31%	0.240%
23	17.151	2452	2459	2466	rBV	992927	1402427	96.72%	17.719%
24	17.245	2470	2475	2485	rVB2	115920	181361	12.51%	2.291%
25	17.639	2537	2542	2547	rBV	25275	30467	2.10%	0.385%
26	18.039	2605	2610	2615	rBV	30296	44316	3.06%	0.560%
27	19.545	2861	2866	2874	rBV	142690	200469	13.83%	2.533%
28	21.044	3117	3121	3129	rBV	42427	69254	4.78%	0.875%
29	21.344	3167	3172	3179	rBV	1122079	1450045	100.00%	18.321%
30	22.386	3346	3349	3353	rBV2	22240	28198	1.94%	0.356%
31	22.897	3433	3436	3441	rVB	18515	25250	1.74%	0.319%
32	23.468	3527	3533	3539	rBV3	86644	157366	10.85%	1.988%
33	23.615	3551	3558	3571	rVB	582020	1107575	76.38%	13.994%
34	24.121	3640	3644	3648	rVB2	18134	29193	2.01%	0.369%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005422.D
Acq On : 12 May 2016 16:23
Operator : UM/SJ
Sample : H2853-19
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X11

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Title : SVOA CALIBRATION


Sum of corrected areas: 7914599

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005422.D
Acq On : 12 May 2016 16:23
Operator : UM/SJ
Sample : H2853-19
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

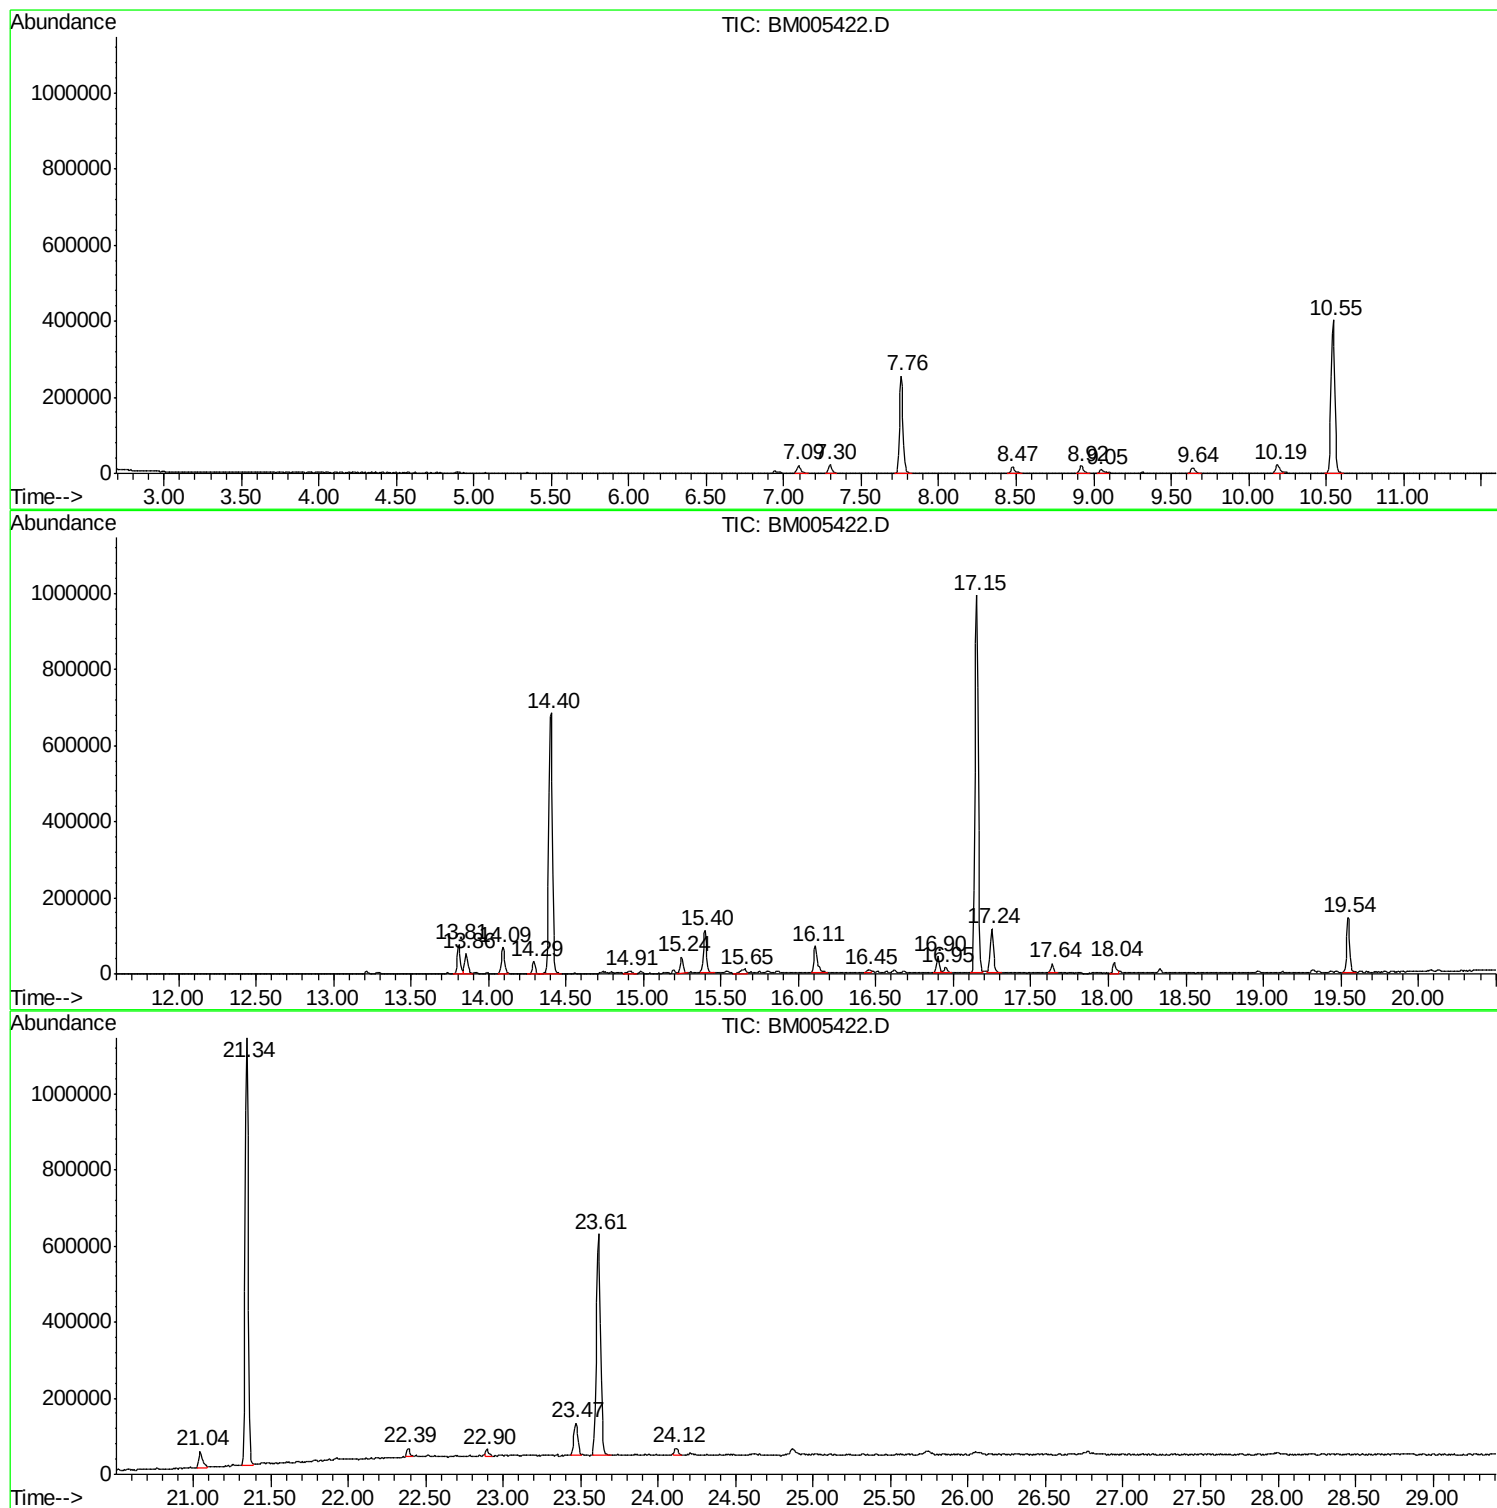

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005422.D
Acq On : 12 May 2016 16:23
Operator : UM/SJ
Sample : H2853-19
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051216\
Data File : BM005422.D
Acq On : 12 May 2016 16:23
Operator : UM/SJ
Sample : H2853-19
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X11

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc