

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051217\
 Data File : BM010032.D
 Acq On : 12 May 2017 20:17
 Operator : SJ/MA
 Sample : I3100-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PMW-1A-051017

Quant Time: May 13 04:27:06 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 19:50:16 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	56311	20.00	ng	-0.02
21) Naphthalene-d8	10.55	136	244593	20.00	ng	-0.03
38) Acenaphthene-d10	14.41	164	147829	20.00	ng	-0.03
63) Phenanthrene-d10	17.17	188	367634	20.00	ng	-0.03
75) Chrysene-d12	21.36	240	432267	20.00	ng	-0.03
86) Perylene-d12	23.65	264	333062	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	243073	67.55	ng	-0.02
7) Phenol-d6	6.94	99	218844	37.96	ng	-0.03
23) Nitrobenzene-d5	8.93	82	720599	107.67	ng	-0.02
41) 2,4,6-Tribromophenol	15.92	330	337984	167.06	ng	-0.02
44) 2-Fluorobiphenyl	13.03	172	1228637	111.15	ng	-0.02
78) Terphenyl-d14	19.79	244	2463177	120.09	ng	-0.02
Target Compounds						
49) Dimethylphthalate	13.88	163	34873	2.68	ng	Qvalue # 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051217\
Data File : BM010032.D
Acq On : 12 May 2017 20:17
Operator : SJ/MA
Sample : I3100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PMW-1A-051017

Quant Time: May 13 04:27:06 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

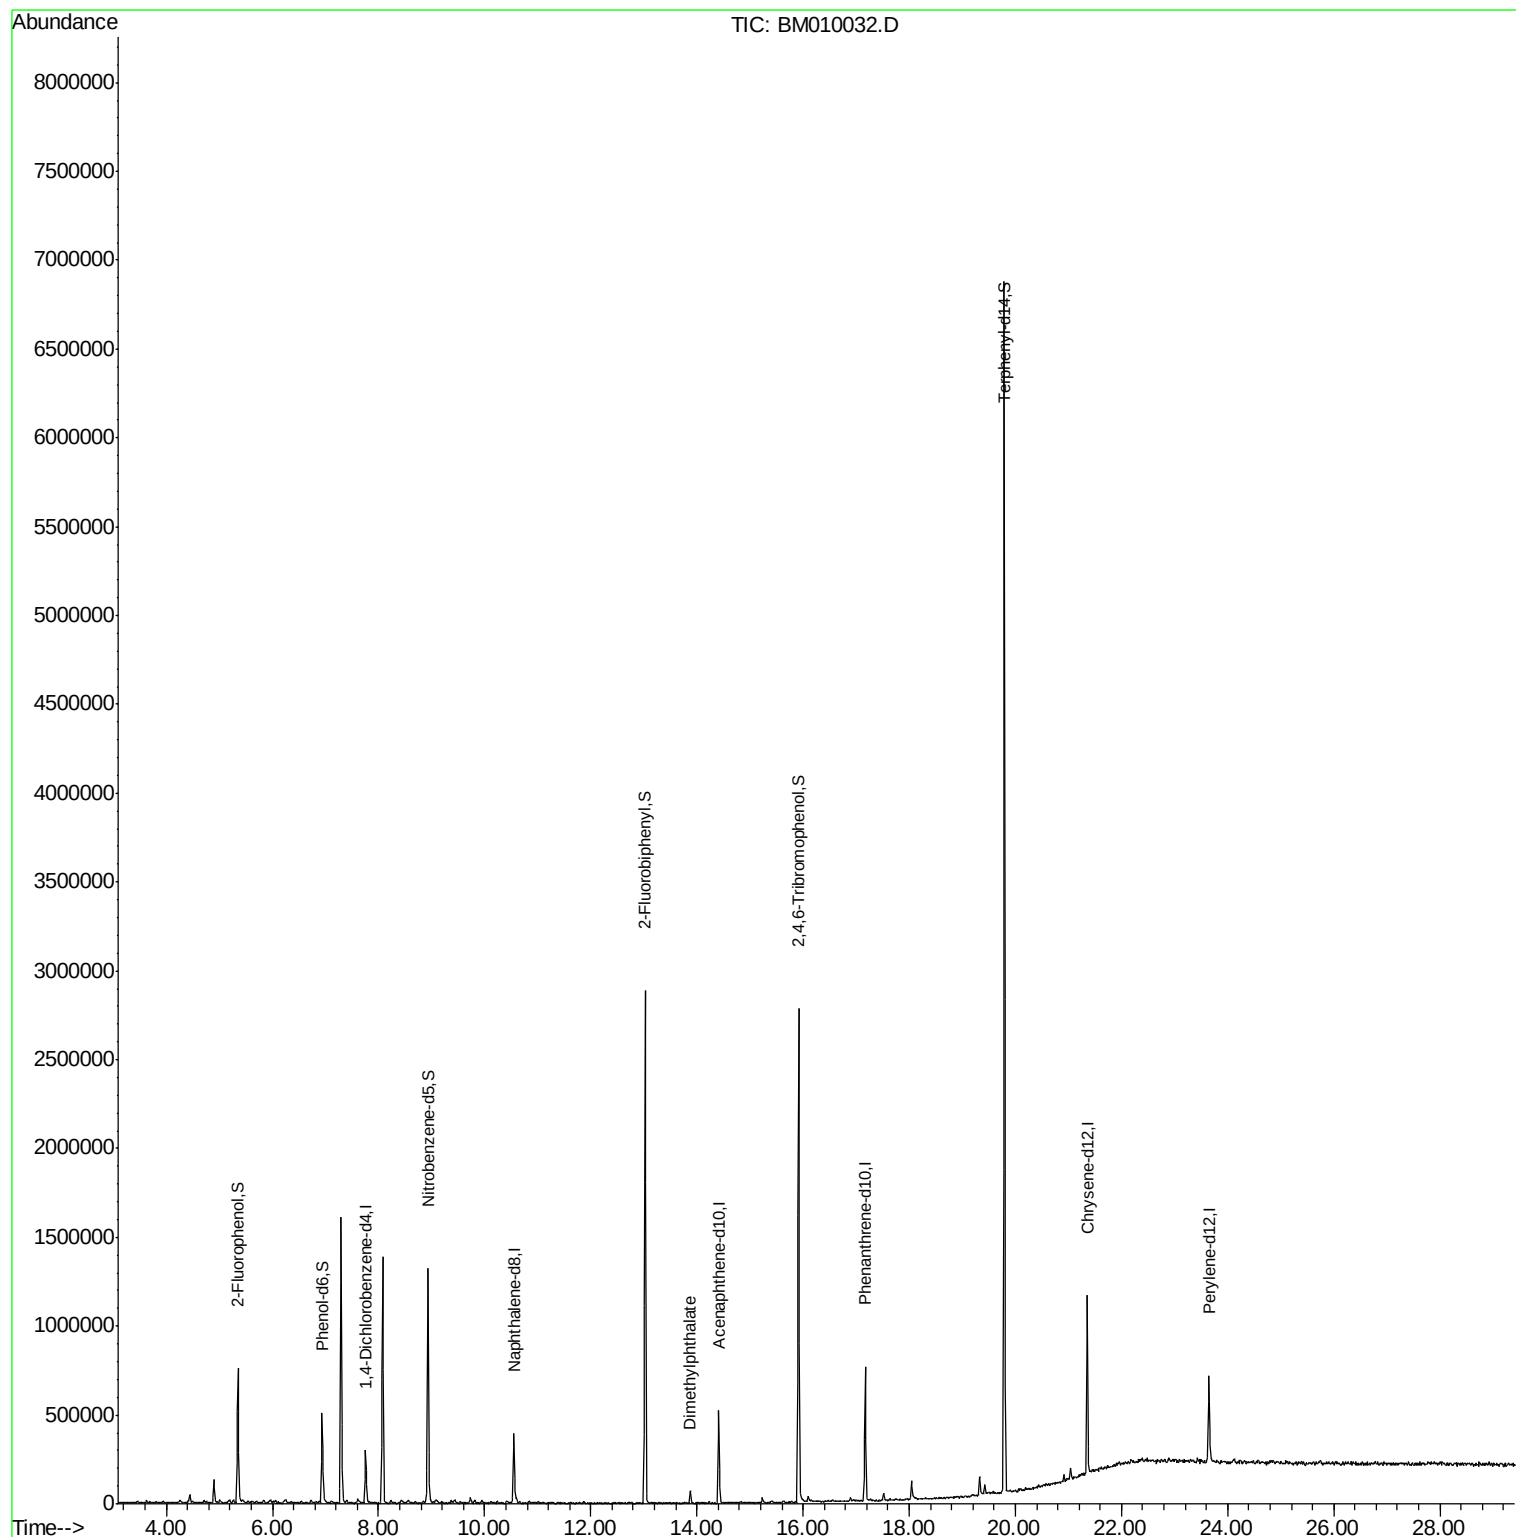

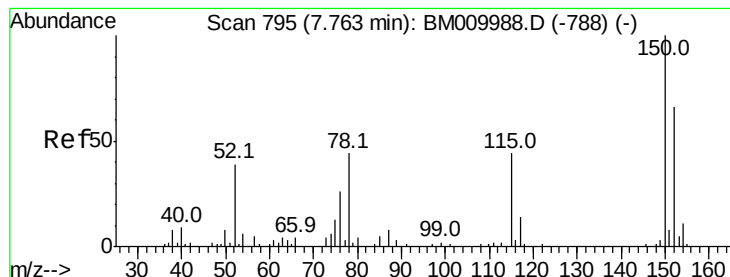

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.76 min Scan# 794

Delta R.T. -0.02 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17

Instrument :

BNA_M

ClientSampleId :

PMW-1A-051017


Tot Ion:152 Resp: 56311

Ion Ratio Lower Upper

152 100

150 149.4 119.5 179.3




115 70.2 43.0 64.4#

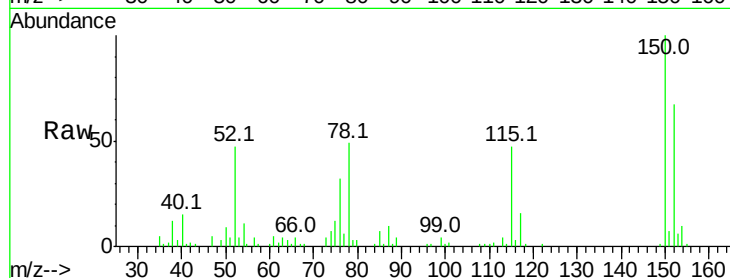

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

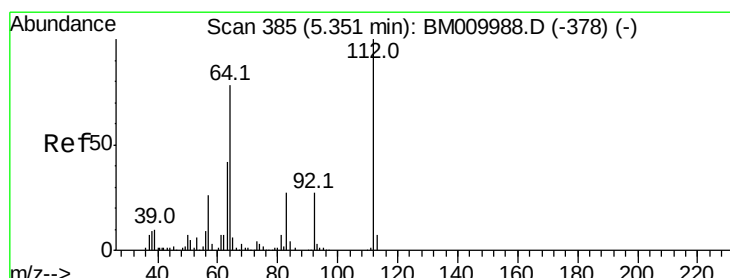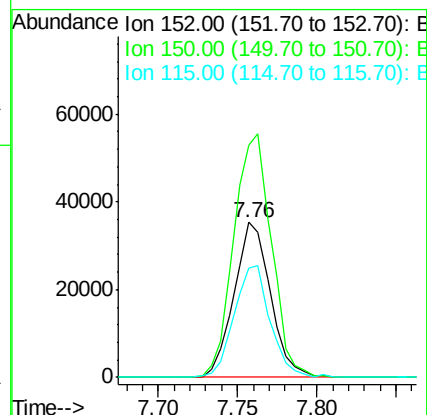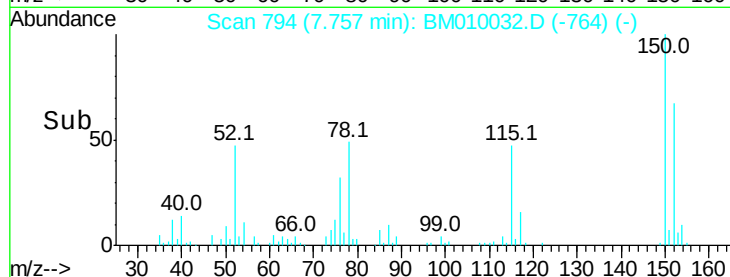

#5

2-Fluorophenol

Concen: 67.55 ng

RT: 5.35 min Scan# 385

Delta R.T. -0.02 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17


Tgt Ion:112 Resp: 243073

Ion Ratio Lower Upper

112 100

64 78.8 38.6 57.8#



63 50.9 19.3 28.9#

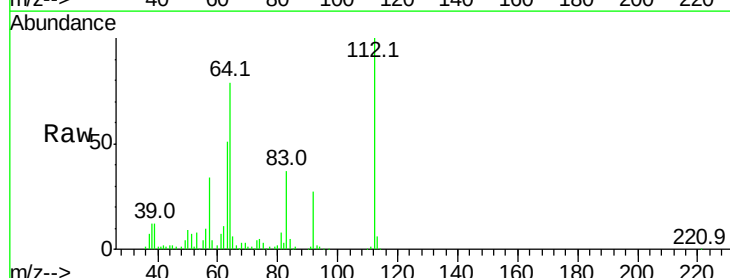


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

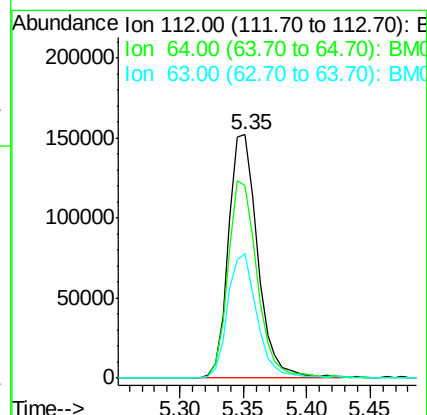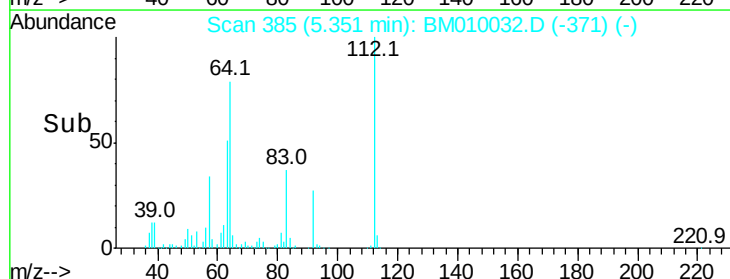

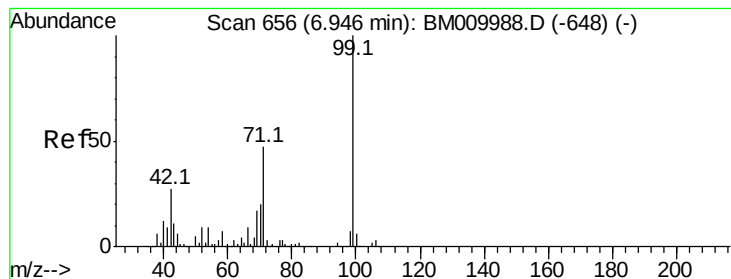

#7

Phenol-d6

Concen: 37.96 ng

RT: 6.94 min Scan# 655

Delta R.T. -0.03 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17

Instrument :

BNA_M

ClientSampleId :

PMW-1A-051017


Tot Ion: 99 Resp: 218844

Ion Ratio Lower Upper

99 100

42 33.5 11.0 16.4#




71 51.5 23.4 35.2#

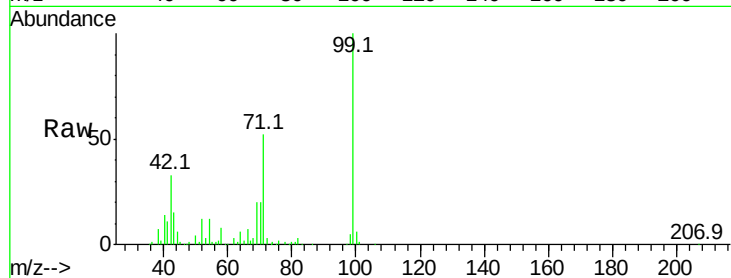

Abundance Ion 99.00 (98.70 to 99.70): BM010032.D (-648) (-)

Ion 42.00 (41.70 to 42.70): BM010032.D (-648) (-)

Ion 71.00 (70.70 to 71.70): BM010032.D (-648) (-)

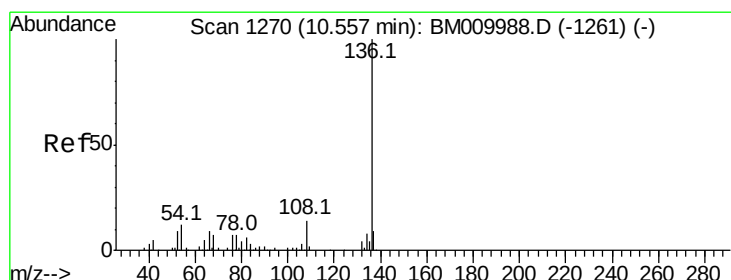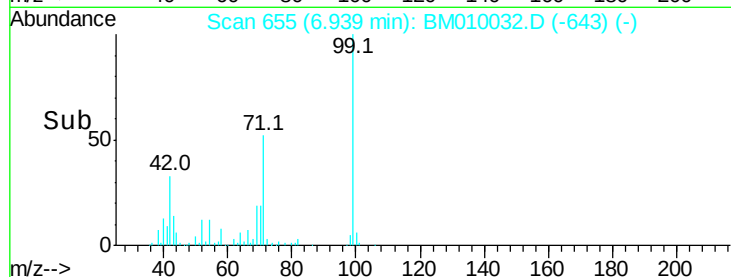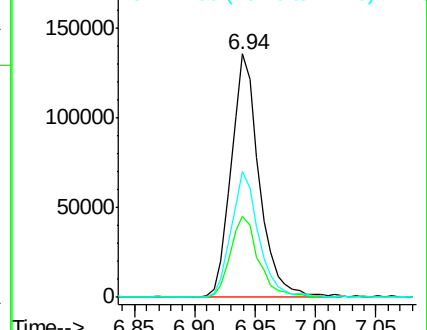

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.55 min Scan# 1269

Delta R.T. -0.03 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17

Tgt Ion: 136 Resp: 244593


Ion Ratio Lower Upper

136 100

137 12.1 8.7 13.1

54 13.0 4.6 6.8#

68 9.4 3.7 5.5#


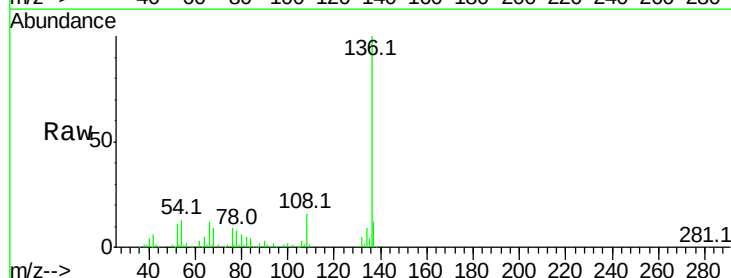



Abundance Ion 136.00 (135.70 to 136.70): BM010032.D (-1257) (-)

Ion 137.00 (136.70 to 137.70): BM010032.D (-1257) (-)

Ion 54.00 (53.70 to 54.70): BM010032.D (-1257) (-)

Ion 68.00 (67.70 to 68.70): BM010032.D (-1257) (-)



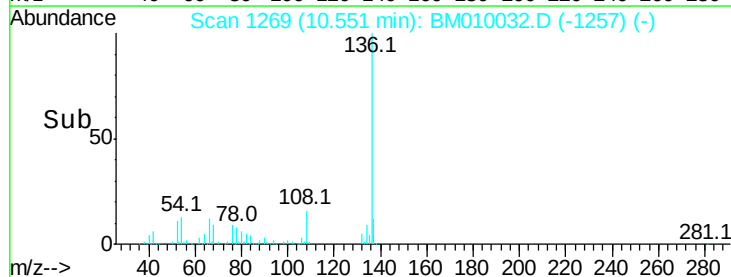
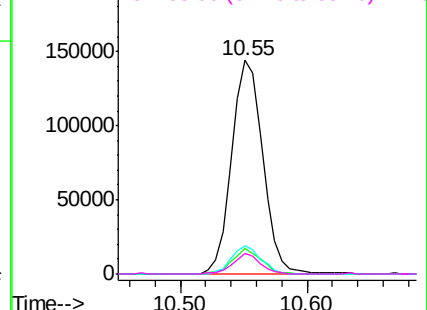


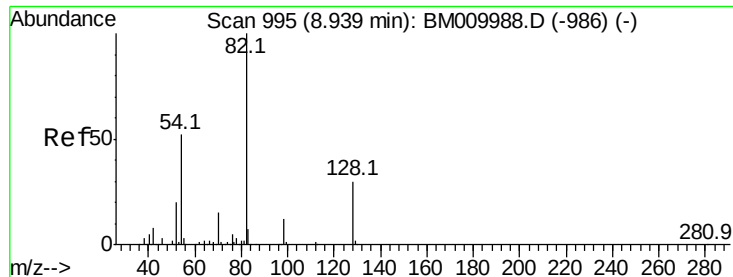

#23
 Nitrobenzene-d5
 Concen: 107.67 ng
 RT: 8.93 min Scan# 994
 Delta R.T. -0.02 min
 Lab File: BM010032.D
 Acq: 12 May 2017 20:17




Instrument :
 BNA_M
 ClientSampleId :
 PMW-1A-051017


Tot Ion	82	Resp	720599
Ion	Ratio	Lower	Upper
82	100		
128	26.7	32.8	49.2#
54	58.5	40.6	60.8

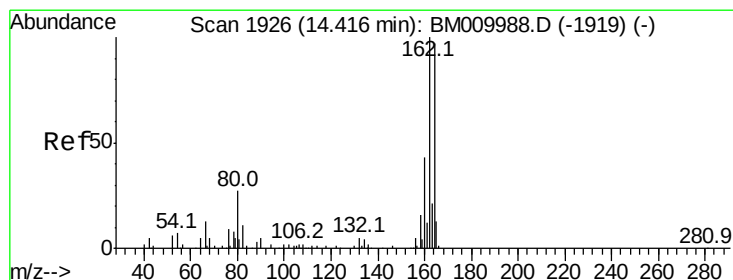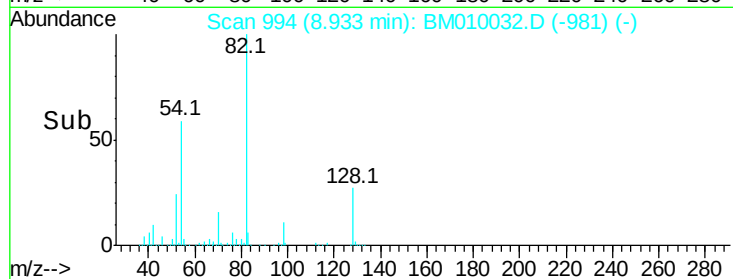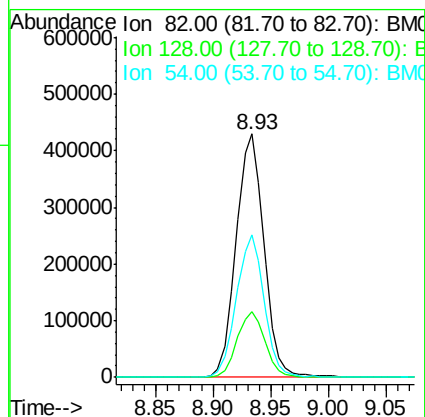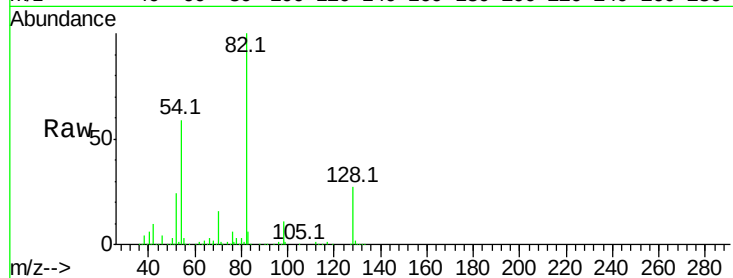

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.41 min Scan# 1925
 Delta R.T. -0.03 min
 Lab File: BM010032.D
 Acq: 12 May 2017 20:17

Tgt Ion	164	Resp	147829
Ion	Ratio	Lower	Upper
164	100		
162	99.8	82.4	123.6
160	43.6	35.8	53.6

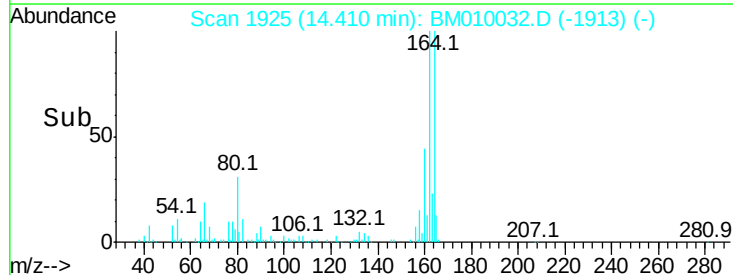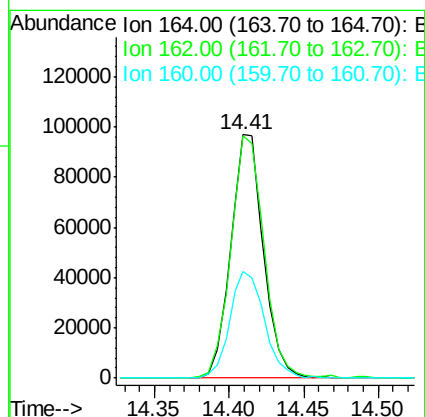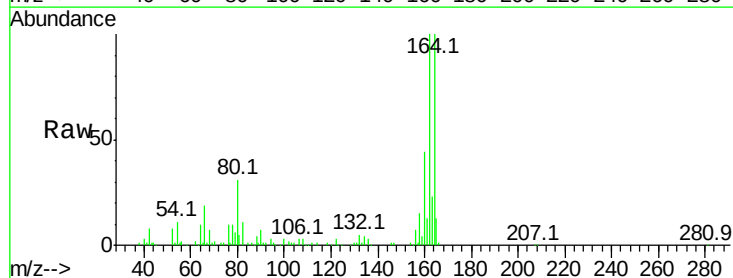


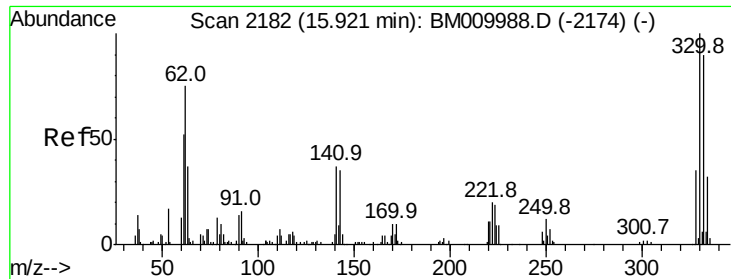




#41
 2,4,6-Tribromophenol
 Concen: 167.06 ng
 RT: 15.92 min Scan# 2181
 Delta R.T. -0.02 min
 Lab File: BM010032.D
 Acq: 12 May 2017 20:17

Instrument :
 BNA_M
 ClientSampleId :
 PMW-1A-051017

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.9	0.0	0.0#
141	51.6	0.0	0.0#

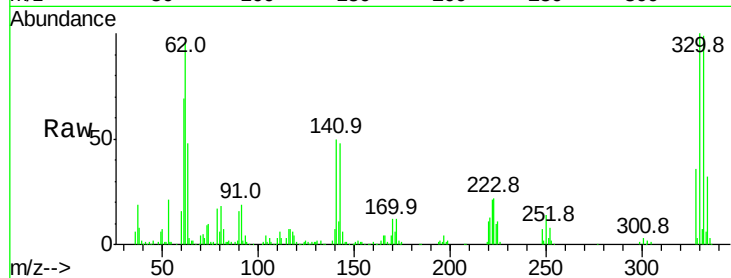


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

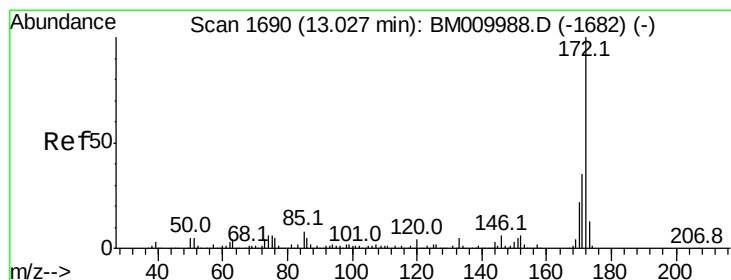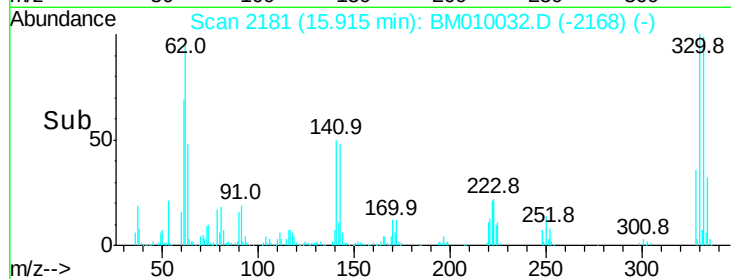
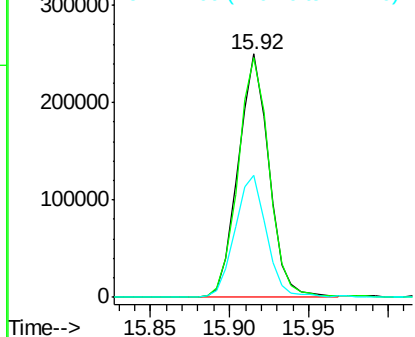



#44
 2-Fluorobiphenyl
 Concen: 111.15 ng
 RT: 13.03 min Scan# 1690
 Delta R.T. -0.02 min
 Lab File: BM010032.D
 Acq: 12 May 2017 20:17

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.9	28.5	42.7
170	23.7	18.8	28.2

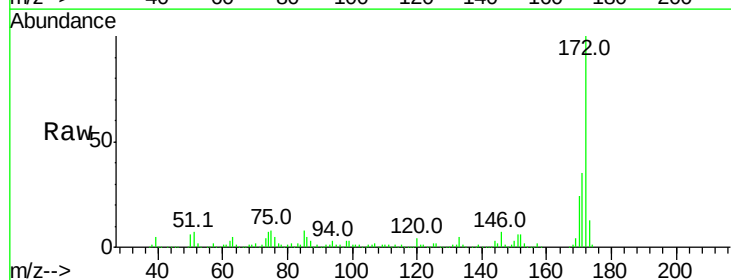

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

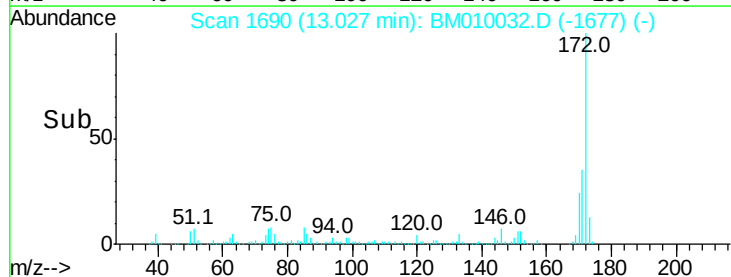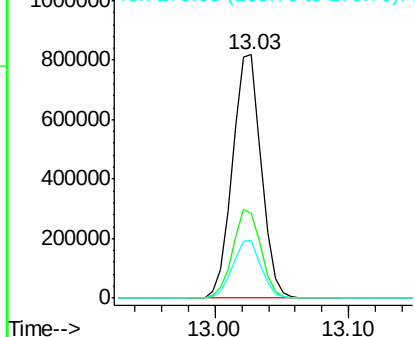

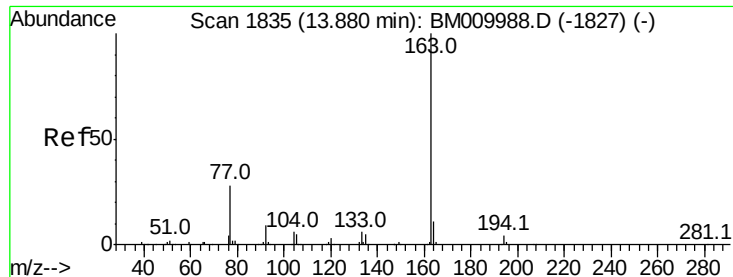

#49

Dimethylphthalate

Concen: 2.68 ng

RT: 13.88 min Scan# 1835

Delta R.T. -0.02 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17

Instrument :

BNA_M

ClientSampleId :

PMW-1A-051017


Tot Ion:163 Resp: 34873

Ion Ratio Lower Upper

163 100

194 5.5 2.7 4.1#




164 7.5 8.2 12.2#

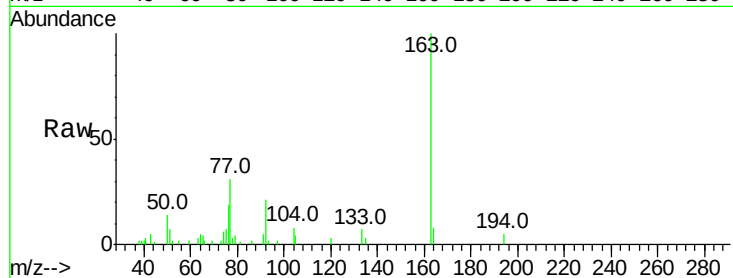

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

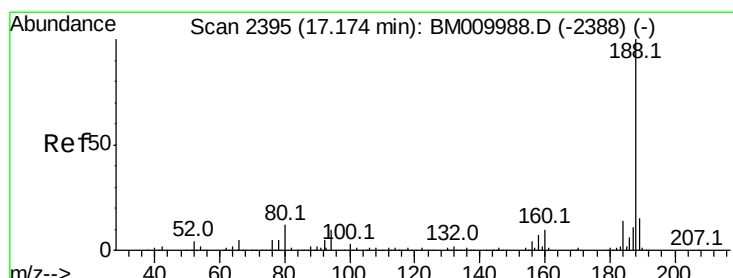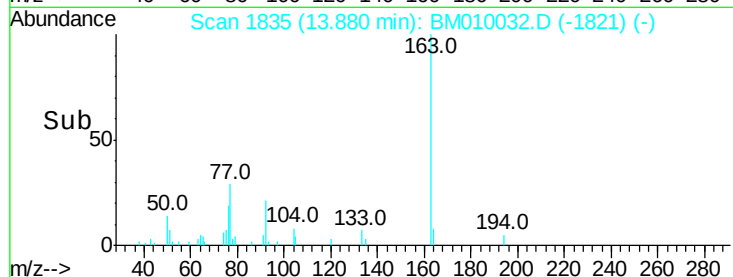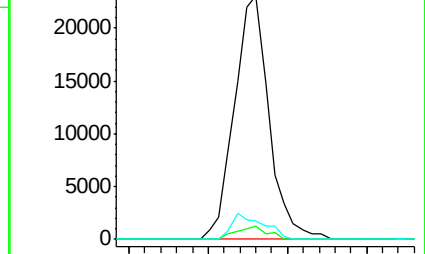

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.17 min Scan# 2394

Delta R.T. -0.03 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17


Tgt Ion:188 Resp: 367634

Ion Ratio Lower Upper

188 100

94 9.3 8.7 13.1



80 12.1 9.3 13.9

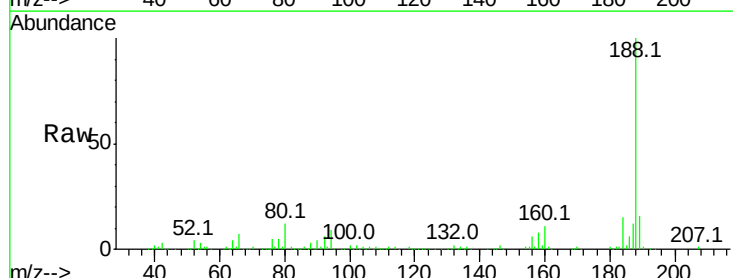


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

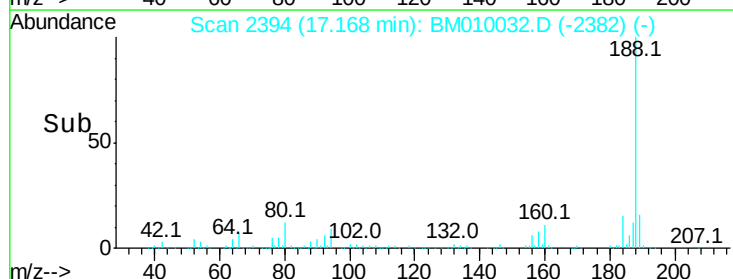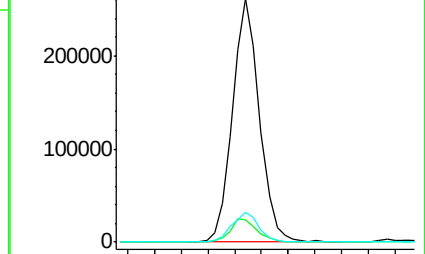

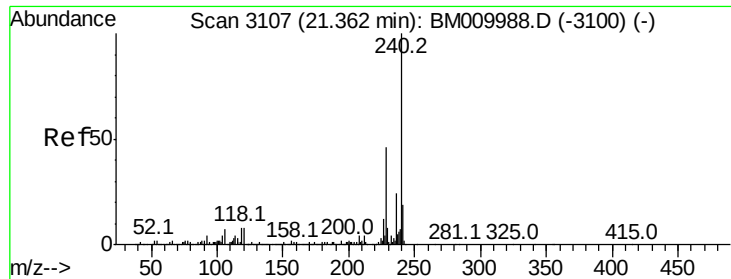

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.36 min Scan# 3106

Delta R.T. -0.03 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17

Instrument :

BNA_M

ClientSampleId :

PMW-1A-051017


Tot Ion:240 Resp: 432267

Ion Ratio Lower Upper

240 100

120 9.5 8.2 12.2




236 24.9 20.0 30.0

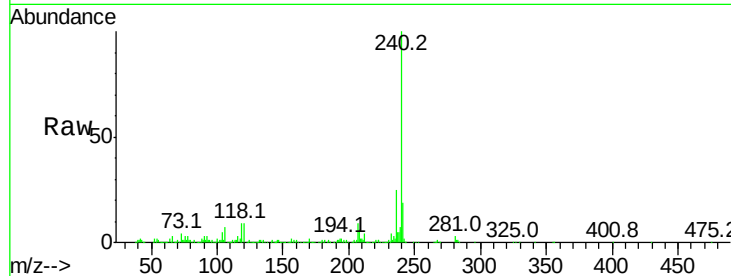

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

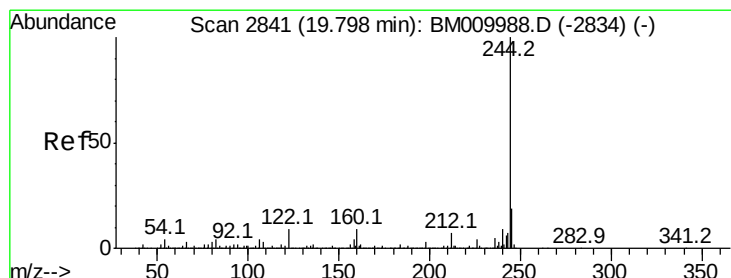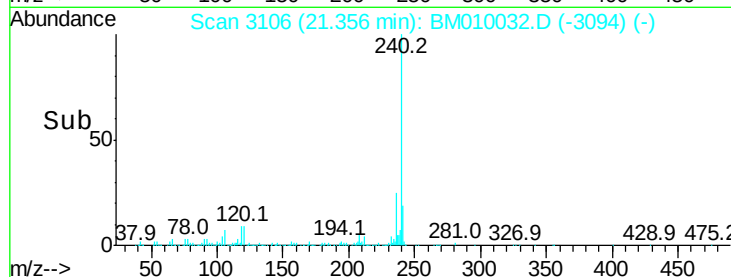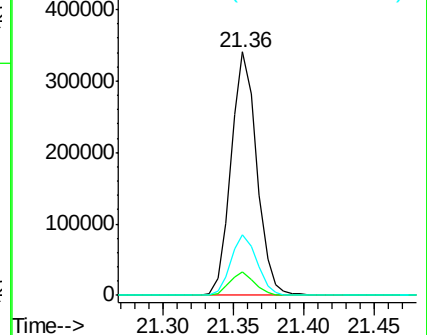

#78

Terphenyl-d14

Concen: 120.09 ng

RT: 19.79 min Scan# 2840

Delta R.T. -0.02 min

Lab File: BM010032.D

Acq: 12 May 2017 20:17


Tgt Ion:244 Resp: 2463177

Ion Ratio Lower Upper

244 100

212 8.1 4.9 7.3#



122 9.2 6.2 9.4

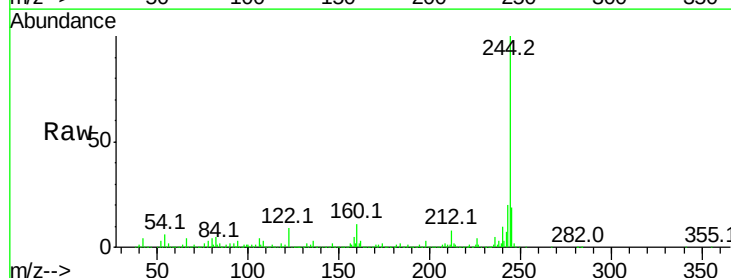


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

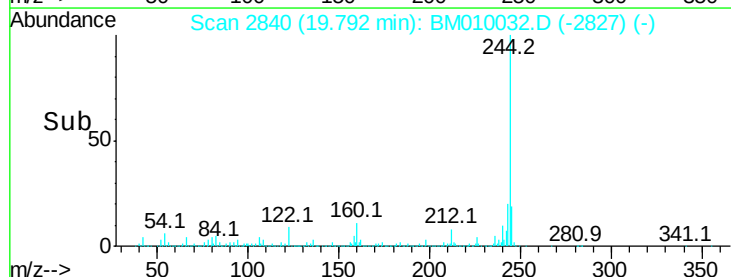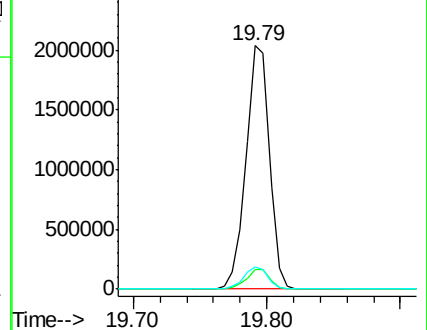


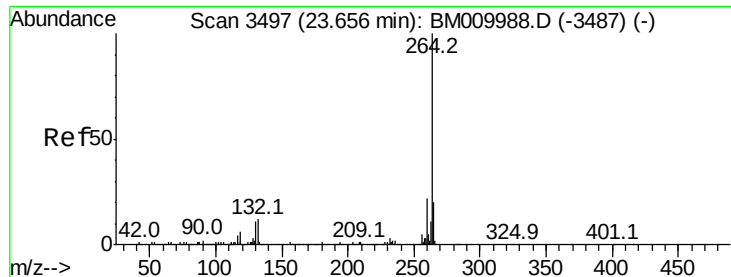

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.65 min Scan# 3496
Delta R.T. -0.04 min
Lab File: BM010032.D
Acq: 12 May 2017 20:17

Instrument :
BNA_M
ClientSampleId :
PMW-1A-051017

Tot Ion	Ratio	Lower	Upper
264	100		
260	21.7	18.6	27.8
265	22.0	17.3	25.9

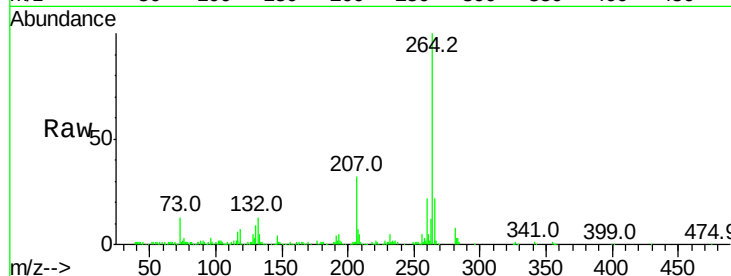

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

