


Data Path : Z:\HPCHEM1\BNA M\DATA\BM051217\
 Data File : BM010020.D
 Acq On : 12 May 2017 13:03
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

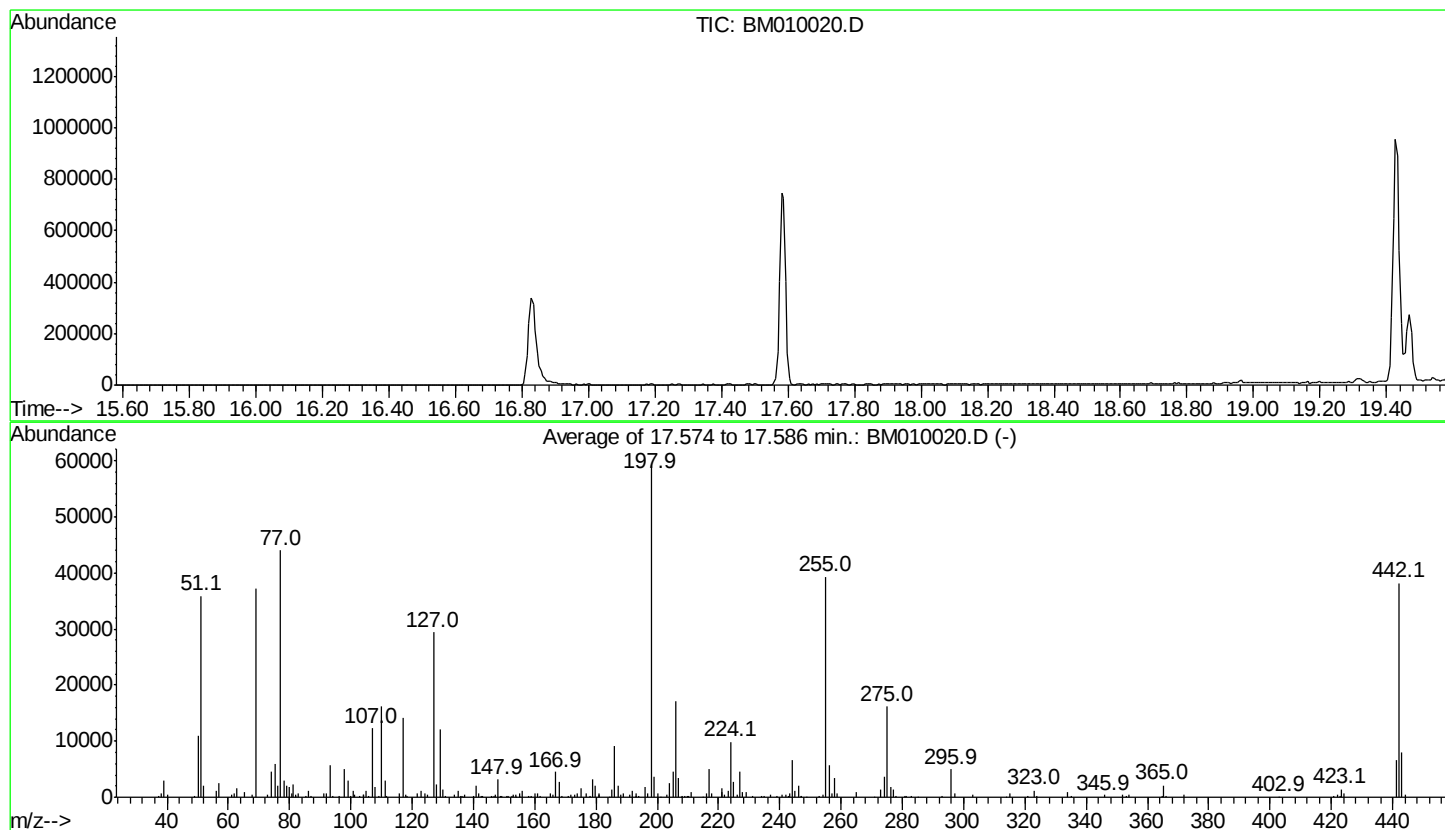

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	35941	PASS
68	69	0.00	2	1.4	536	PASS
69	198	0.00	100	63.0	37234	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	29432	PASS
197	198	0.00	2	1.2	681	PASS
198	198	100	100	100.0	59128	PASS
199	198	5	9	6.3	3732	PASS
275	198	10	60	27.3	16169	PASS
365	198	1	100	3.5	2085	PASS
441	442	0.01	24	17.2	6566	PASS
442	198	50	100	64.5	38120	PASS
443	442	15	24	20.8	7915	PASS