
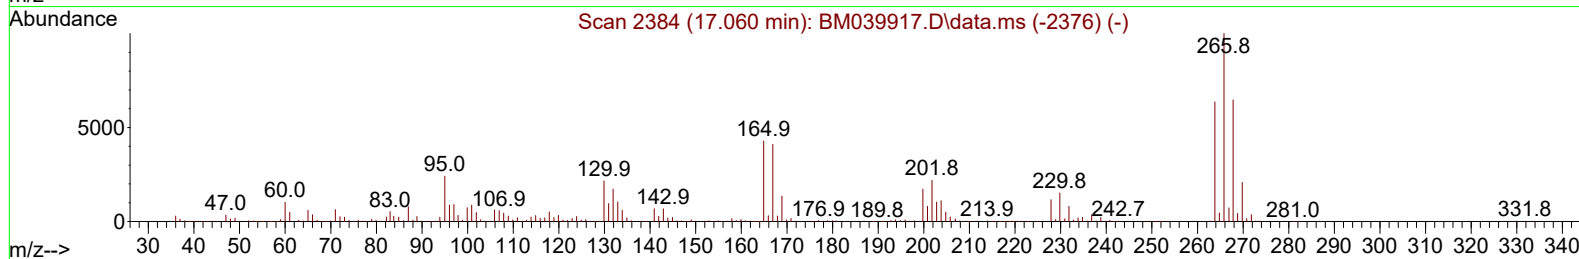
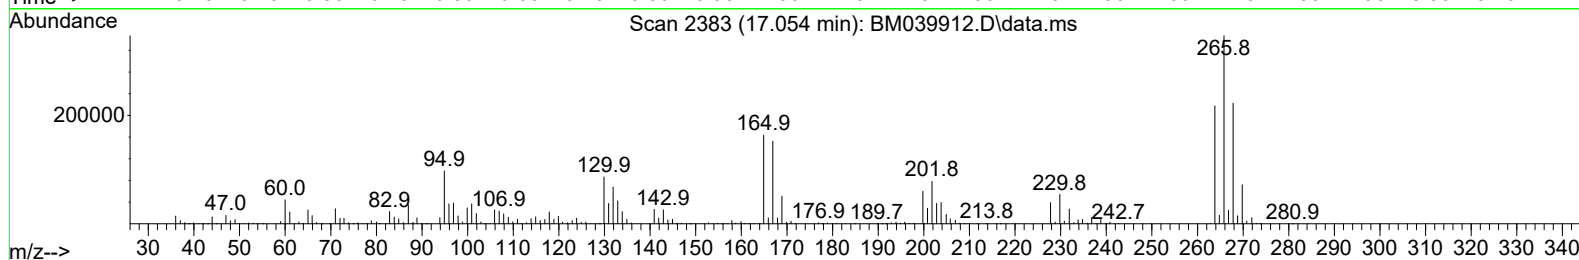


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051223\
Data File : BM039912.D
Acq On : 12 May 2023 10:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:18:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 13 02:16:09 2023
Response via : Initial Calibration

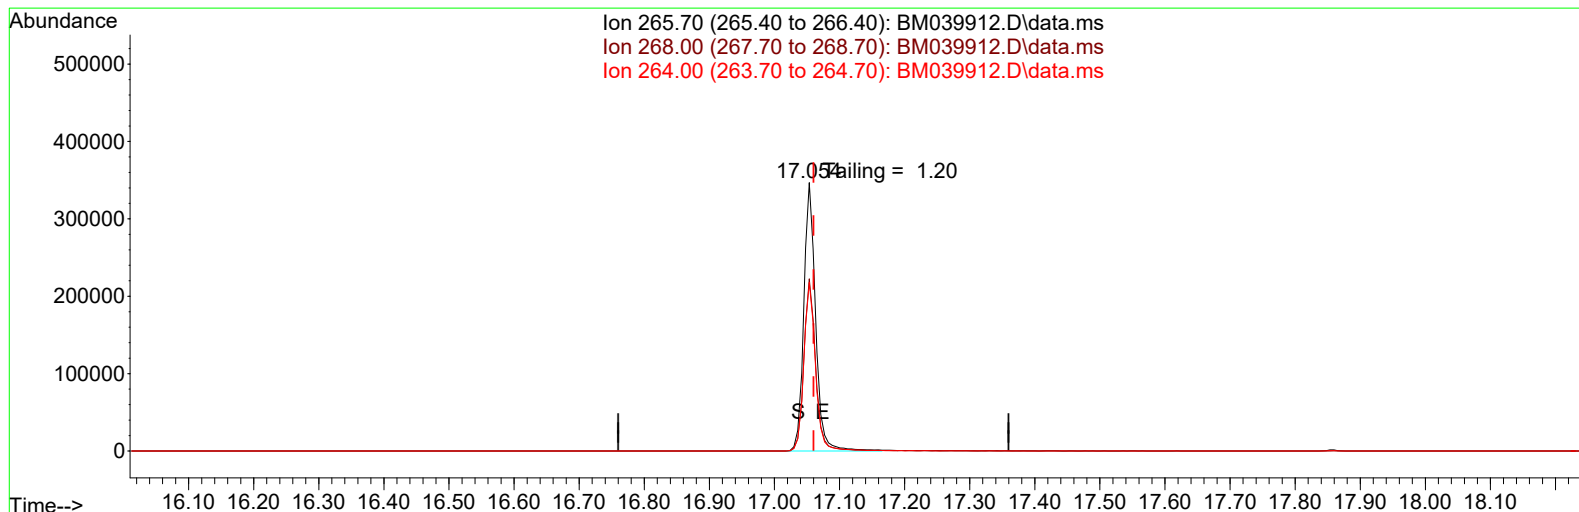

TIC: BM039912.D\data.ms

(70) Pentachlorophenol (C)




17.054min (-0.006) 0.00 ng

response 443911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.14
264.00	63.70	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051223\
Data File : BM039912.D
Acq On : 12 May 2023 10:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:18:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 13 02:16:09 2023
Response via : Initial Calibration

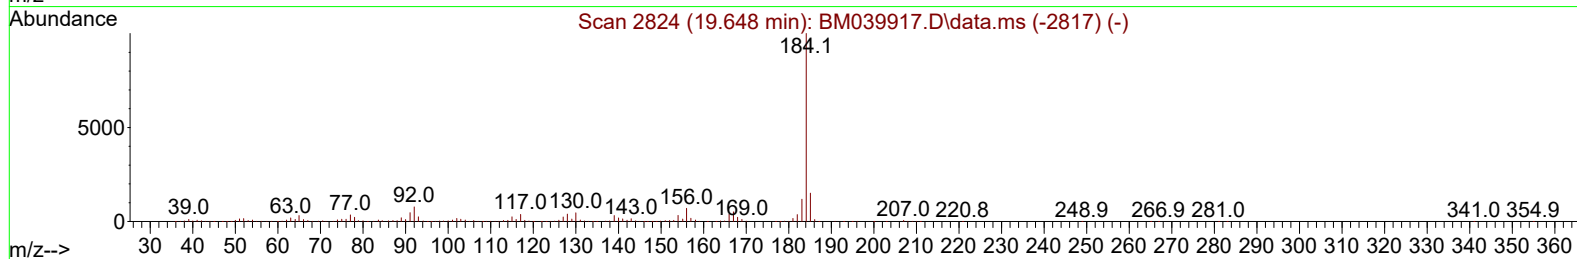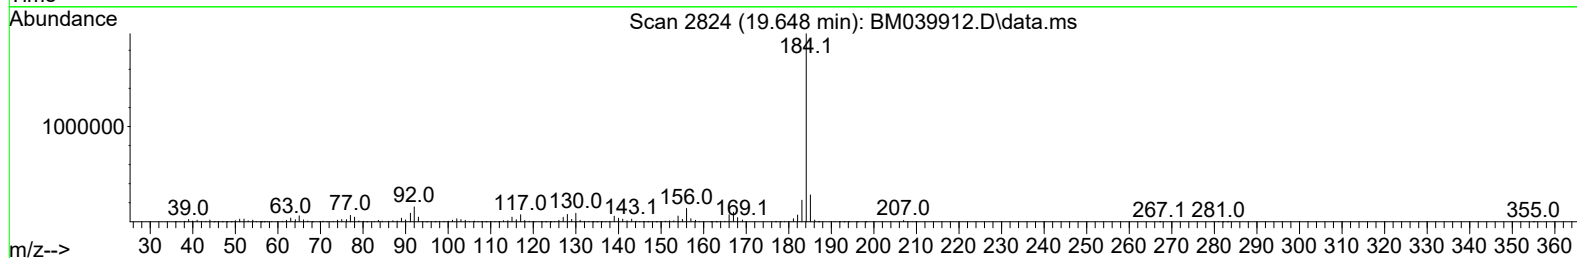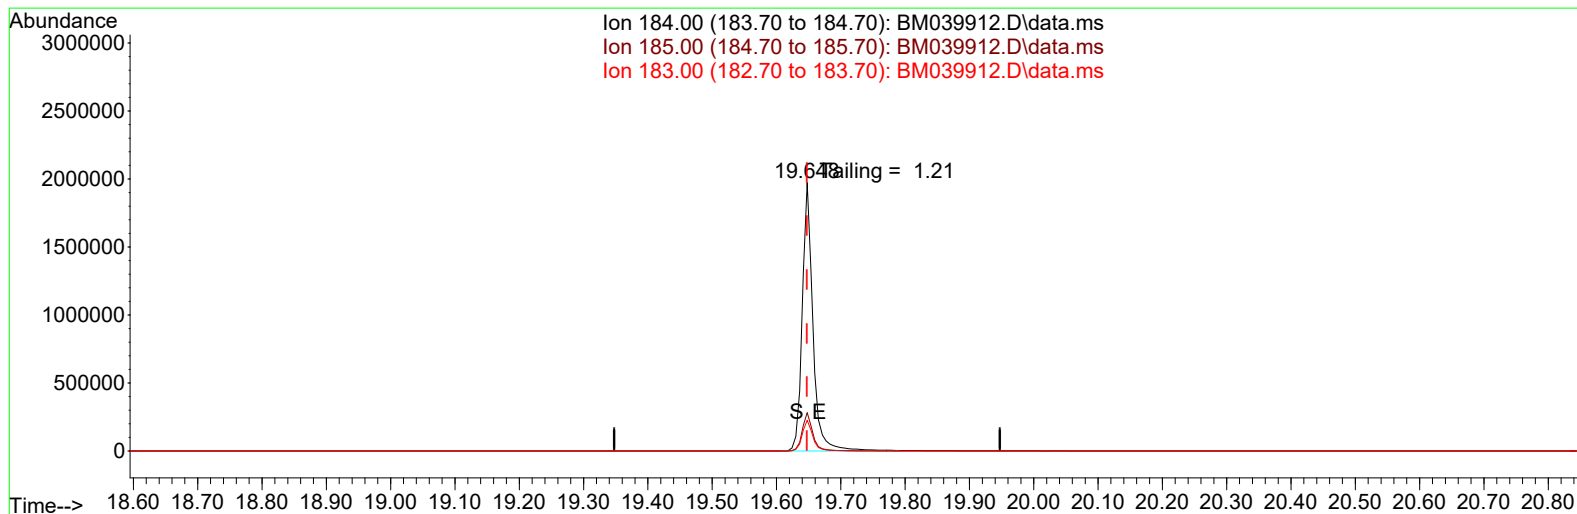

TIC: BM039912.D\data.ms

(77) Benzidine**19.648min (-0.000) 1072219.19 ng****response 2307146**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.29
183.00	11.90	11.48
0.00	0.00	0.00