

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051315\
 Data File : BM001270.D
 Acq On : 13 May 2015 02:41
 Operator : TP/IZ
 Sample : G2183-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-1(7-8)

Quant Time: May 13 05:50:01 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM051315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 13 05:24:15 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	13780	5.00	ng	0.00
6) Naphthalene-d8	10.22	136	48105	5.00	ng	0.00
12) Acenaphthene-d10	14.12	164	24745	5.00	ng	0.00
18) Phenanthrene-d10	16.85	188	58970	5.00	ng	0.00
24) Chrysene-d12	21.08	240	43738	5.00	ng	0.00
30) Perylene-d12	23.18	264	40771	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.04	112	17399	6.48	ng	0.00
5) Phenol-d6	6.63	99	22775	7.52	ng	0.00
7) Nitrobenzene-d5	8.60	82	12316	4.08	ng	0.00
13) 2,4,6-Tribromophenol	15.63	330	5720	6.76	ng	0.00
14) 2-Fluorobiphenyl	12.73	172	40951	5.33	ng	0.00
26) Terphenyl-d14	19.51	244	32856	5.59	ng	-0.01
Target Compounds						Qvalue
3) n-Nitrosodimethylamine	3.18	42	67	0.04	ng	# 1
8) Nitrobenzene	8.60	77	44	0.14	ng	# 18
17) Fluorene	14.74	166	301	0.05	ng	# 1
20) Pentachlorophenol	16.55	266	15	0.43	ng	# 73
21) Phenanthrene	16.88	178	387	0.04	ng	# 99
22) Anthracene	16.88	178	389	0.04	ng	# 100
23) Fluoranthene	18.93	202	514	0.04	ng	# 97
25) Pyrene	19.30	202	452	0.03	ng	# 97
27) Benzo(a)anthracene	21.07	228	365	0.03	ng	# 70
31) Benzo(b)fluoranthene	22.56	252	408	0.03	ng	# 1
32) Benzo(k)fluoranthene	22.56	252	408	0.04	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051315\
Data File : BM001270.D
Acq On : 13 May 2015 02:41
Operator : TP/IZ
Sample : G2183-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-1(7-8)

Quant Time: May 13 05:50:01 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 05:24:15 2015
Response via : Initial Calibration

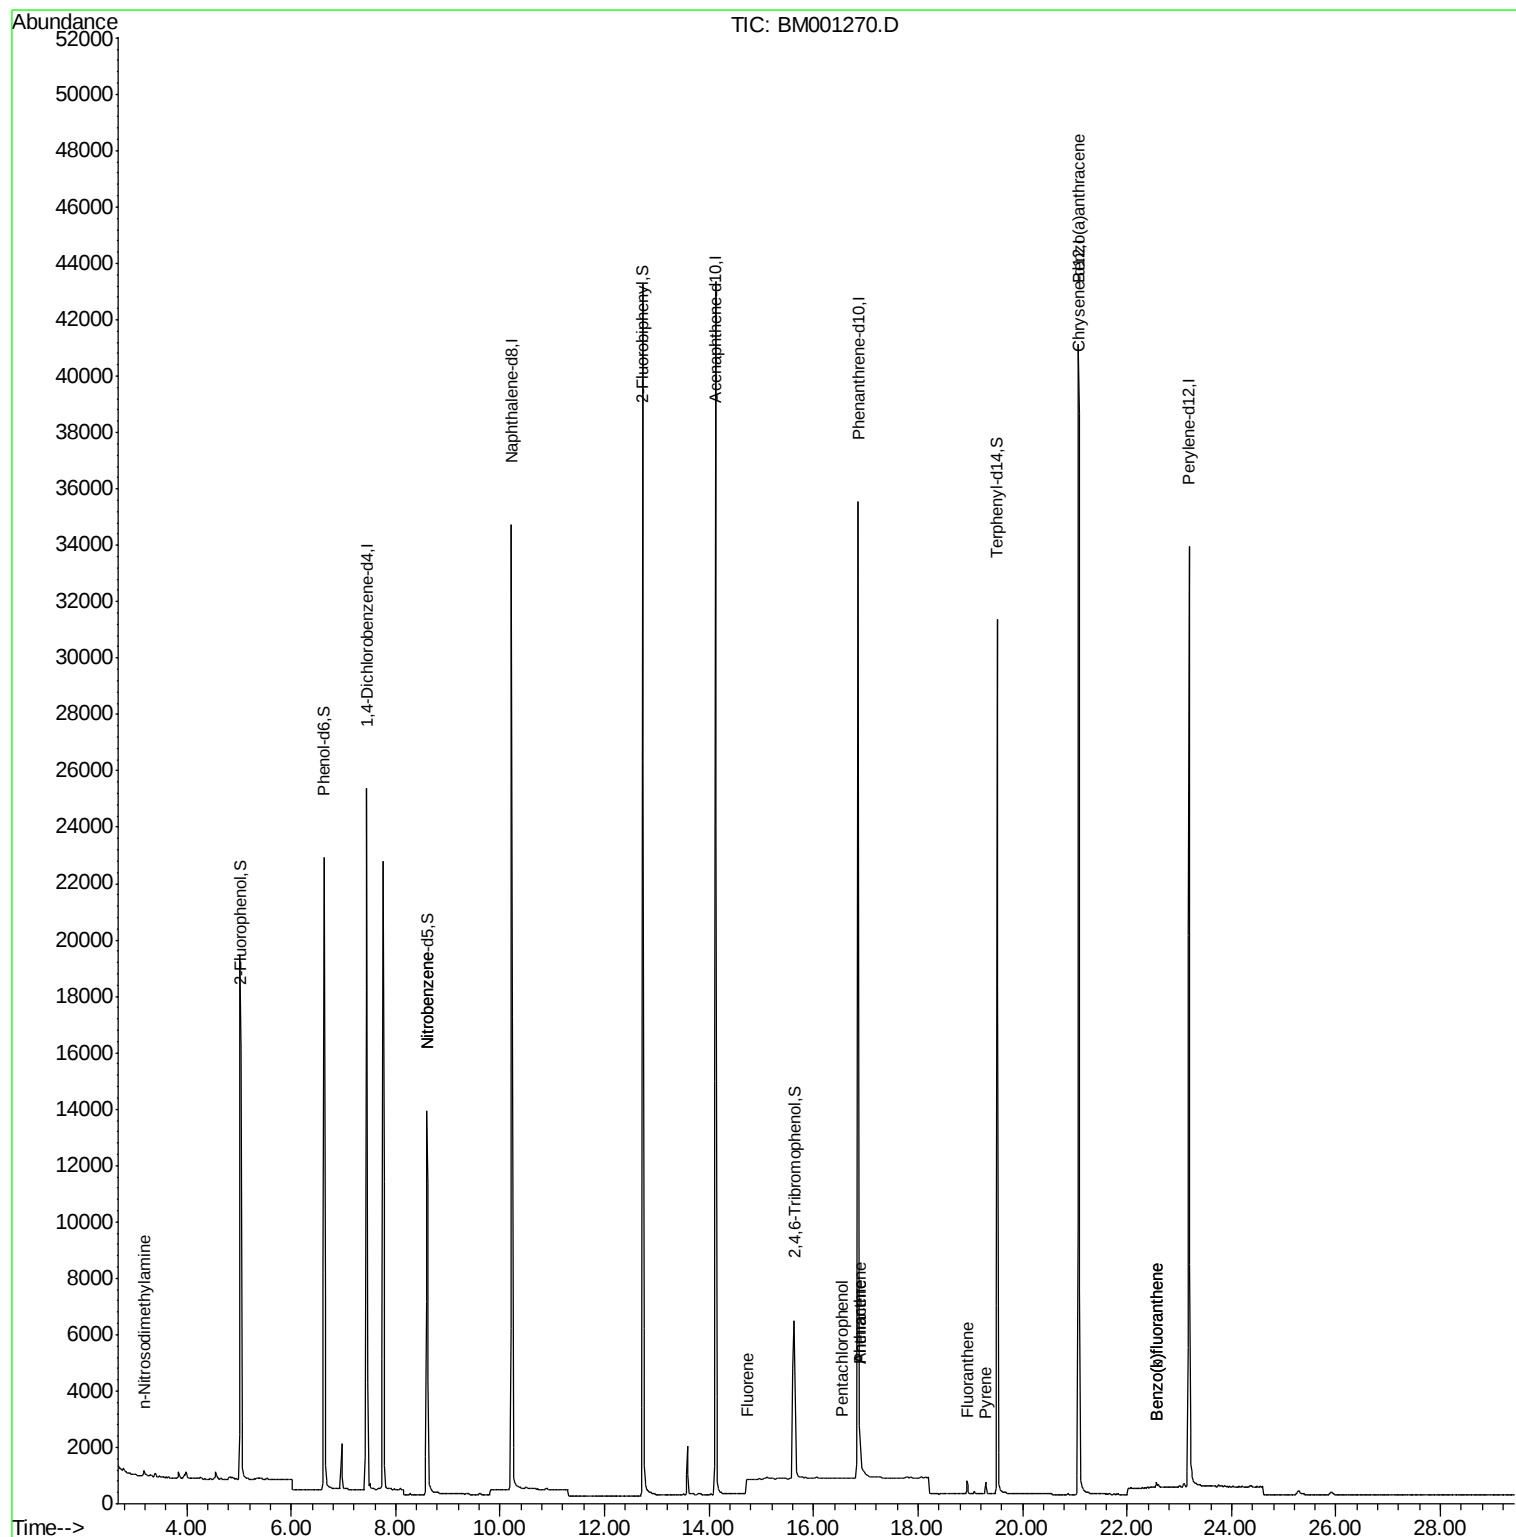



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.45 min Scan# 309

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)





Tgt Ion:152 Resp: 13780

Ion Ratio Lower Upper

152 100

150 142.7 114.6 172.0

115 48.9 39.3 58.9

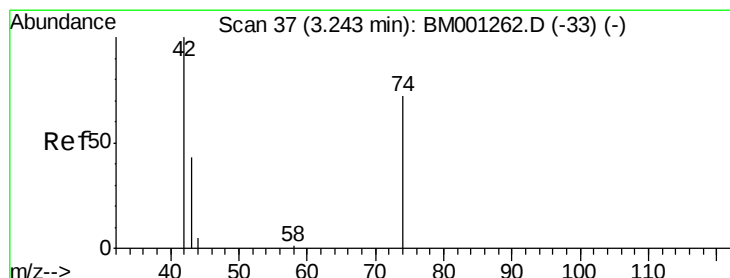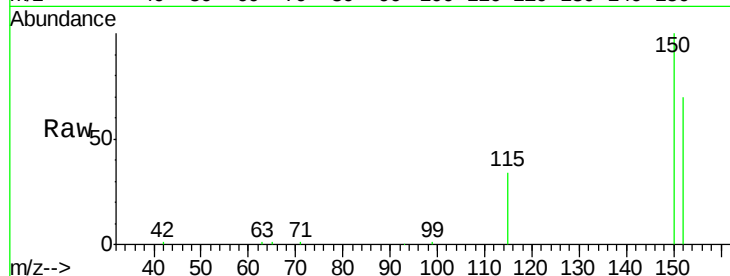

#3

n-Nitrosodimethylamine

Concen: 0.04 ng

RT: 3.18 min Scan# 33

Delta R.T. -0.06 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41



Tgt Ion: 42 Resp: 67


Ion Ratio Lower Upper

42 100

74 0.0 82.1 123.1#

44 256.7 3.0 4.4#

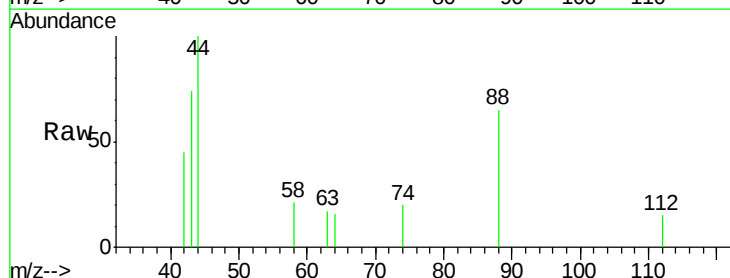

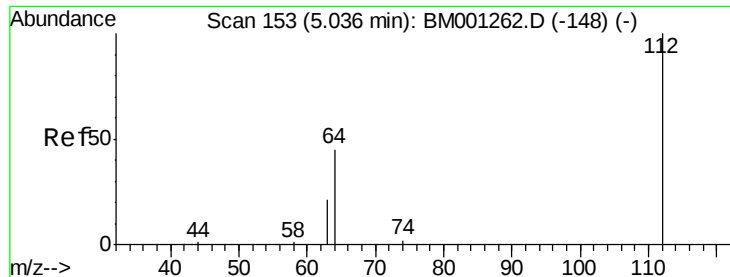

#4

2-Fluorophenol

Concen: 6.48 ng

RT: 5.04 min Scan# 153

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)


Tgt Ion: 112 Resp: 17399

Ion Ratio Lower Upper

112 100

64 64.4 50.8 76.2




63 35.7 28.2 42.4

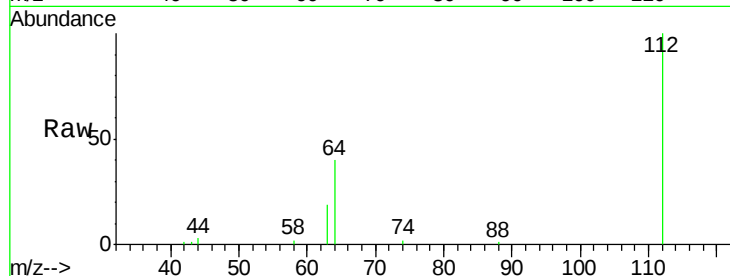

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): B

Ion 63.00 (62.70 to 63.70): B

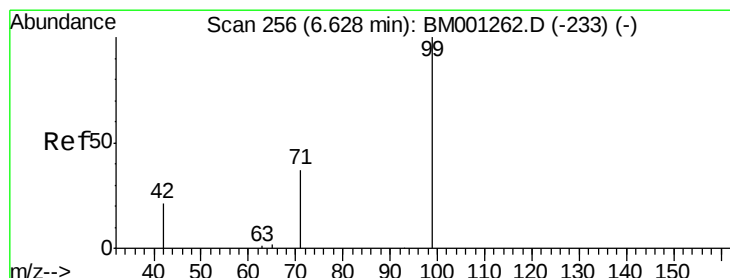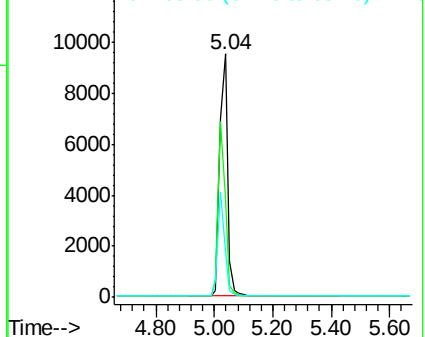

#5

Phenol-d6

Concen: 7.52 ng

RT: 6.63 min Scan# 256

Delta R.T. 0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion: 99 Resp: 22775

Ion Ratio Lower Upper

99 100

42 24.1 19.9 29.9



71 34.8 28.0 42.0

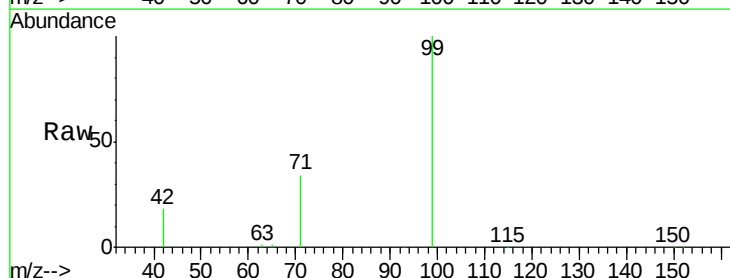


Abundance Ion 99.00 (98.70 to 99.70): B

Ion 42.00 (41.70 to 42.70): B

Ion 71.00 (70.70 to 71.70): B

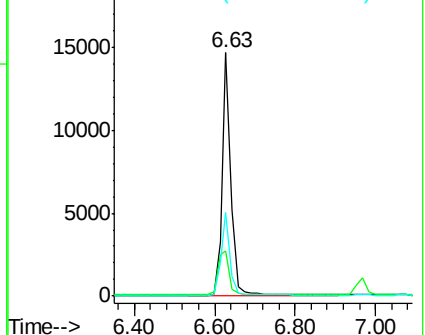

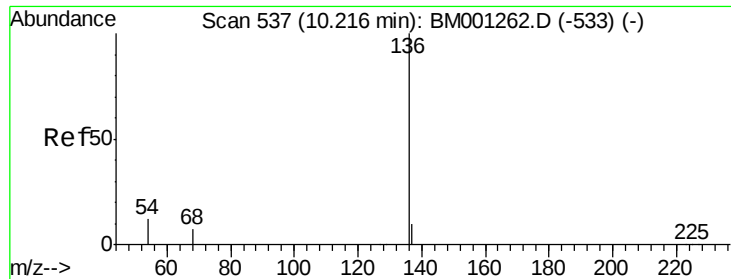

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.22 min Scan# 537

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)

Tgt Ion: 136 Resp: 48105


Ion Ratio Lower Upper

136 100

137 10.3 8.2 12.4

54 11.3 9.5 14.3

68 6.7 5.5 8.3






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BM

Ion 68.00 (67.70 to 68.70): BM

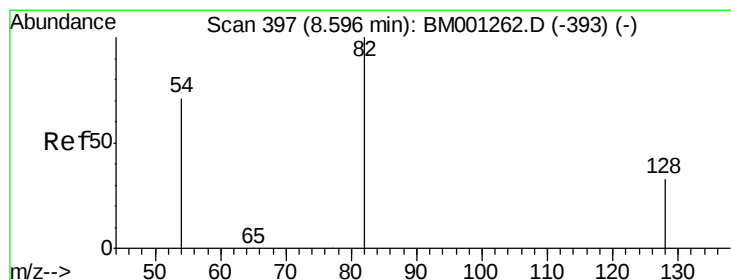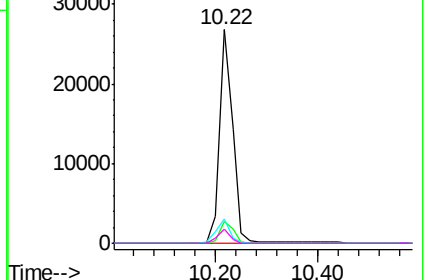

#7

Nitrobenzene-d5

Concen: 4.08 ng

RT: 8.60 min Scan# 397

Delta R.T. 0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion: 82 Resp: 12316

Ion Ratio Lower Upper

82 100

128 34.5 28.0 42.0



54 67.9 57.3 85.9

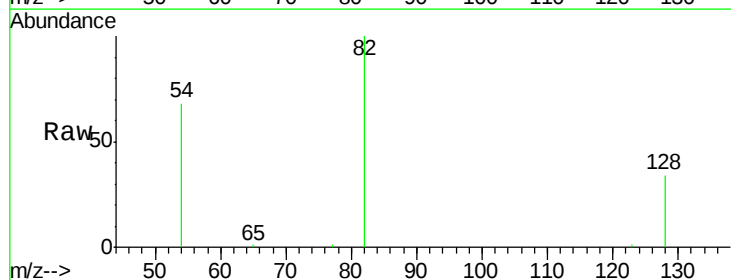


Abundance Ion 82.00 (81.70 to 82.70): BM

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BM

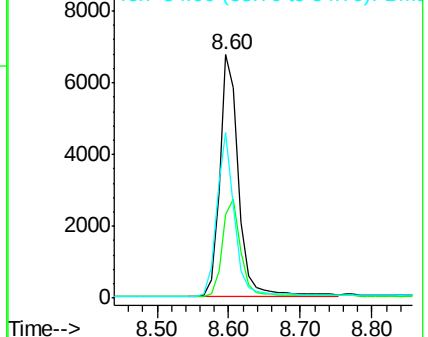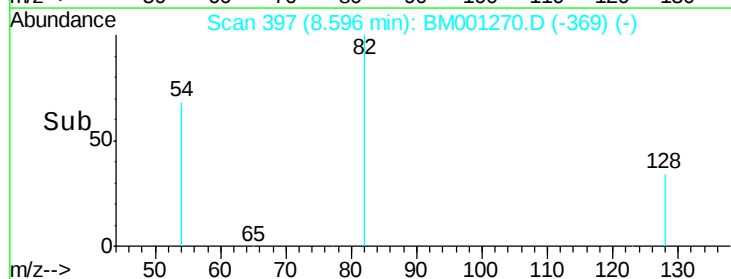

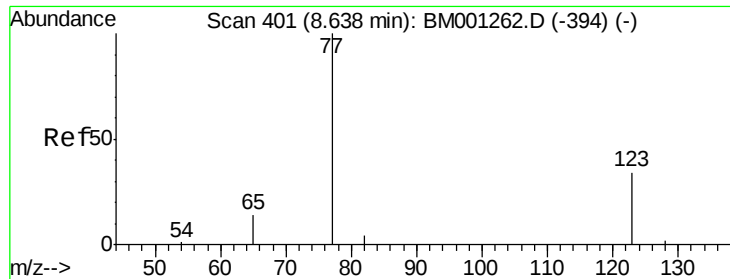

#8

Nitrobenzene

Concen: 0.14 ng

RT: 8.60 min Scan# 397

Delta R.T. -0.04 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampled :

SB-1(7-8)


Tgt Ion: 77 Resp: 44

Ion Ratio Lower Upper

77 100

123 0.0 33.4 50.2#




65 65.9 10.6 15.8#

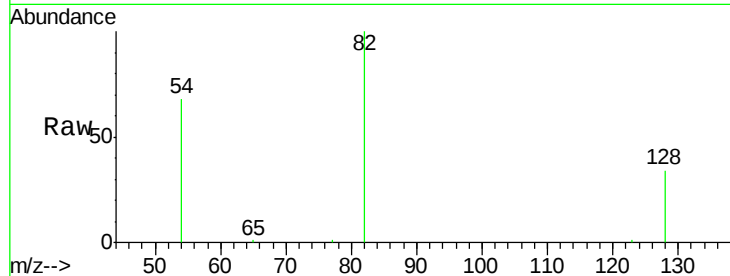

Abundance Ion 77.00 (76.70 to 77.70): BM001262.D (-394) (-)

Ion 123.00 (122.70 to 123.70): BM001262.D (-394) (-)

Ion 65.00 (64.70 to 65.70): BM001262.D (-394) (-)

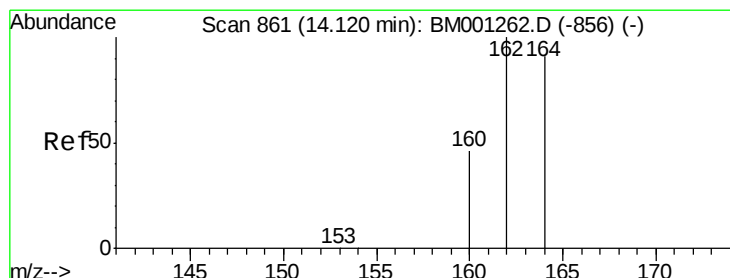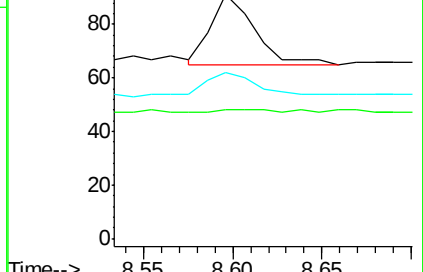

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.12 min Scan# 861

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion: 164 Resp: 24745

Ion Ratio Lower Upper

164 100

162 106.8 87.9 131.9



160 48.8 40.9 61.3

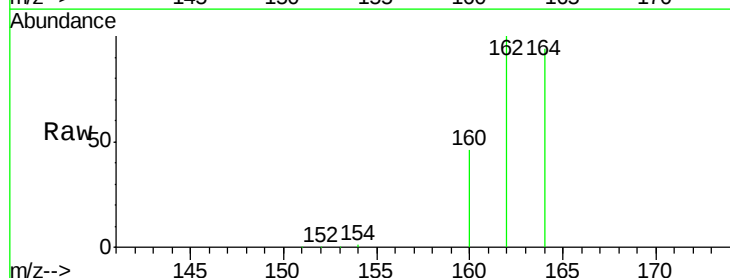


Abundance Ion 164.00 (163.70 to 164.70): BM001262.D (-856) (-)

Ion 162.00 (161.70 to 162.70): BM001262.D (-856) (-)

Ion 160.00 (159.70 to 160.70): BM001262.D (-856) (-)




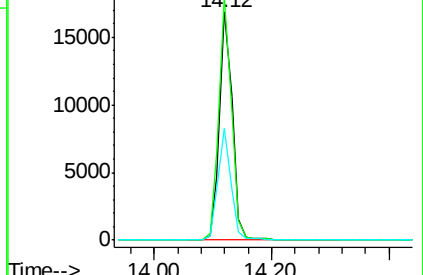


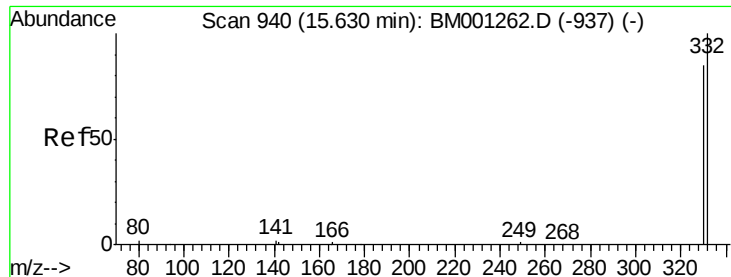

#13
 2,4,6-Tribromophenol
 Concen: 6.76 ng
 RT: 15.63 min Scan# 940
 Delta R.T. 0.00 min
 Lab File: BM001270.D
 Acq: 13 May 2015 02:41




Instrument :
 BNA_M
 ClientSampleId :
 SB-1(7-8)


Tgt Ion:330 Resp: 5720
 Ion Ratio Lower Upper
 330 100
 332 111.0 89.0 133.4
 141 0.0 0.0 0.0

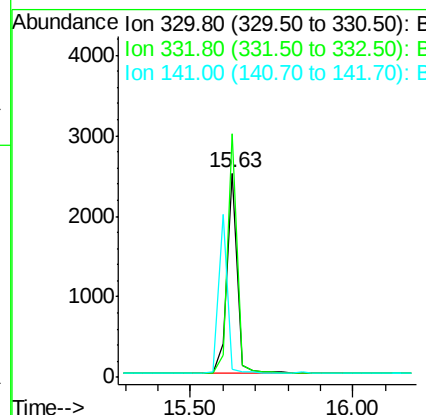

#14
 2-Fluorobiphenyl
 Concen: 5.33 ng
 RT: 12.73 min Scan# 737
 Delta R.T. -0.00 min
 Lab File: BM001270.D
 Acq: 13 May 2015 02:41

Tgt Ion:172 Resp: 40951
 Ion Ratio Lower Upper
 172 100
 171 34.7 28.7 43.1
 170 23.0 19.5 29.3

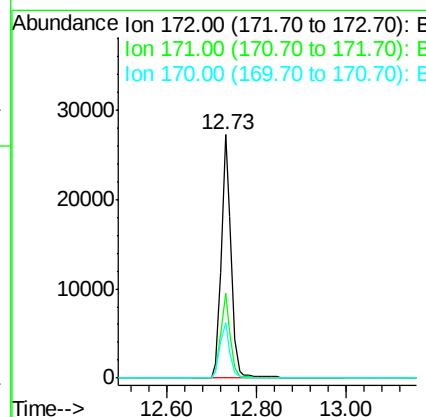

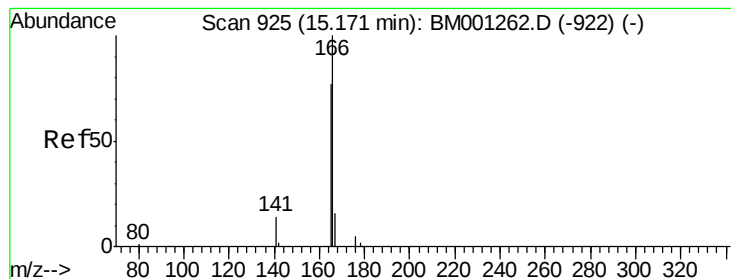

#17

Fluorene

Concen: 0.05 ng

RT: 14.74 min Scan# 911

Delta R.T. -0.43 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)


Tgt Ion:166 Resp: 301

Ion Ratio Lower Upper

166 100

165 257.8 70.6 106.0#




167 0.0 11.3 16.9#



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

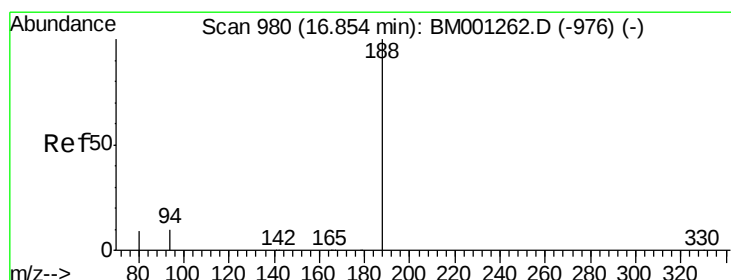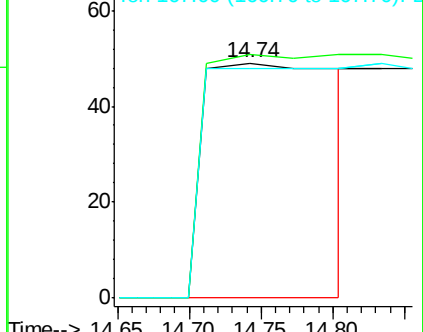

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.85 min Scan# 980

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion:188 Resp: 58970

Ion Ratio Lower Upper

188 100

94 8.4 7.8 11.8



80 7.8 7.5 11.3




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

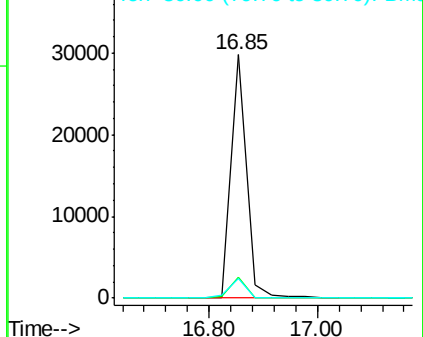

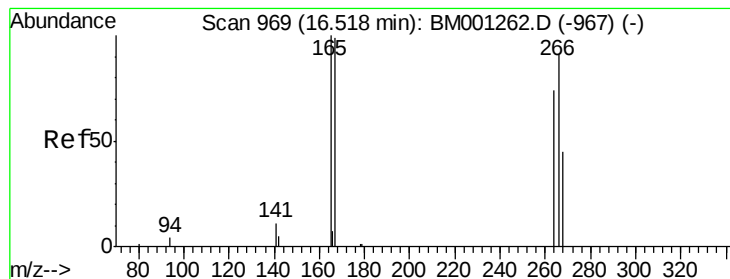

#20

Pentachlorophenol

Concen: 0.43 ng

RT: 16.55 min Scan# 970

Delta R.T. 0.03 min

Lab File: BM001270.D


Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)

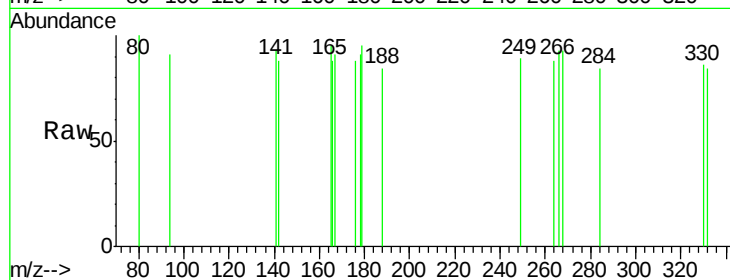




Tgt Ion:266 Resp: 15

Ion Ratio Lower Upper

266 100

268 100.0 49.4 74.0#

264 94.2 67.8 101.6

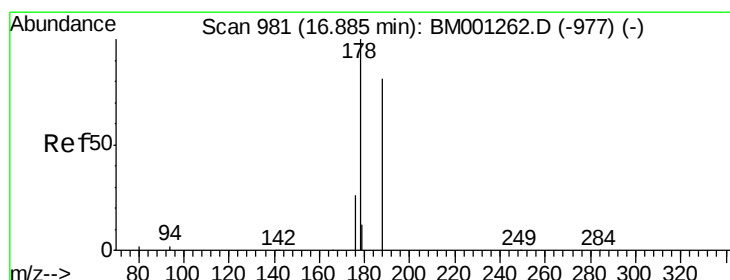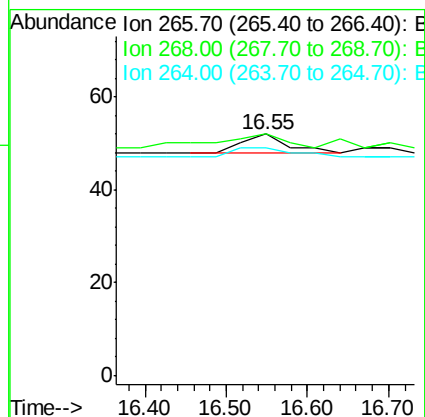

#21

Phenanthrene

Concen: 0.04 ng

RT: 16.88 min Scan# 981

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41




Tgt Ion:178 Resp: 387


Ion Ratio Lower Upper

178 100

176 19.4 15.9 23.9

179 0.0 0.0 0.0

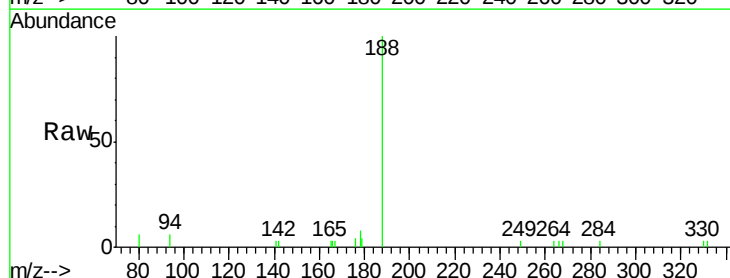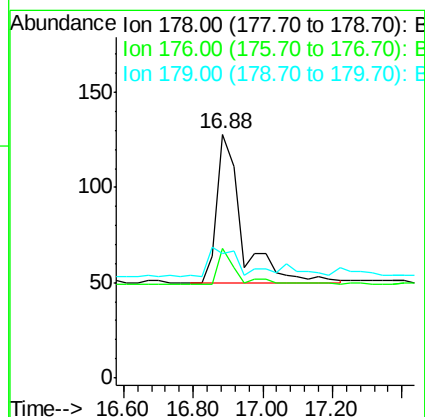



#22

Anthracene

Concen: 0.04 ng

RT: 16.88 min Scan# 981

Delta R.T. -0.09 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)


Tgt Ion:178 Resp: 389

Ion Ratio Lower Upper

178 100

176 19.3 15.3 22.9




179 0.0 0.0 0.0



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

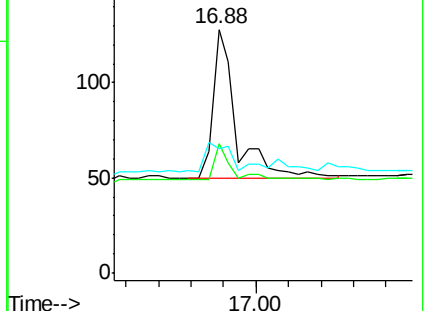

#23

Fluoranthene

Concen: 0.04 ng

RT: 18.93 min Scan# 1083

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion:202 Resp: 514

Ion Ratio Lower Upper

202 100

101 14.2 9.1 13.7#



203 17.5 13.8 20.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

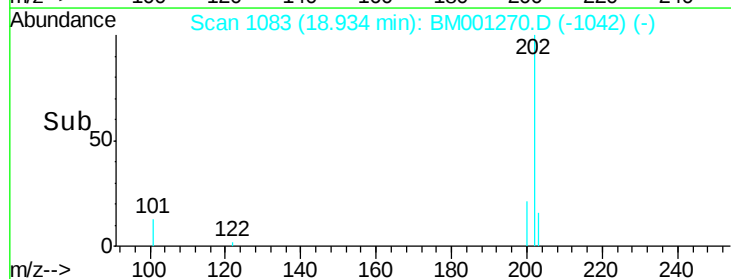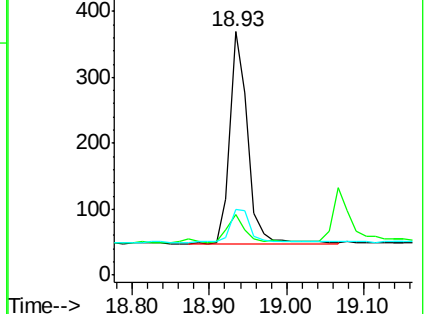



#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.08 min Scan# 1267

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)


Tgt Ion:240 Resp: 43738

Ion Ratio Lower Upper

240 100

120 5.0 5.5 8.3#




236 24.2 20.4 30.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

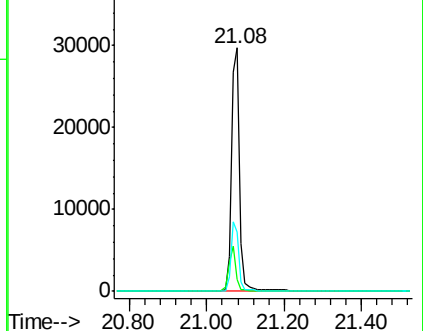

#25

Pyrene

Concen: 0.03 ng

RT: 19.30 min Scan# 1113

Delta R.T. -0.00 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41


Tgt Ion:202 Resp: 452

Ion Ratio Lower Upper

202 100

200 20.6 16.4 24.6



203 20.6 13.9 20.9




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

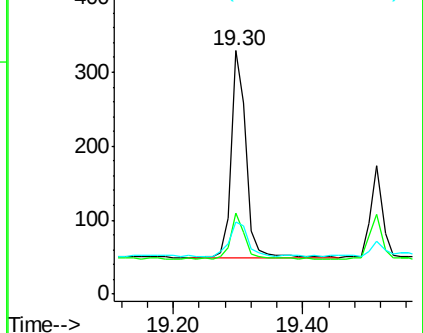



#26

Terphenyl-d14

Concen: 5.59 ng

RT: 19.51 min Scan# 1131

Delta R.T. -0.01 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)





Tgt Ion:244 Resp: 32856

Ion Ratio Lower Upper

244 100

212 10.6 7.2 10.8

122 19.9 5.6 8.4#

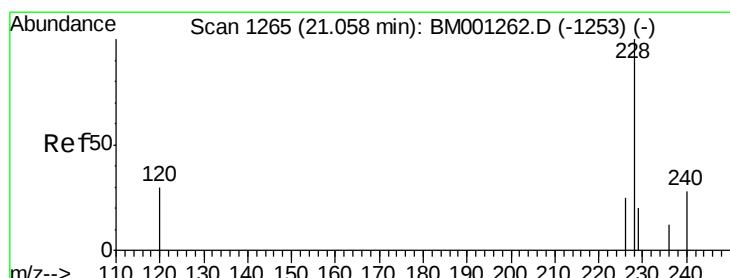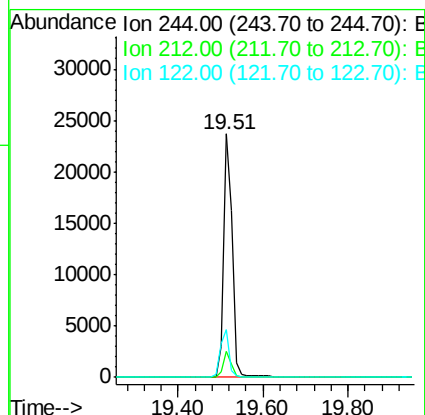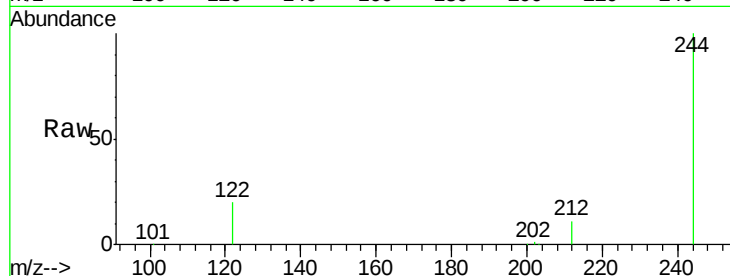

#27

Benzo(a)anthracene

Concen: 0.03 ng

RT: 21.07 min Scan# 1266

Delta R.T. 0.01 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41




Tgt Ion:228 Resp: 365


Ion Ratio Lower Upper

228 100

226 34.0 20.5 30.7#

229 42.4 16.2 24.4#


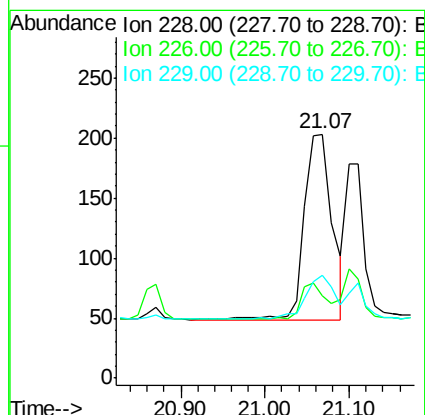
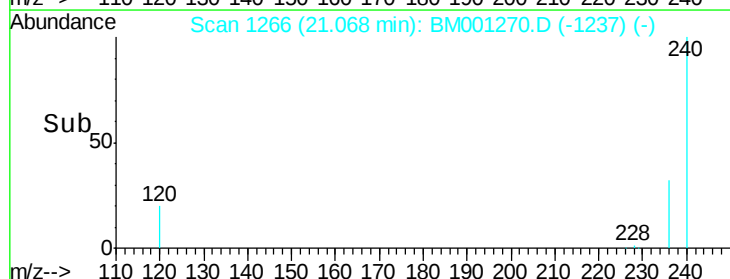
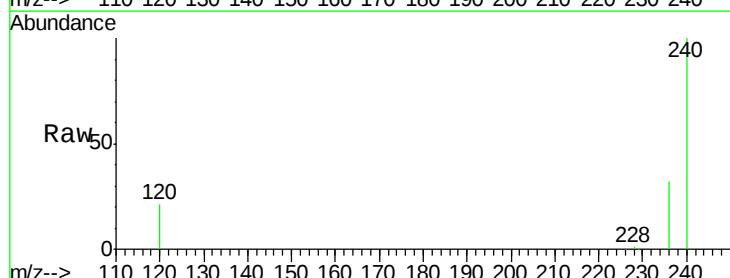


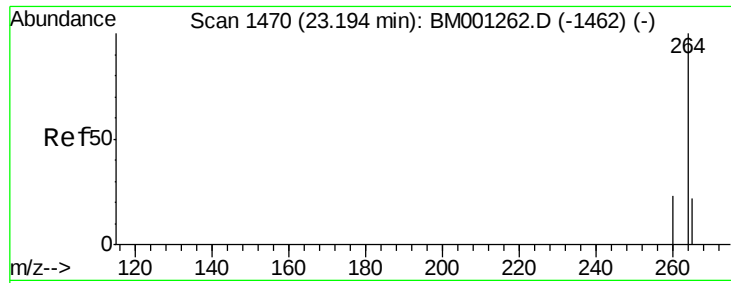

#30
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.18 min Scan# 1469
 Delta R.T. -0.01 min
 Lab File: BM001270.D
 Acq: 13 May 2015 02:41




Instrument :
 BNA_M
 ClientSampleId :
 SB-1(7-8)




Tgt Ion: 264 Resp: 40771
 Ion Ratio Lower Upper
 264 100
 260 25.6 18.9 28.3
 265 21.3 18.1 27.1

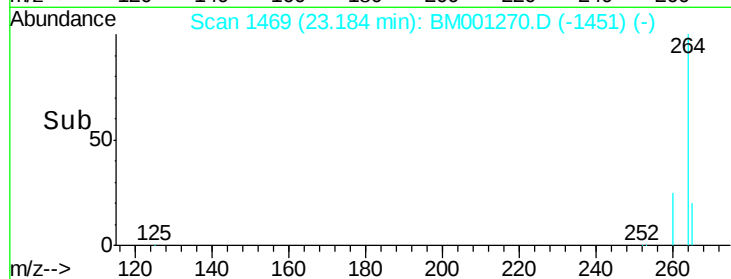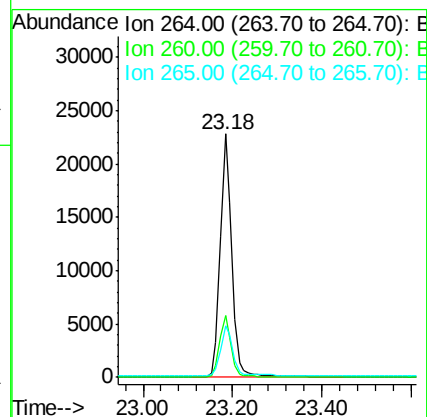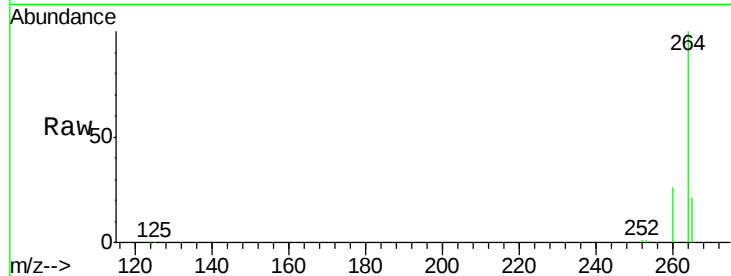

#31
 Benzo(b)fluoranthene
 Concen: 0.03 ng
 RT: 22.56 min Scan# 1409
 Delta R.T. -0.00 min
 Lab File: BM001270.D
 Acq: 13 May 2015 02:41

Tgt Ion: 252 Resp: 408
 Ion Ratio Lower Upper
 252 100
 253 83.8 17.8 26.6#
 125 58.1 10.4 15.6#

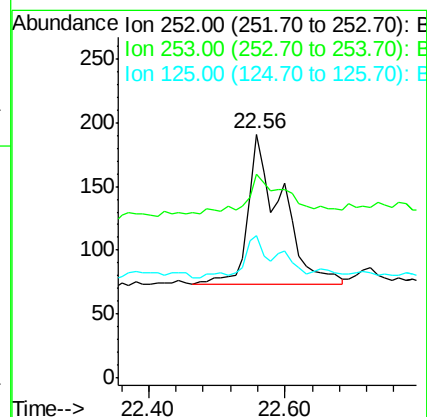

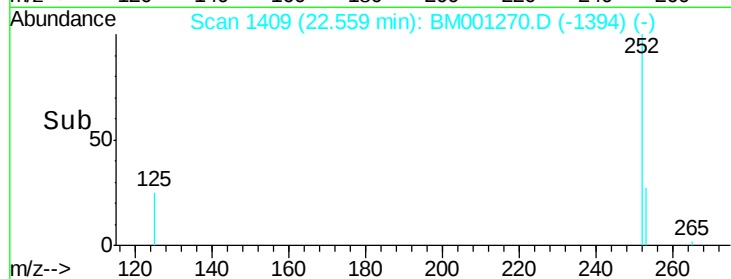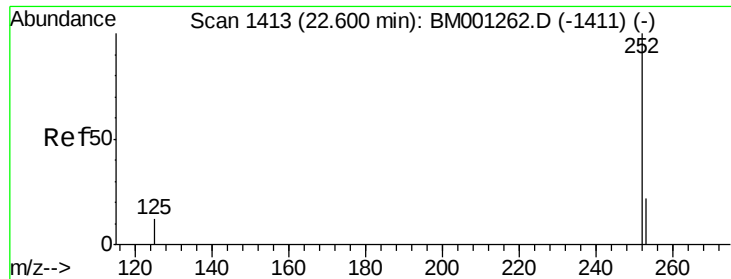

#32

Benzo(k)fluoranthene

Concen: 0.04 ng

RT: 22.56 min Scan# 1409

Delta R.T. -0.04 min

Lab File: BM001270.D

Acq: 13 May 2015 02:41

Instrument :

BNA_M

ClientSampleId :

SB-1(7-8)

Tgt Ion: 252 Resp: 408

Ion Ratio Lower Upper

252 100

253 83.8 18.6 27.8#

125 58.1 10.2 15.4#

