


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051315\
 Data File : BM001258.D
 Acq On : 12 May 2015 19:30
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

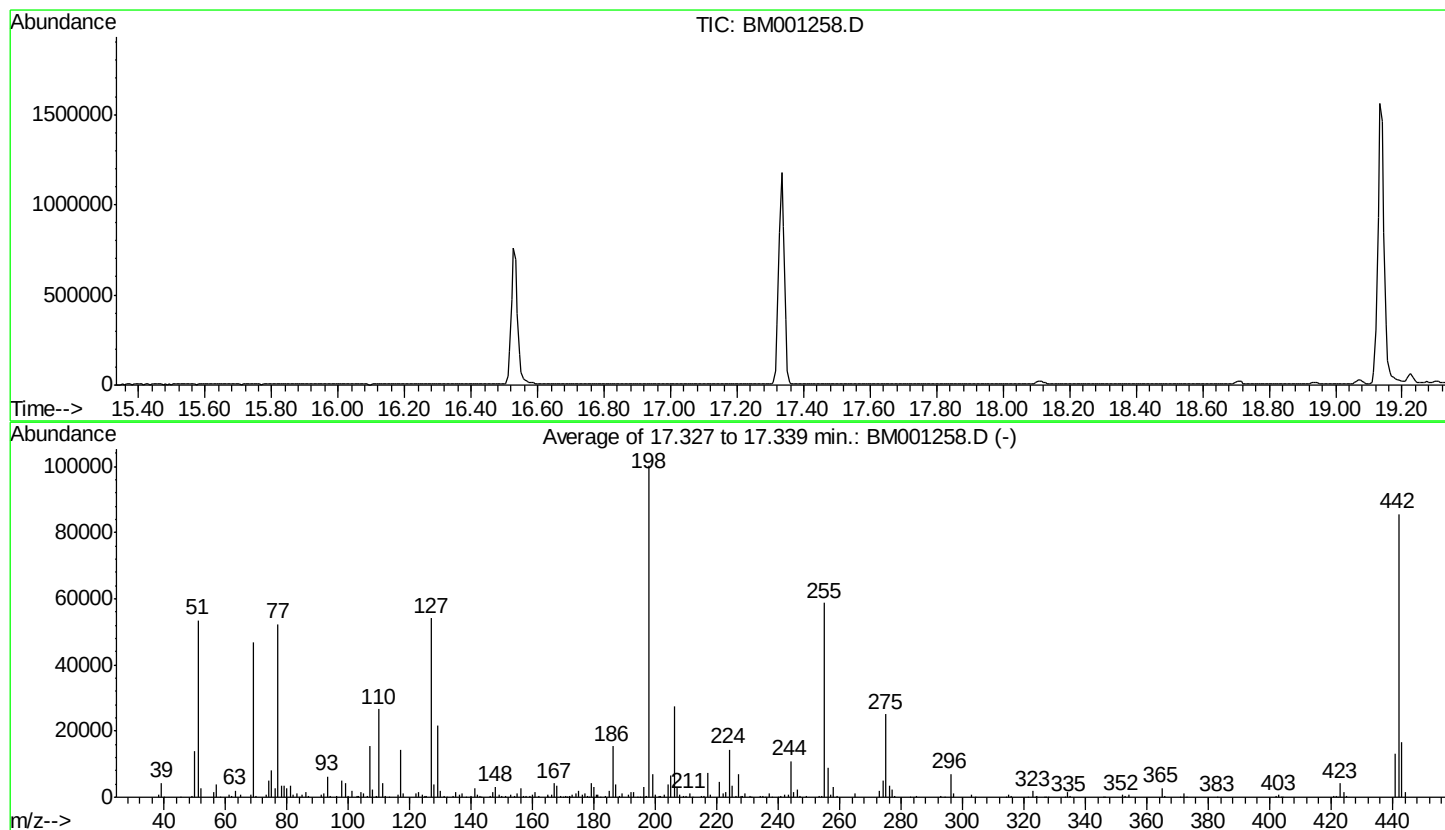

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	53560	PASS
68	69	0.00	2	2.0	956	PASS
69	198	0.00	100	46.8	46925	PASS
70	69	0.00	2	0.5	241	PASS
127	198	10	80	54.0	54218	PASS
197	198	0.00	2	0.5	491	PASS
198	198	100	100	100.0	100322	PASS
199	198	5	9	7.0	6999	PASS
275	198	10	60	25.1	25152	PASS
365	198	1	100	2.9	2865	PASS
441	442	0.01	24	15.6	13357	PASS
442	198	50	100	85.3	85610	PASS
443	442	15	24	19.5	16728	PASS