

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051316\
 Data File : BM005434.D
 Acq On : 13 May 2016 16:02
 Operator : UM/SJ
 Sample : H2874-24
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H4097

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.928	717	721	730	rBV	67440	113434	4.07%	0.457%
2	7.087	741	748	761	rBV	290706	459572	16.48%	1.852%
3	7.287	775	782	795	rBV	295161	478613	17.16%	1.928%
4	7.751	854	861	874	rVB	304159	498138	17.86%	2.007%
5	8.463	976	982	993	rBV	219952	378143	13.56%	1.524%
6	8.910	1051	1058	1072	rBV	368645	632256	22.67%	2.548%
7	9.628	1173	1180	1190	rBV	324779	550995	19.75%	2.220%
8	10.163	1265	1271	1286	rBV	419246	744039	26.67%	2.998%
9	10.534	1327	1334	1345	rBV	465875	804731	28.85%	3.242%
10	10.686	1354	1360	1369	rBV	18228	33317	1.19%	0.134%
11	13.804	1884	1890	1897	rBV	983171	1366601	48.99%	5.506%
12	14.086	1931	1938	1948	rBV	1037163	1591321	57.05%	6.412%
13	14.239	1958	1964	1978	rBV	27844	67544	2.42%	0.272%
14	14.392	1984	1990	1999	rVB2	775835	1178419	42.25%	4.748%
15	14.633	2026	2031	2044	rBV	38444	99499	3.57%	0.401%
16	15.392	2152	2160	2169	rBV	1333007	2045740	73.34%	8.243%
17	15.521	2176	2182	2196	rBV	474994	682586	24.47%	2.750%
18	17.145	2451	2458	2468	rBV2	1039987	1514216	54.28%	6.101%
19	17.245	2468	2475	2489	rVV2	1479233	2285622	81.94%	9.209%
20	19.545	2859	2866	2879	rBV2	1933867	2789486	100.00%	11.240%
21	21.339	3165	3171	3181	rBV	1527701	2002933	71.80%	8.070%
22	22.886	3430	3434	3440	rVB3	19628	30048	1.08%	0.121%
23	23.468	3524	3533	3541	rBV2	1315219	2624395	94.08%	10.574%
24	23.609	3549	3557	3571	rVB2	908455	1796797	64.41%	7.240%
25	24.097	3637	3640	3651	rVB	26566	50040	1.79%	0.202%


Sum of corrected areas: 24818485

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051316\
Data File : BM005434.D
Acq On : 13 May 2016 16:02
Operator : UM/SJ
Sample : H2874-24
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4097

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

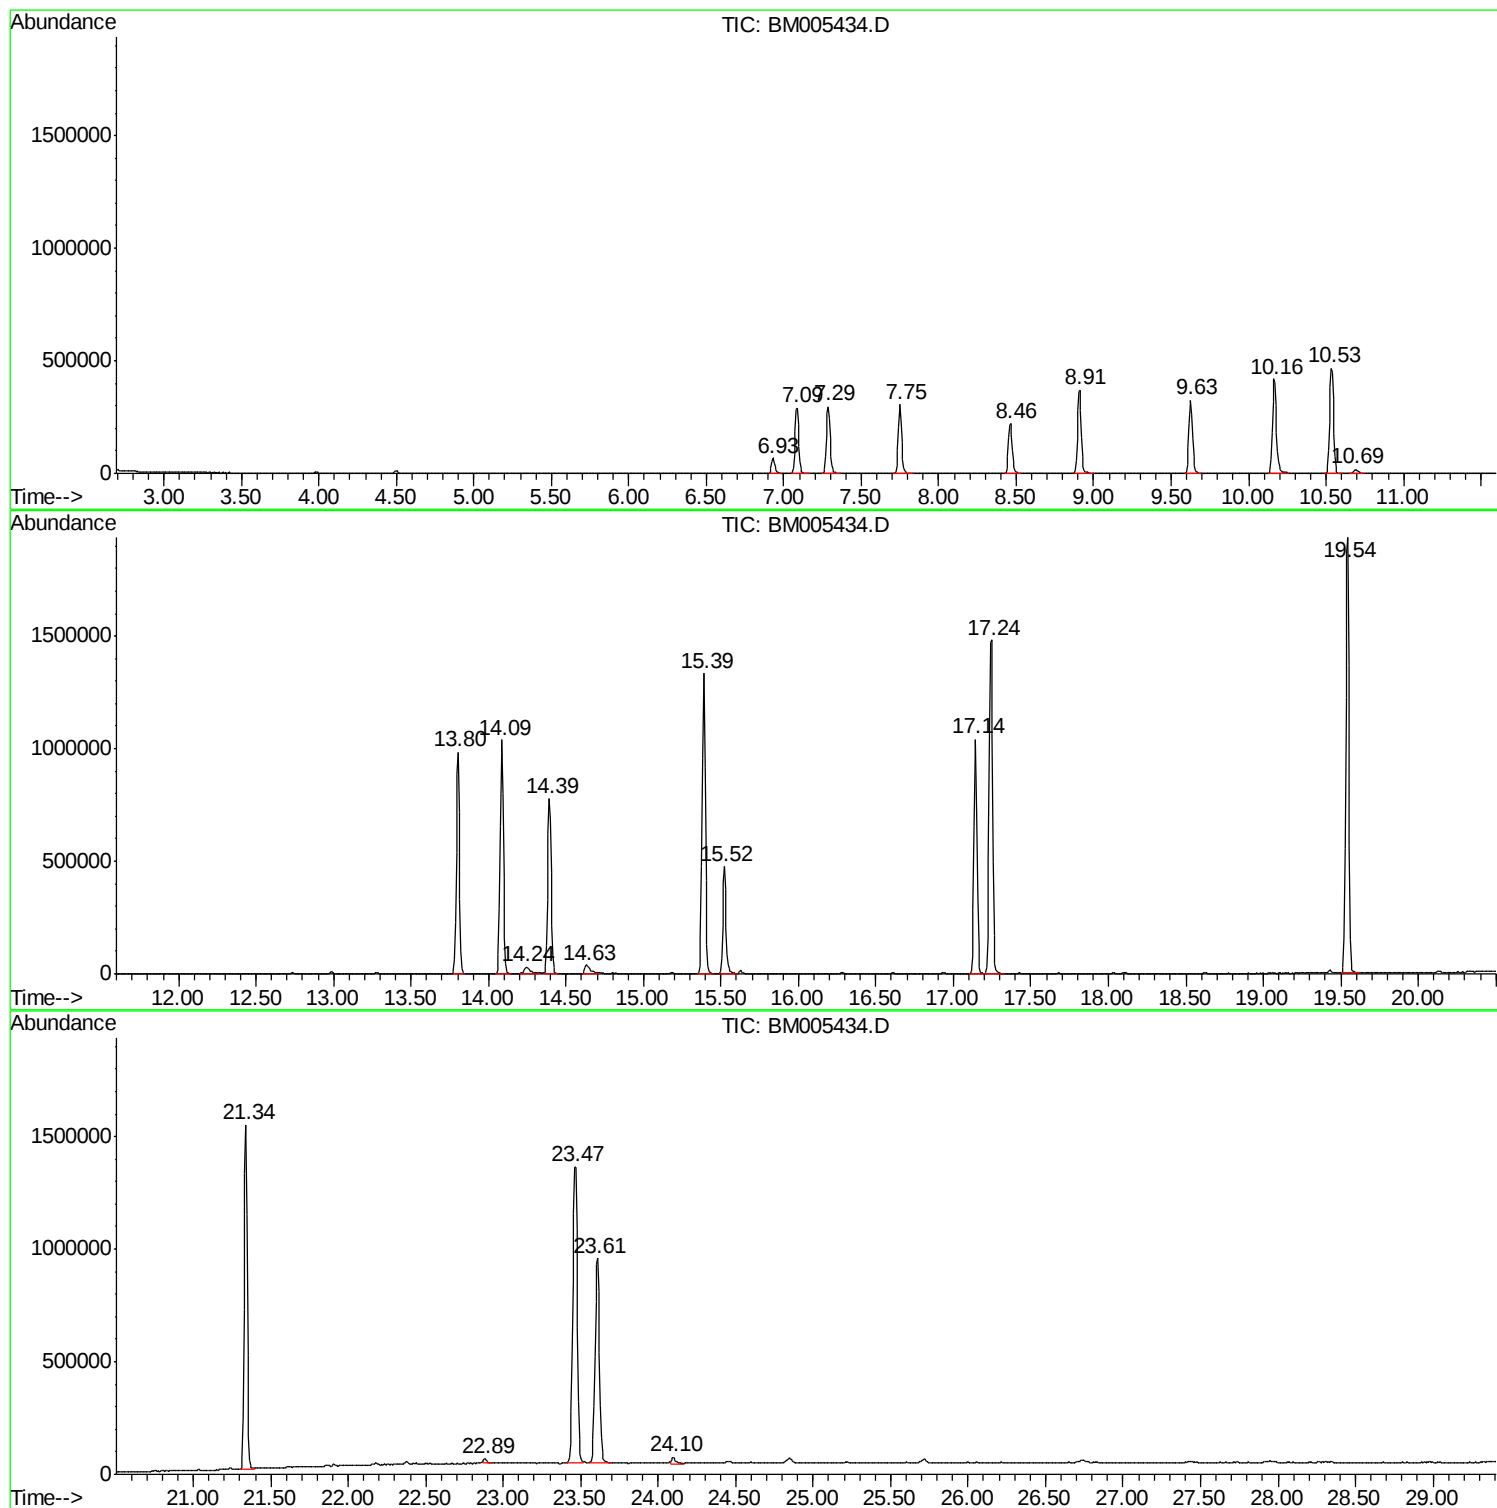

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051316\
Data File : BM005434.D
Acq On : 13 May 2016 16:02
Operator : UM/SJ
Sample : H2874-24
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4097

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051316\
Data File : BM005434.D
Acq On : 13 May 2016 16:02
Operator : UM/SJ
Sample : H2874-24
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H4097

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM050516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc